
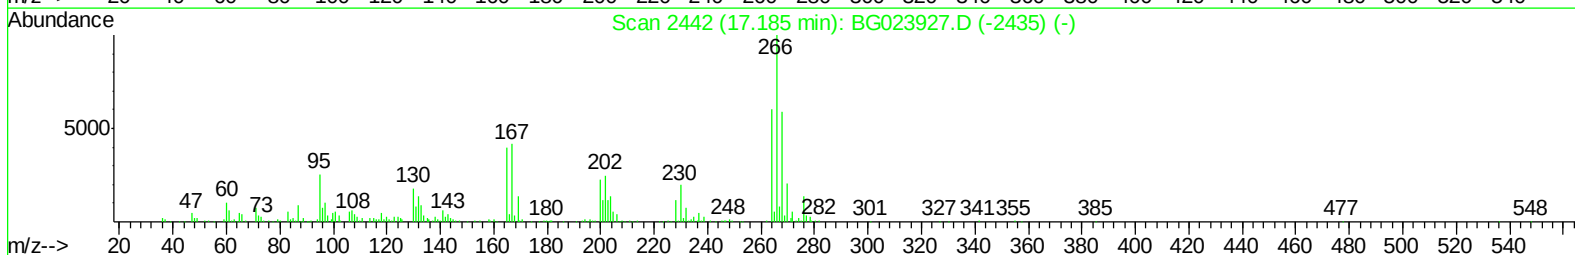
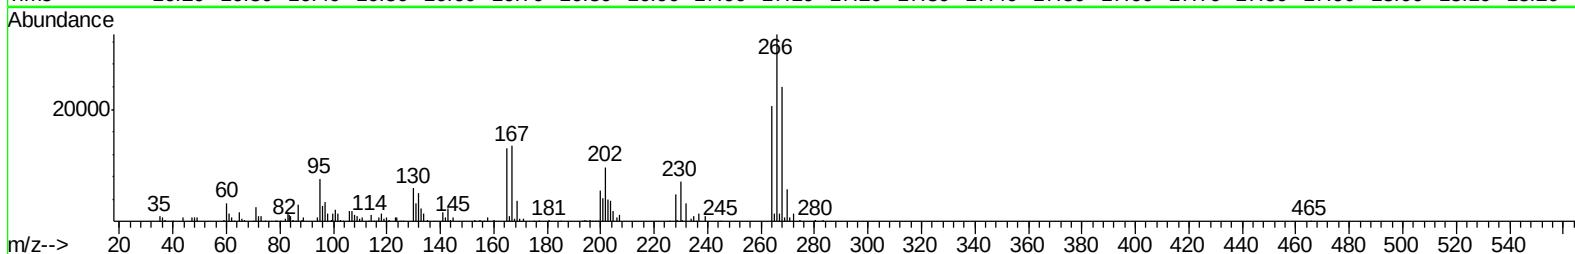


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG091916\
Data File : BG024019.D
Acq On : 19 Sep 2016 15:41
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 03:30:20 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 01:00:00 2016
Response via : Initial Calibration

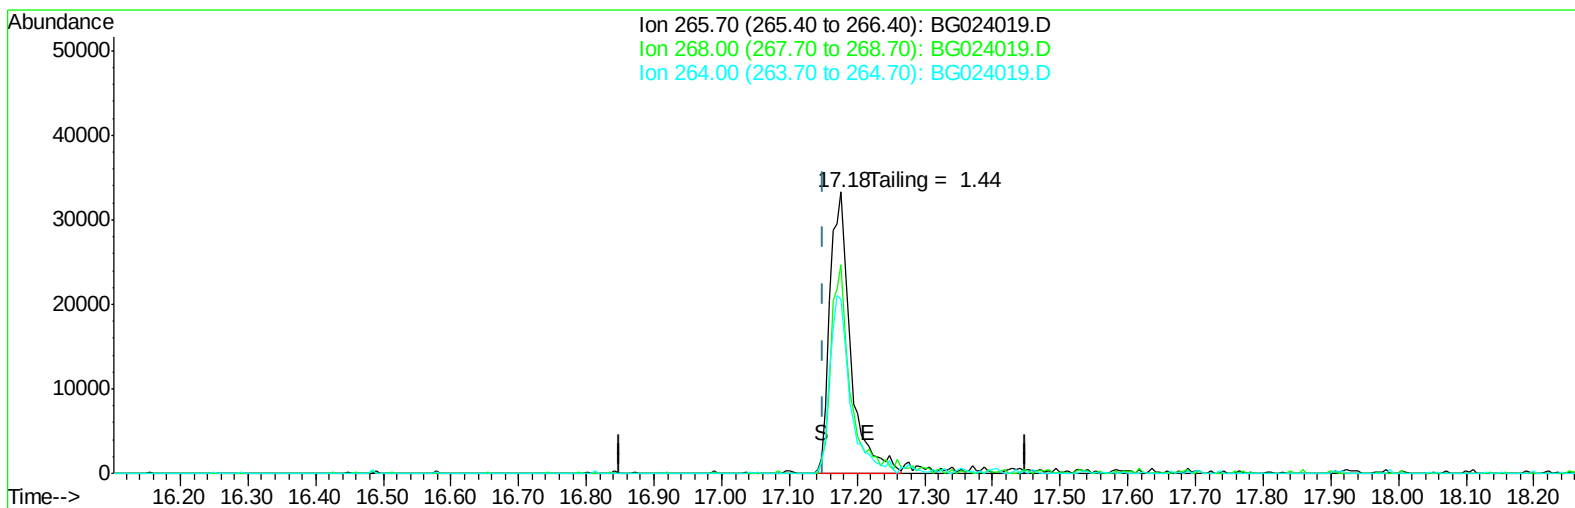

TIC: BG024019.D

(69) Pentachlorophenol (C)




17.177min (+0.027) 171612.06ng

response 70230

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	74.11
264.00	63.20	61.65
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG091916\
Data File : BG024019.D
Acq On : 19 Sep 2016 15:41
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 03:30:20 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 01:00:00 2016
Response via : Initial Calibration

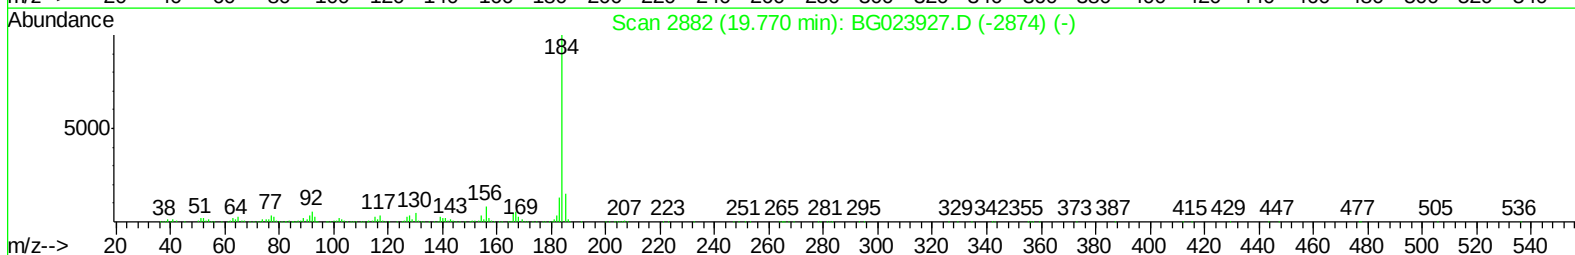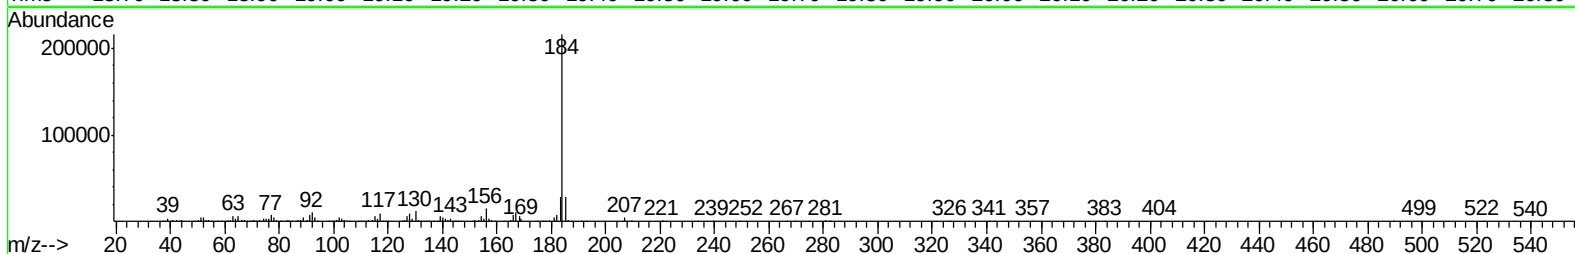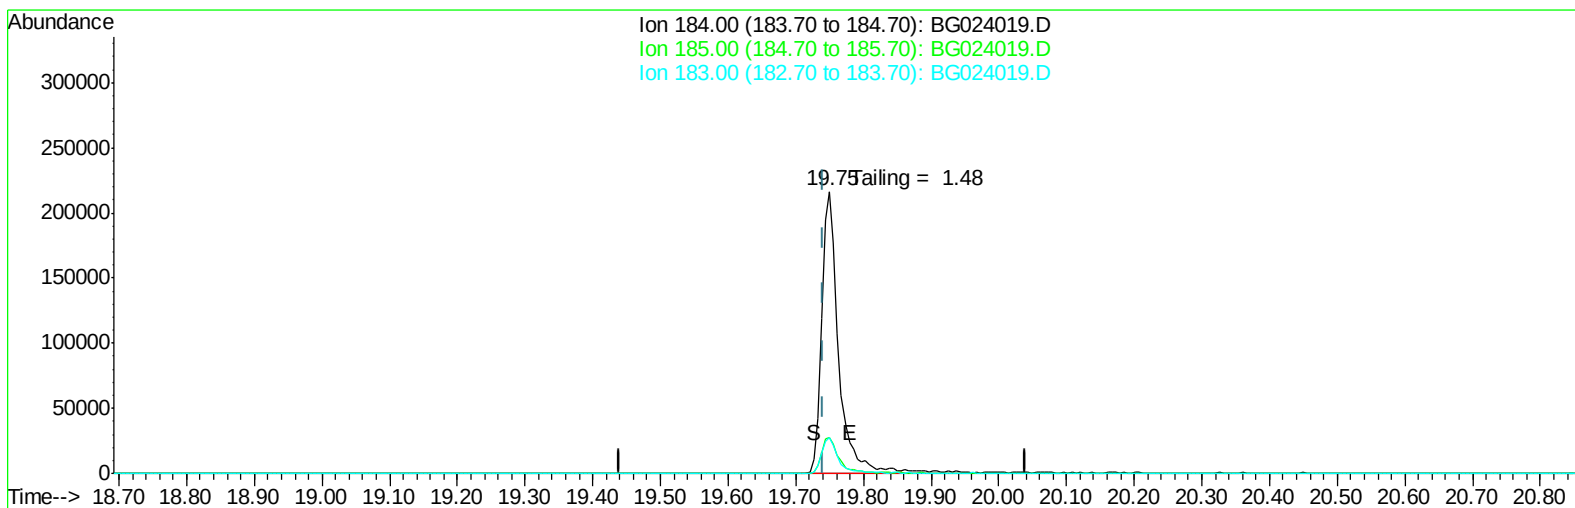

TIC: BG024019.D

(76) Benzidine

19.750min (+0.010) 7131.31ng

response 376951

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	12.78
183.00	13.40	12.85
0.00	0.00	0.00