


Data Path : Z:\HPCHEM1\BNA G\DATA\BG091916\
 Data File : BG024019.D
 Acq On : 19 Sep 2016 15:41
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG083116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 09 16:24:09 2016

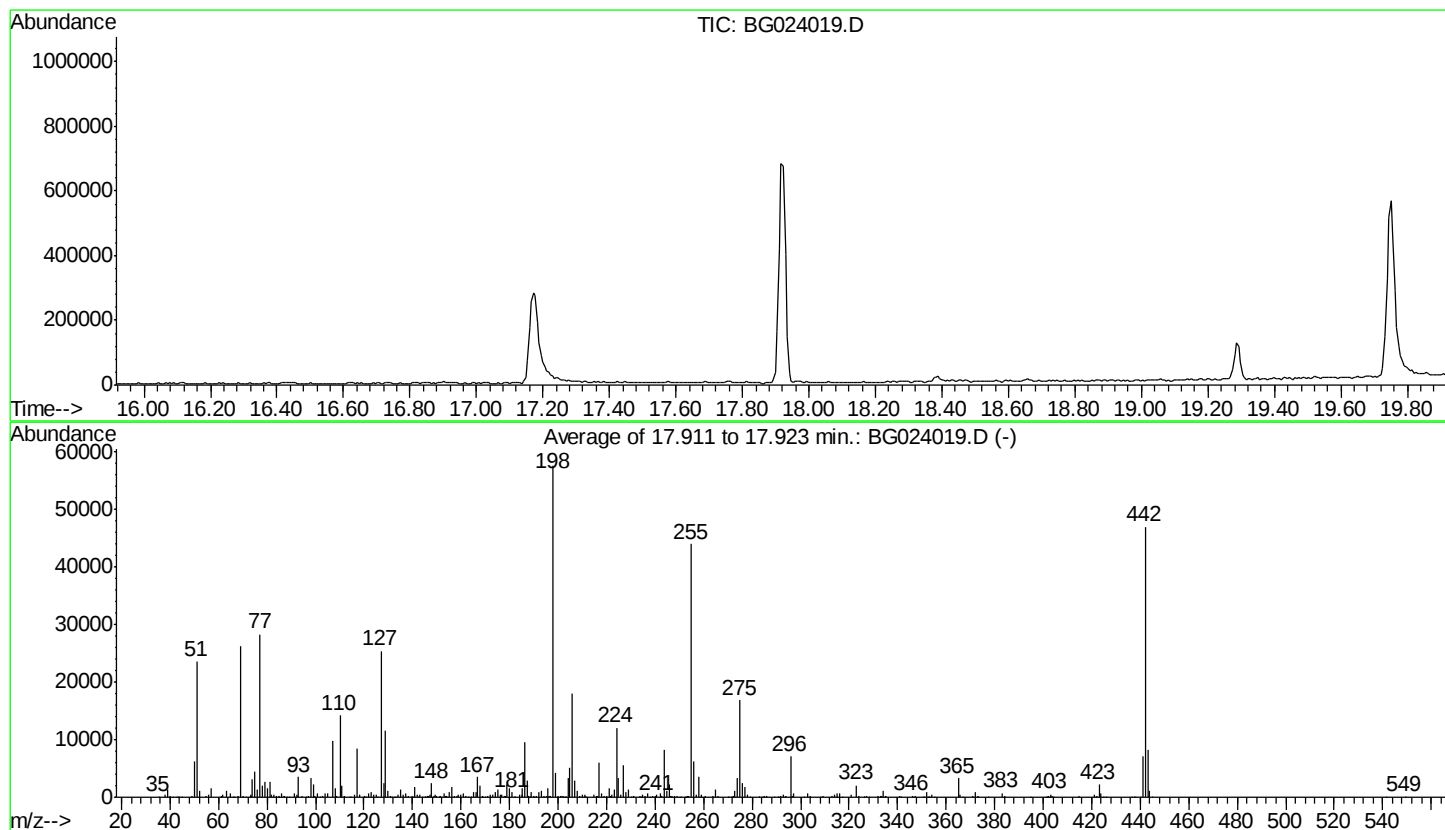

AutoFind: Scans 2566, 2567, 2568; Background Corrected with Scan 2560

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.9	23584	PASS
68	69	0.00	2	0.7	187	PASS
69	198	0.00	100	45.7	26320	PASS
70	69	0.00	2	0.8	213	PASS
127	198	10	80	44.2	25456	PASS
197	198	0.00	2	0.3	151	PASS
198	198	100	100	100.0	57650	PASS
199	198	5	9	7.4	4293	PASS
275	198	10	60	29.2	16810	PASS
365	198	1	100	5.8	3337	PASS
441	442	0.01	24	15.0	7052	PASS
442	198	50	100	81.6	47032	PASS
443	442	15	24	17.5	8240	PASS