
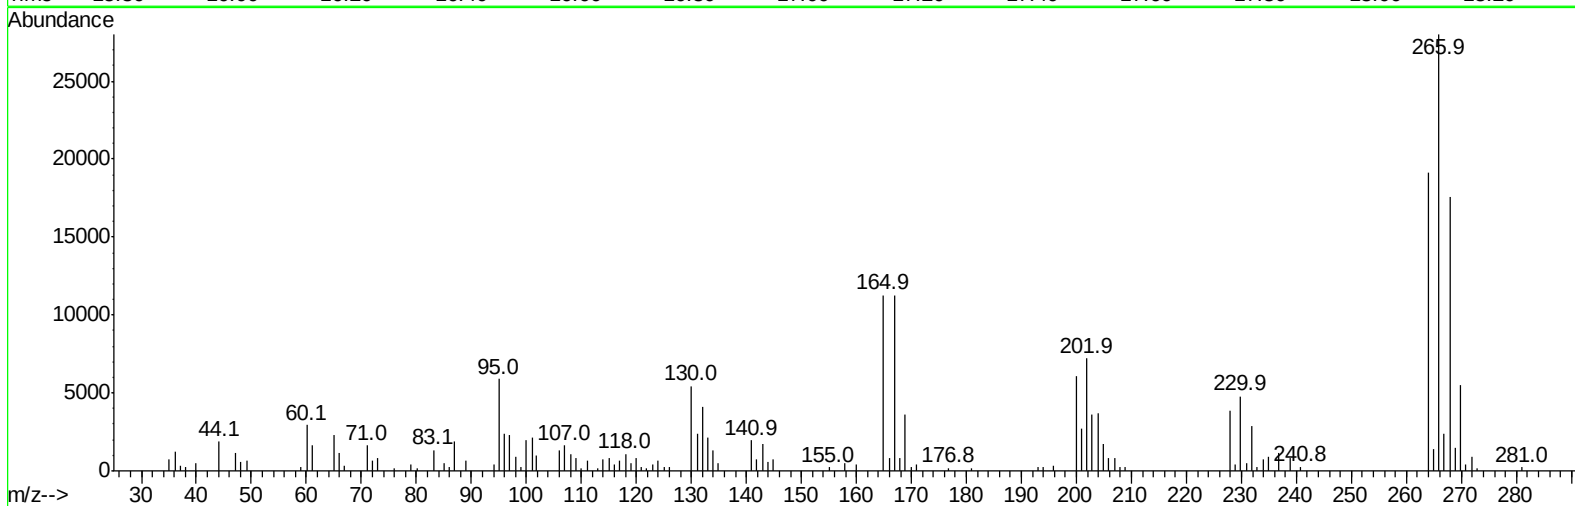


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091918\
Data File : BG036823.D
Acq On : 19 Sep 2018 17:22
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 07:46:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 31 13:03:20 2018
Response via : Initial Calibration

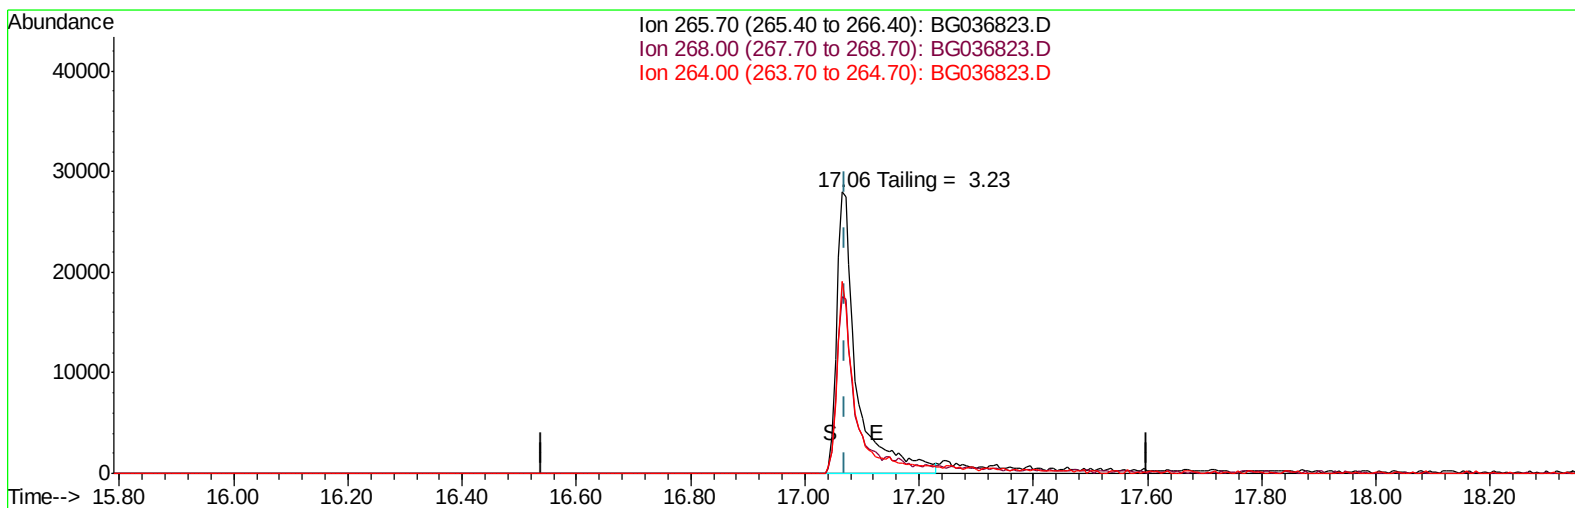

TIC: BG036823.D

(69) Pentachlorophenol (C)



17.065min (-0.006) 7104.16ng

response 65664

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	62.89
264.00	61.10	68.31
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091918\
 Data File : BG036823.D
 Acq On : 19 Sep 2018 17:22
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 07:46:07 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 31 13:03:20 2018
 Response via : Initial Calibration

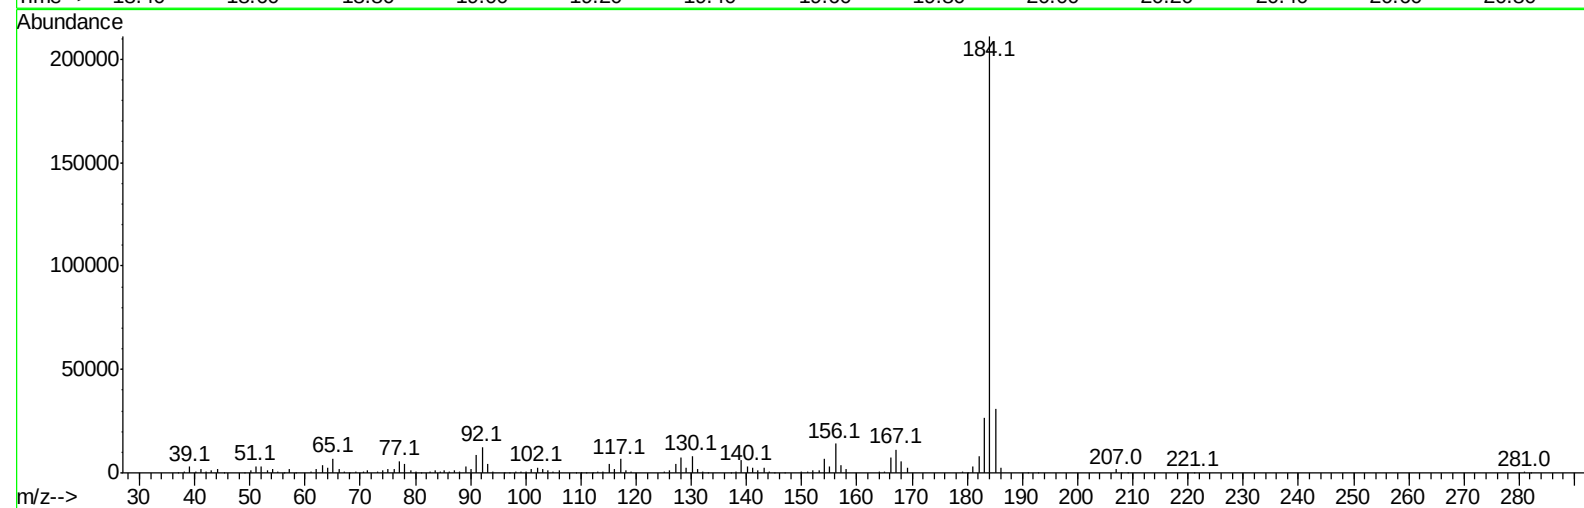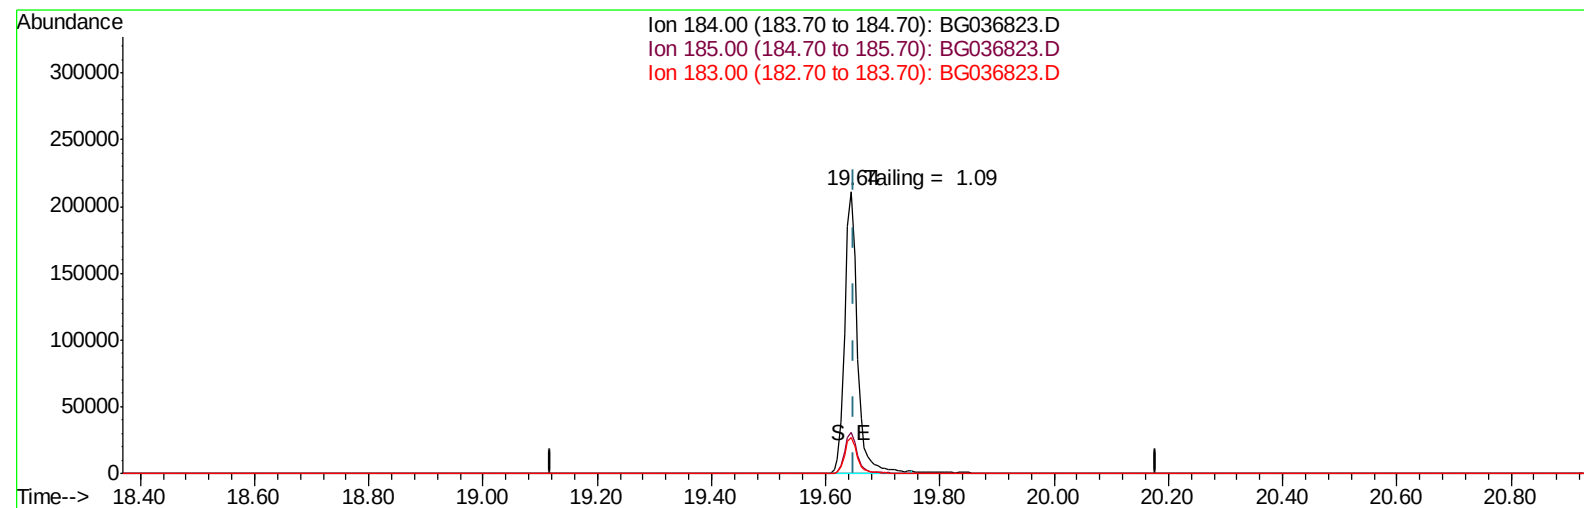

TIC: BG036823.D

(76) Benzidine

19.644min (-0.006) 10439.75ng

response 325747

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.68
183.00	13.60	12.59
0.00	0.00	0.00