

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091918\
 Data File : BG036835.D
 Acq On : 20 Sep 2018 1:11
 Operator : JU/SJ
 Sample : PB113024BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB113024BL

Quant Time: Sep 20 07:37:05 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 31 13:03:20 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	51824	20.00	ng	-0.02
21) Naphthalene-d8	10.85	136	212181	20.00	ng	-0.02
38) Acenaphthene-d10	14.67	164	141403	20.00	ng	-0.02
63) Phenanthrene-d10	17.41	188	362293	20.00	ng	-0.02
75) Chrysene-d12	21.68	240	369489	20.00	ng	-0.02
86) Perylene-d12	24.88	264	350084	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.62	112	386746	118.38	ng	0.00
7) Phenol-d6	7.21	99	542570	116.00	ng	-0.01
23) Nitrobenzene-d5	9.20	82	331129	84.67	ng	-0.02
41) 2,4,6-Tribromophenol	16.16	330	179722	106.52	ng	-0.02
44) 2-Fluorobiphenyl	13.29	172	782612	79.02	ng	-0.02
78) Terphenyl-d14	20.02	244	1303760	82.47	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG091918\
Data File : BG036835.D
Acq On : 20 Sep 2018 1:11
Operator : JU/SJ
Sample : PB113024BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB113024BL

Quant Time: Sep 20 07:37:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 31 13:03:20 2018
Response via : Initial Calibration

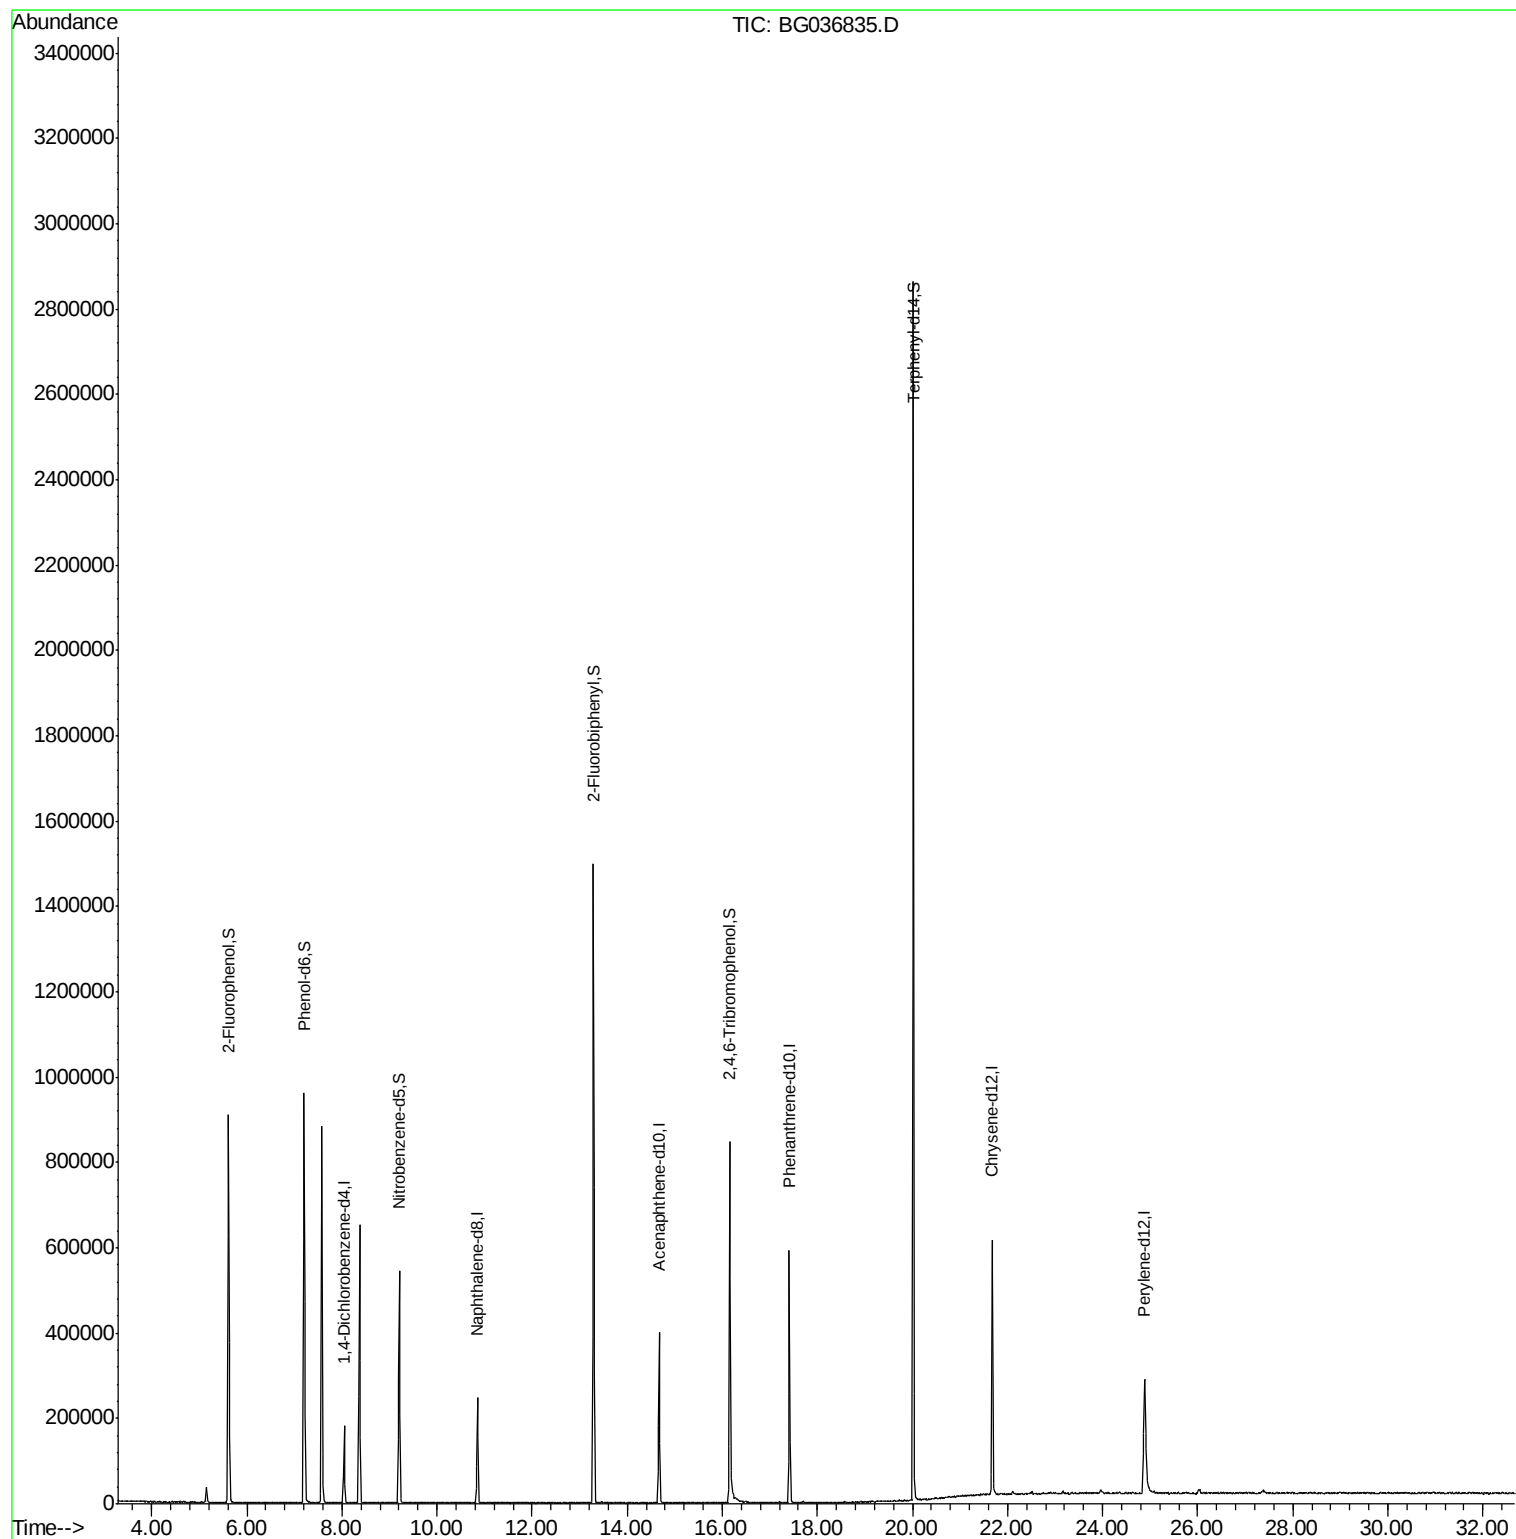

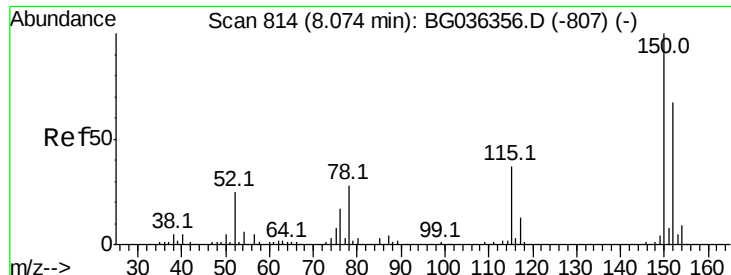


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.05 min Scan# 810
Delta R.T. -0.02 min
Lab File: BG036835.D
Acq: 20 Sep 2018 1:11

Instrument :
BNA_G
ClientSampleId :
PB113024BL

Tot Ion:152 Resp: 51824
Ion Ratio Lower Upper
152 100
150 147.8 119.5 179.3
115 55.6 44.5 66.7

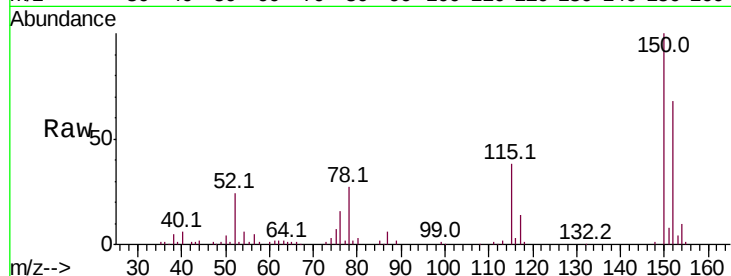


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

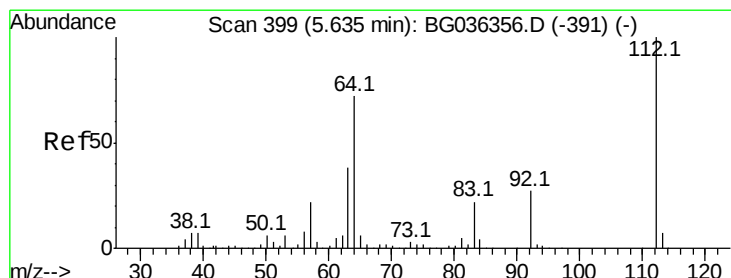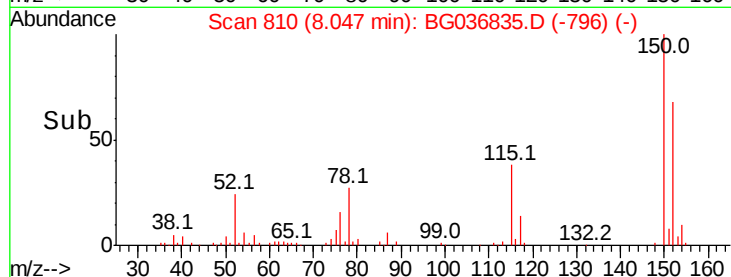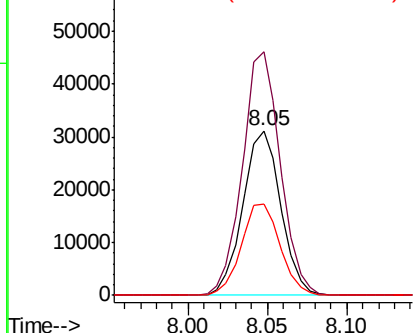



#5


2-Fluorophenol
Concen: 118.380 ng
RT: 5.62 min Scan# 397
Delta R.T. -0.00 min
Lab File: BG036835.D
Acq: 20 Sep 2018 1:11

Tgt Ion:112 Resp: 386746
Ion Ratio Lower Upper
112 100
64 68.1 57.2 85.8
63 35.2 30.8 46.2

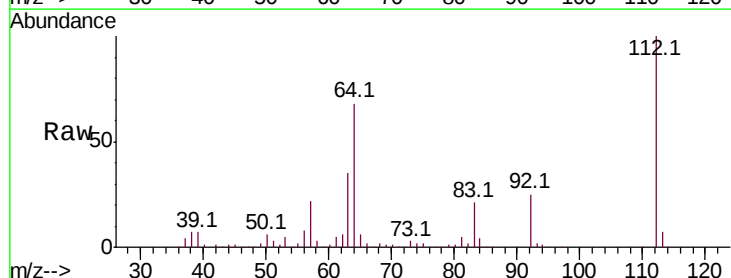

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

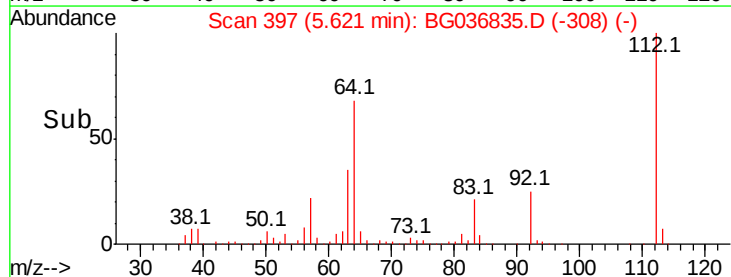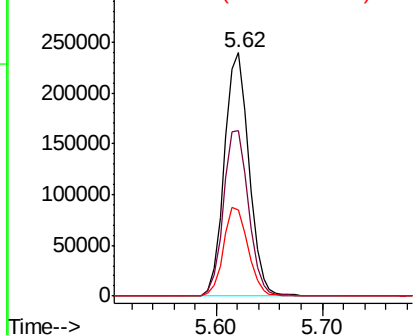

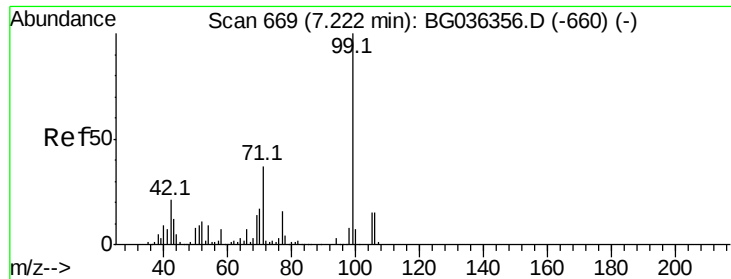

#7

Phenol-d6

Concen: 115.995 ng

RT: 7.21 min Scan# 667

Delta R.T. -0.01 min

Lab File: BG036835.D

Acq: 20 Sep 2018 1:11

Instrument :

BNA_G

ClientSampleId :

PB113024BL


Tot Ion: 99 Resp: 542570

Ion Ratio Lower Upper




99 100

42 19.9 16.5 24.7

71 35.3 29.4 44.2

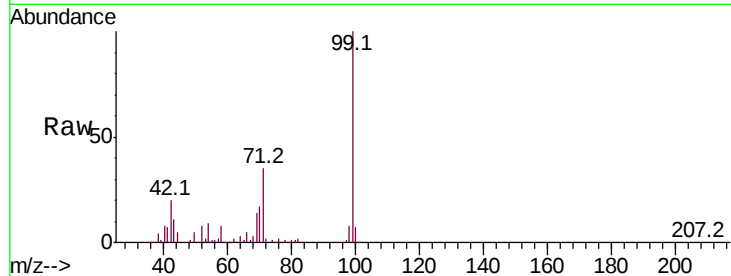

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

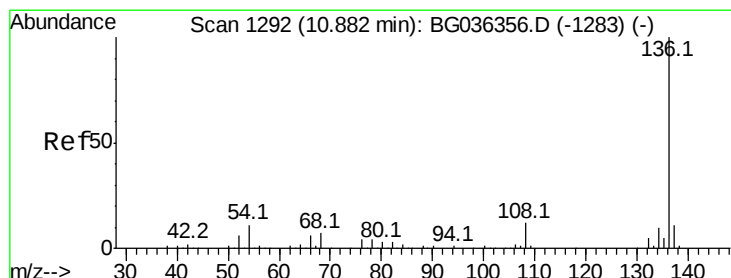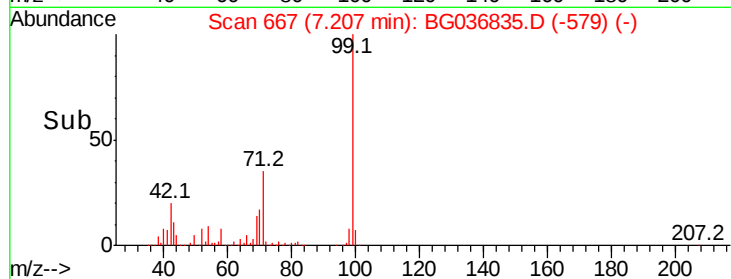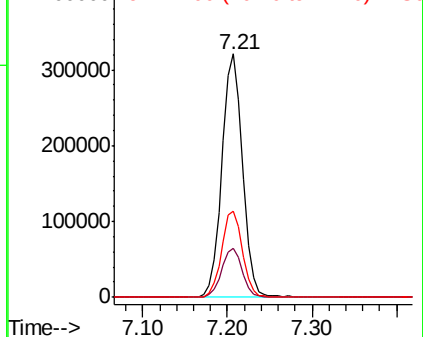

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.85 min Scan# 1287

Delta R.T. -0.02 min

Lab File: BG036835.D

Acq: 20 Sep 2018 1:11

Tgt Ion: 136 Resp: 212181


Ion Ratio Lower Upper

136 100



137 11.6 8.8 13.2


54 9.6 9.2 13.8

68 7.1 5.8 8.6

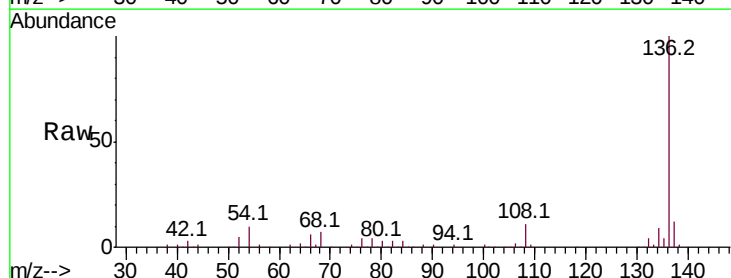

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



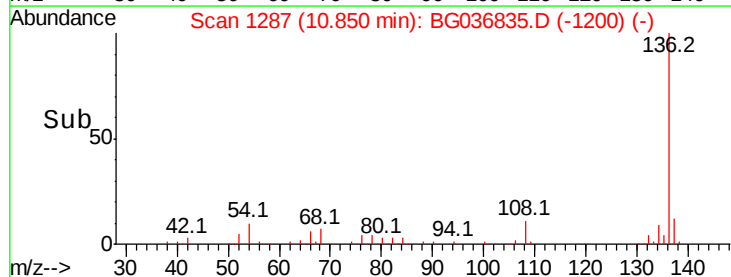
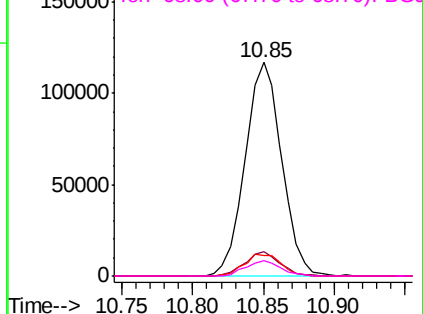


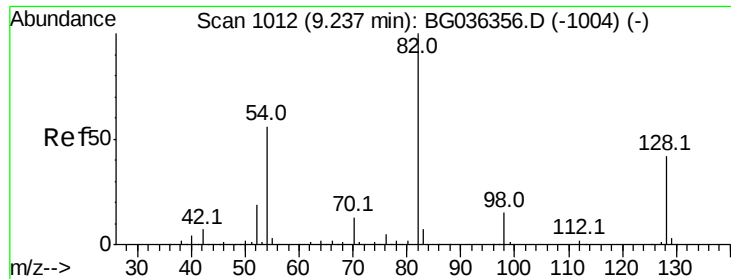

#23
Nitrobenzene-d5
Concen: 84.673 ng
RT: 9.20 min Scan# 1007
Delta R.T. -0.02 min
Lab File: BG036835.D
Acq: 20 Sep 2018 1:11




Instrument :
BNA_G
ClientSampleId :
PB113024BL


Tot Ion: 82 Resp: 331129
Ion Ratio Lower Upper
82 100
128 41.8 33.3 49.9
54 55.2 45.1 67.7

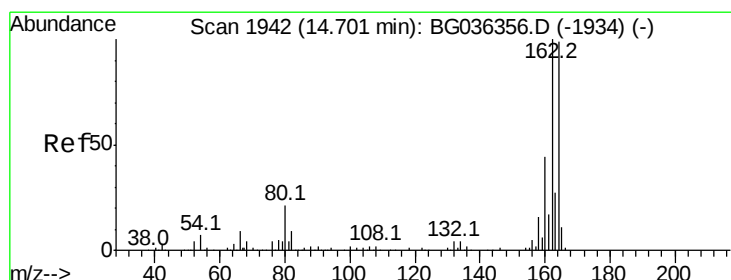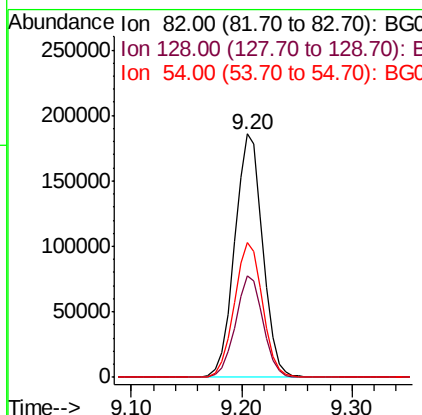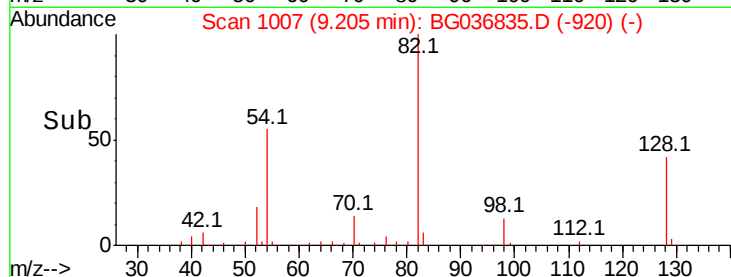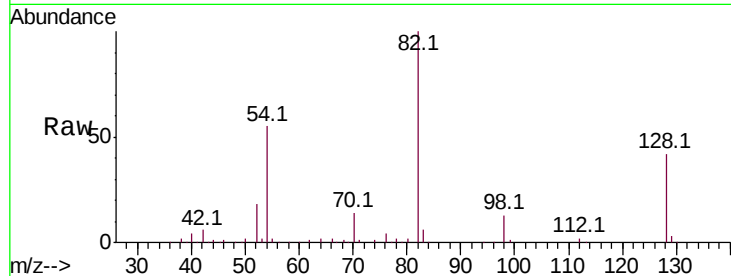

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.67 min Scan# 1937
Delta R.T. -0.02 min
Lab File: BG036835.D
Acq: 20 Sep 2018 1:11

Tgt Ion:164 Resp: 141403
Ion Ratio Lower Upper
164 100
162 107.4 80.7 121.1
160 45.2 35.3 52.9

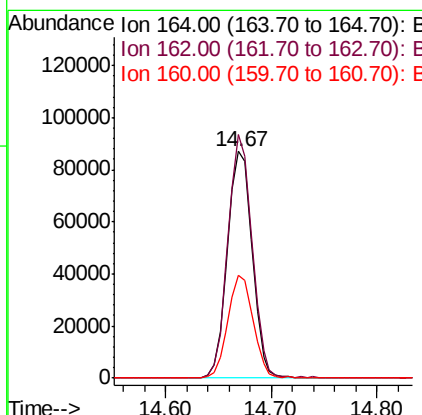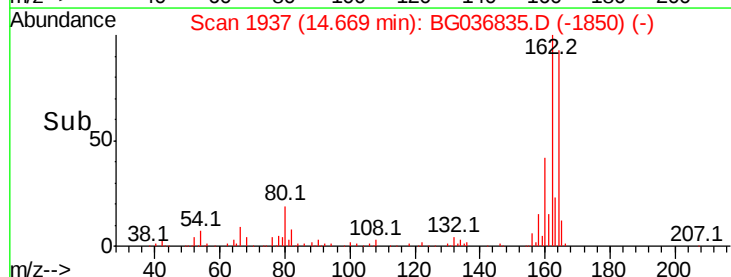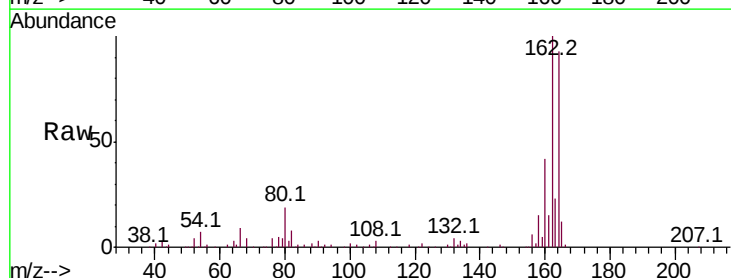


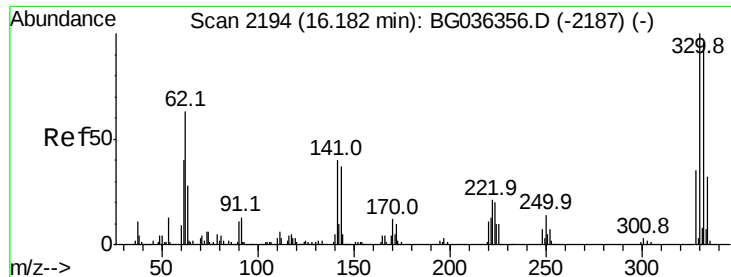




#41
 2,4,6-Tribromophenol
 Concen: 106.517 ng
 RT: 16.16 min Scan# 2190
 Delta R.T. -0.02 min
 Lab File: BG036835.D
 Acq: 20 Sep 2018 1:11

Instrument :
 BNA_G
 ClientSampleId :
 PB113024BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.0	75.4	113.2
141	36.6	30.7	46.1

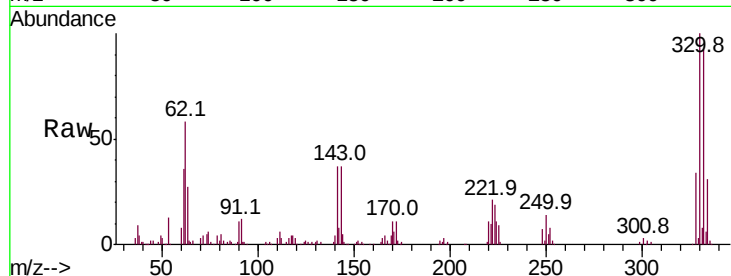


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

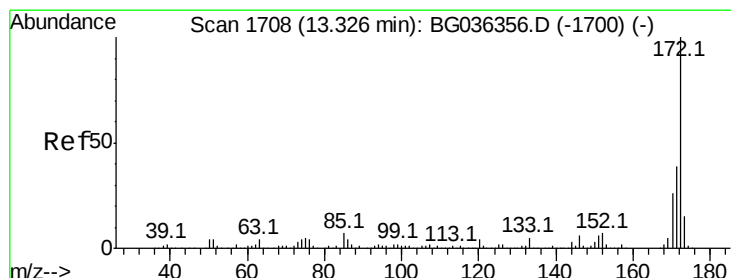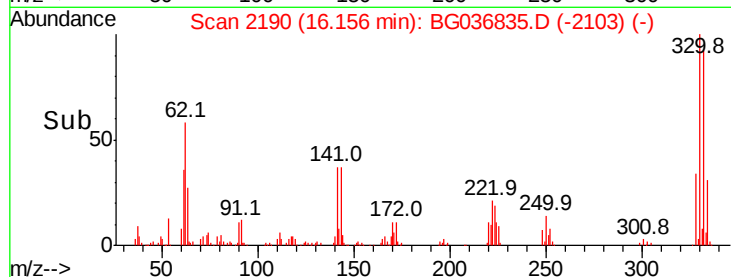
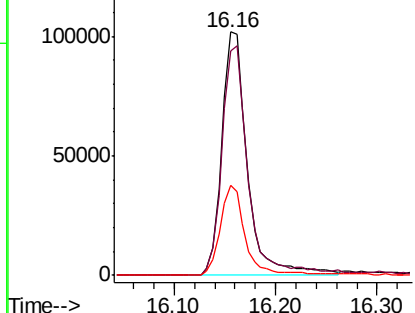



#44
 2-Fluorobiphenyl
 Concen: 79.024 ng
 RT: 13.29 min Scan# 1703
 Delta R.T. -0.02 min
 Lab File: BG036835.D
 Acq: 20 Sep 2018 1:11

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.6	31.3	46.9
170	24.5	21.0	31.6

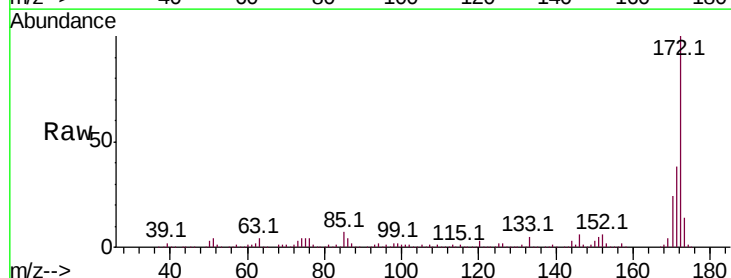

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

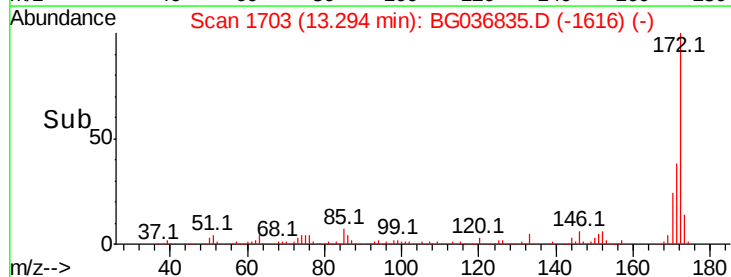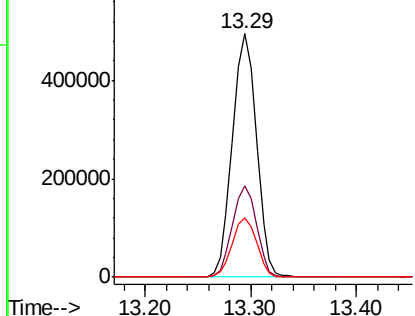

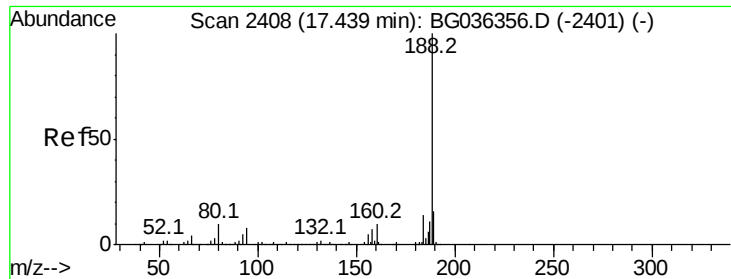

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.41 min Scan# 2404

Delta R.T. -0.02 min

Lab File: BG036835.D

Acq: 20 Sep 2018 1:11

Instrument :

BNA_G

ClientSampleId :

PB113024BL


Tot Ion:188 Resp: 362293

Ion Ratio Lower Upper

188 100

94 7.7 6.7 10.1




80 9.0 8.1 12.1

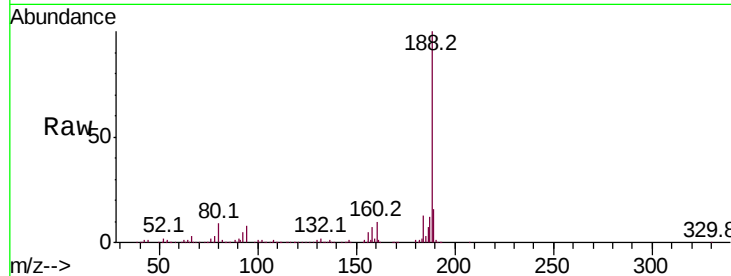

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

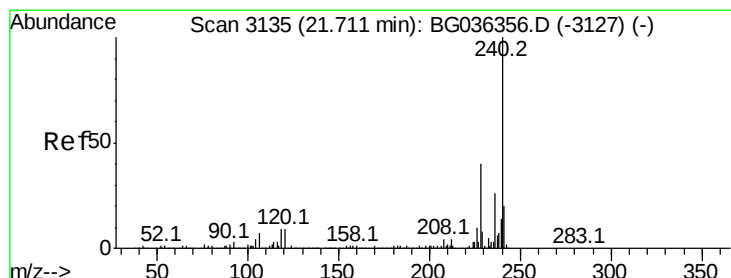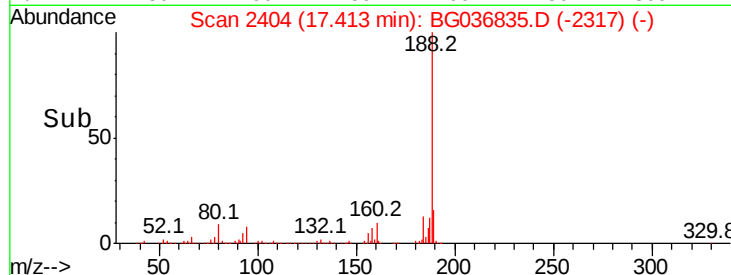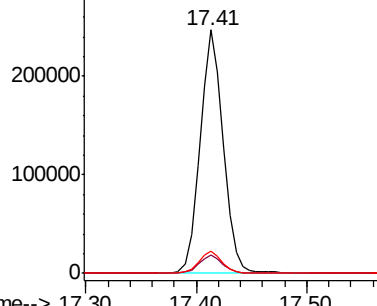

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.68 min Scan# 3130

Delta R.T. -0.02 min

Lab File: BG036835.D

Acq: 20 Sep 2018 1:11


Tgt Ion:240 Resp: 369489

Ion Ratio Lower Upper

240 100

120 8.2 6.9 10.3



236 26.6 21.2 31.8

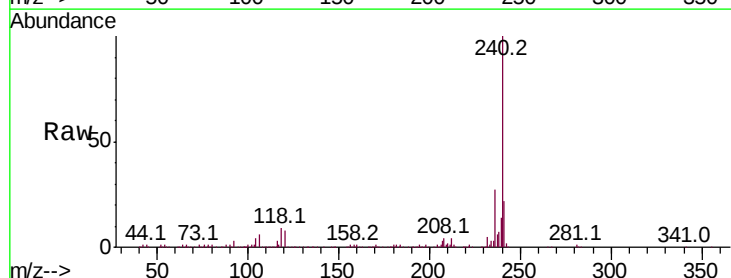


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

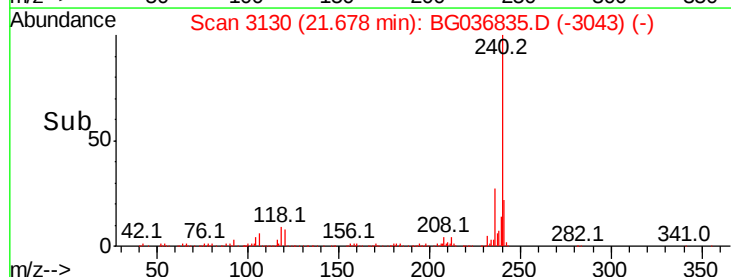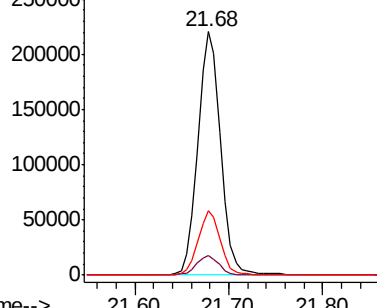

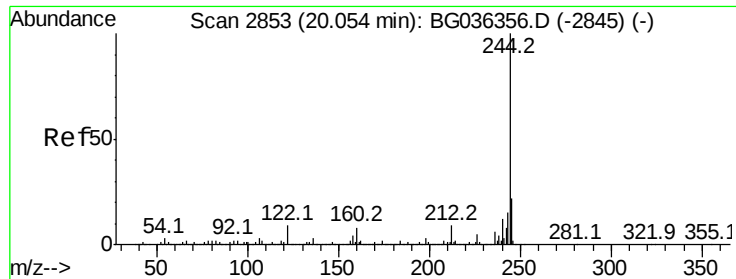

#78

Terphenyl-d14

Concen: 82.474 ng

RT: 20.02 min Scan# 2848

Delta R.T. -0.01 min

Lab File: BG036835.D

Acq: 20 Sep 2018 1:11

Instrument :

BNA_G

ClientSampleId :

PB113024BL





Tot Ion:244 Resp: 1303760

Ion	Ratio	Lower	Upper
244	100		
212	8.8	7.0	10.6
122	8.8	7.1	10.7

244 100

212 8.8 7.0 10.6

122 8.8 7.1 10.7

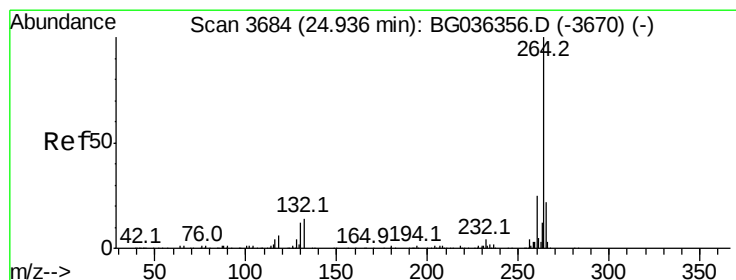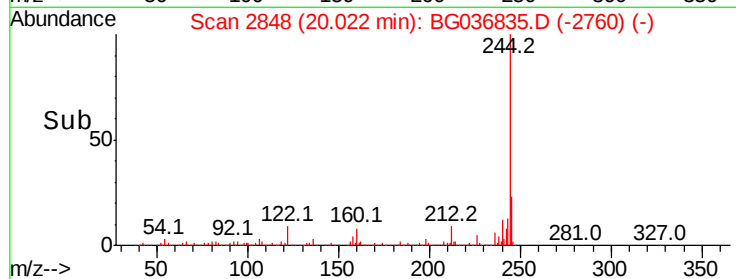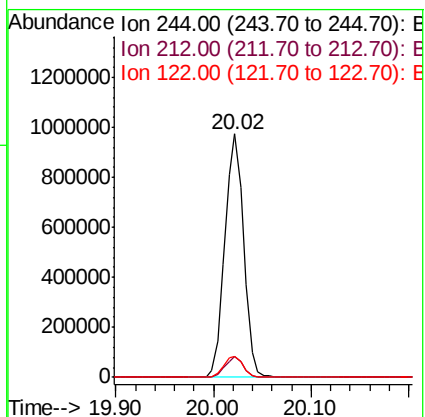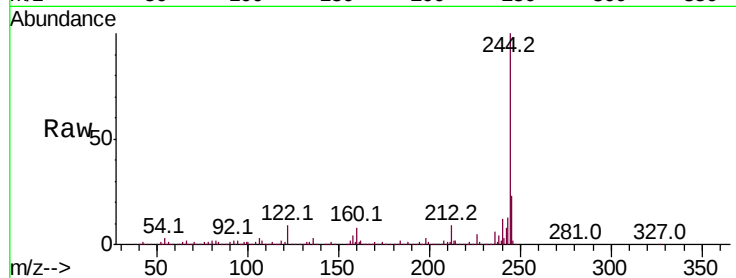

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.88 min Scan# 3675

Delta R.T. -0.02 min

Lab File: BG036835.D

Acq: 20 Sep 2018 1:11

Tgt Ion:264 Resp: 350084

Ion	Ratio	Lower	Upper
264	100		
260	23.6	19.6	29.4
265	22.3	17.4	26.0

264 100

260 23.6 19.6 29.4

265 22.3 17.4 26.0

