


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG091918\
 Data File : BG036823.D
 Acq On : 19 Sep 2018 17:22
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 31 13:03:20 2018

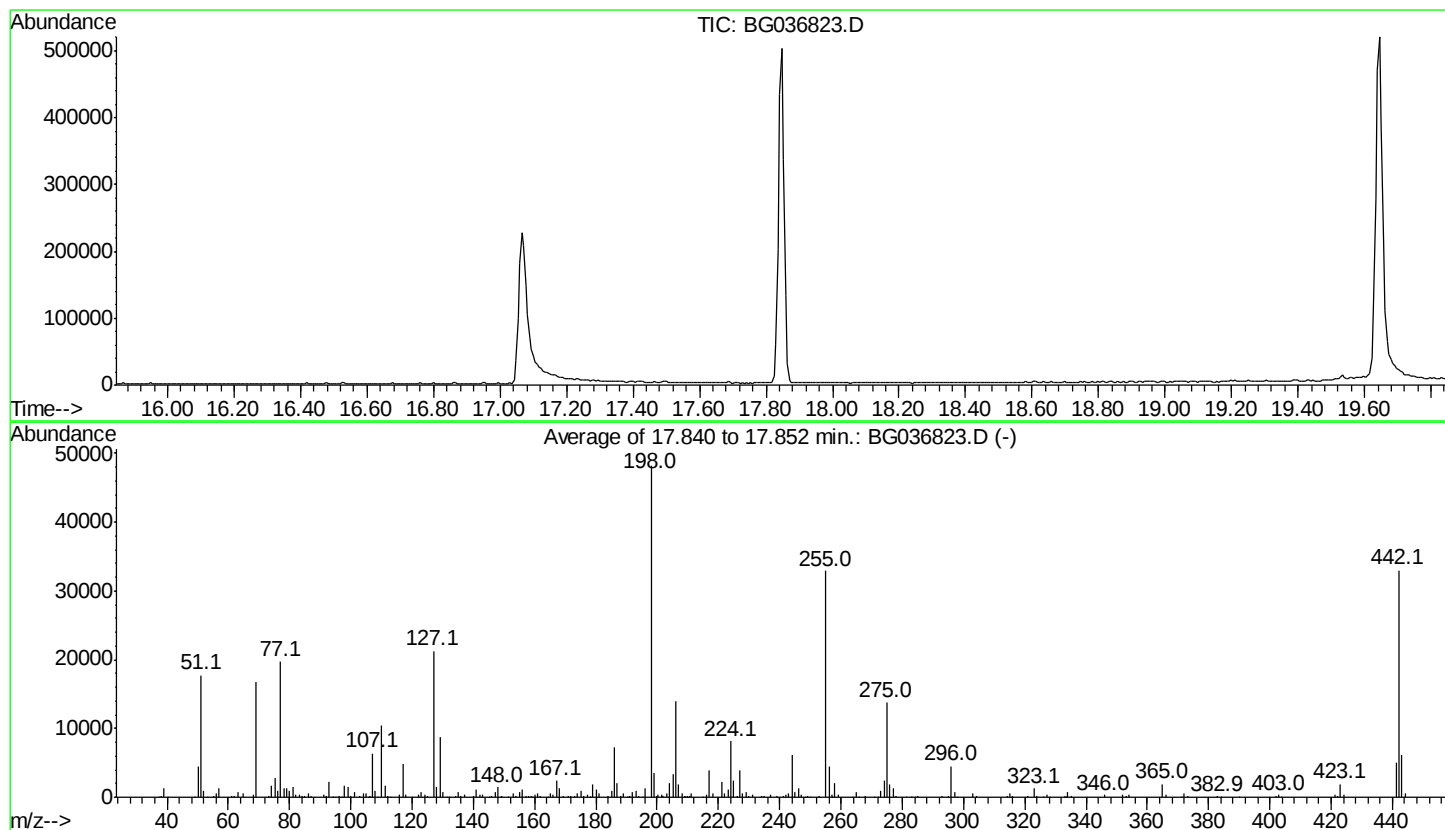

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	17725	PASS
68	69	0.00	2	1.8	300	PASS
69	198	0.00	100	34.9	16806	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.1	21259	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48192	PASS
199	198	5	9	7.2	3475	PASS
275	198	10	60	28.5	13725	PASS
365	198	1	100	4.0	1942	PASS
441	198	0.01	100	10.3	4965	PASS
442	198	50	100	68.4	32965	PASS
443	442	15	24	18.8	6189	PASS