
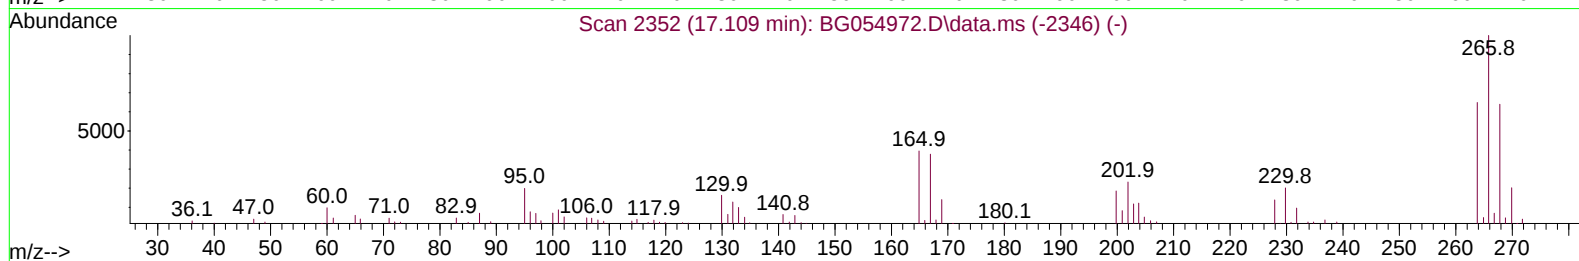
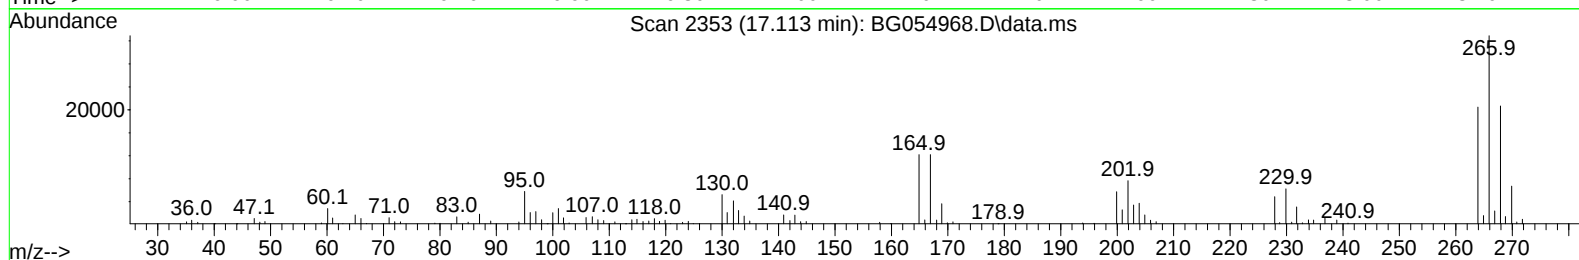


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091922\
Data File : BG054968.D
Acq On : 19 Sep 2022 11:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 19 17:52:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 19 17:41:40 2022
Response via : Initial Calibration

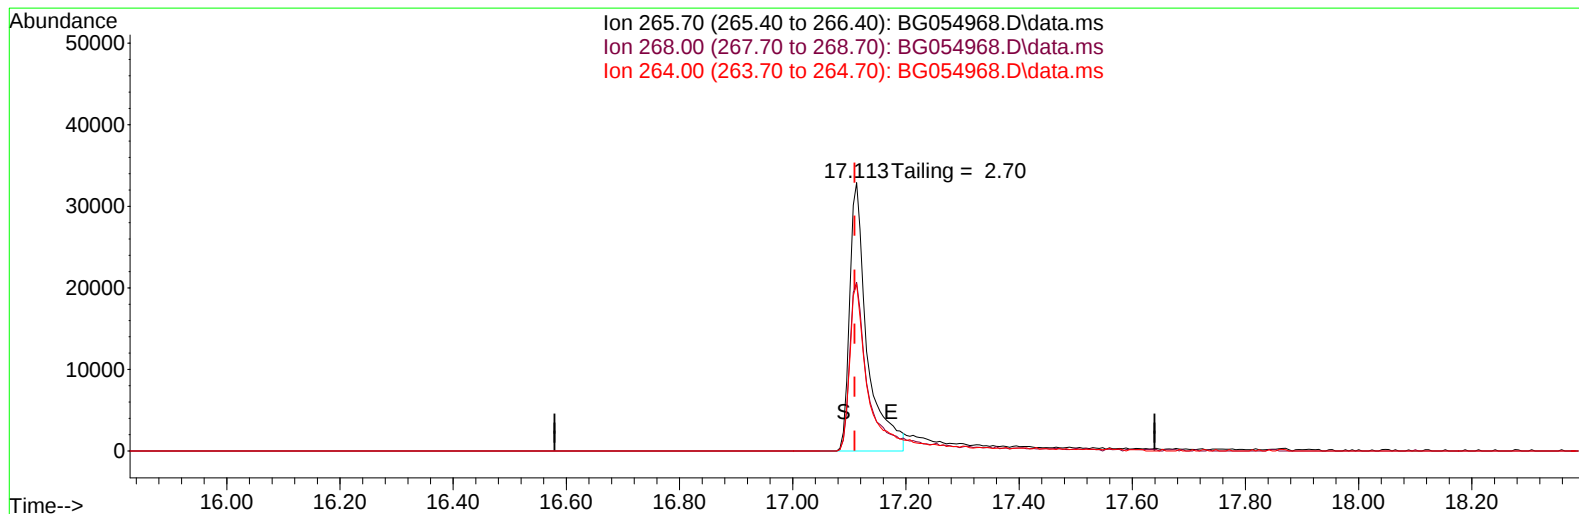

TIC: BG054968.D\data.ms

(70) Pentachlorophenol (C)




17.113min (+ 0.004) 3578.88 ng

response 78288

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	62.85
264.00	61.70	62.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091922\
Data File : BG054968.D
Acq On : 19 Sep 2022 11:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 19 17:52:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 19 17:41:40 2022
Response via : Initial Calibration

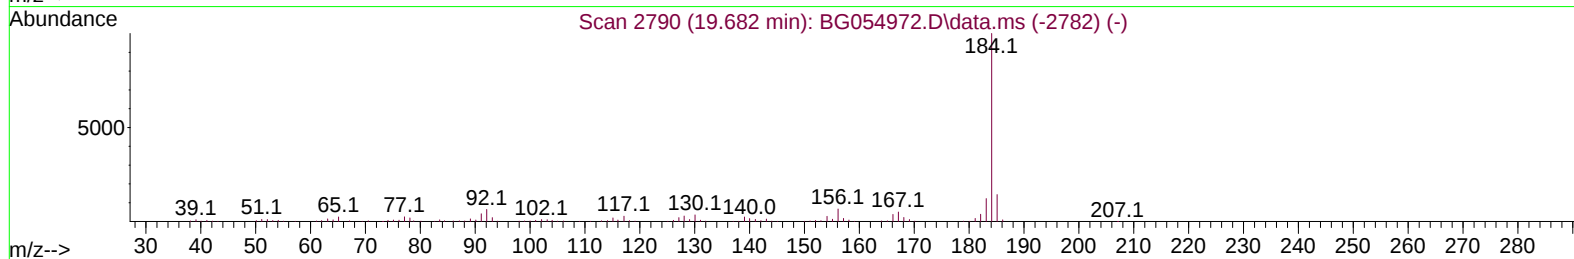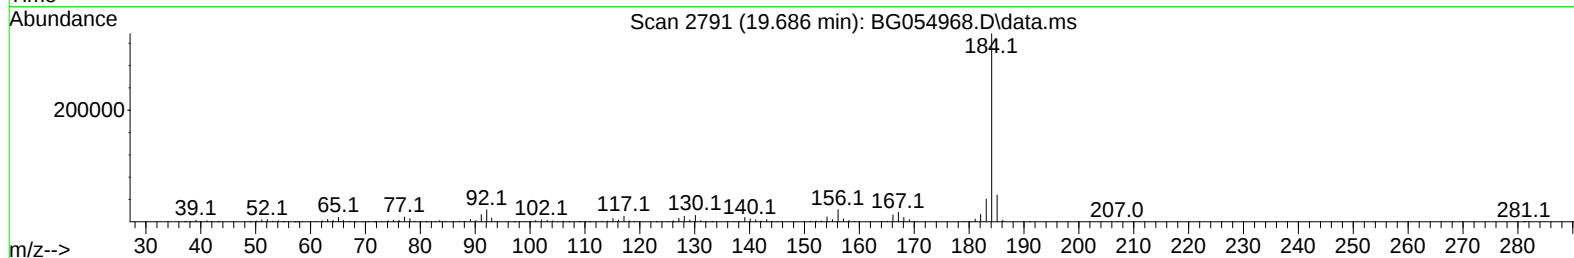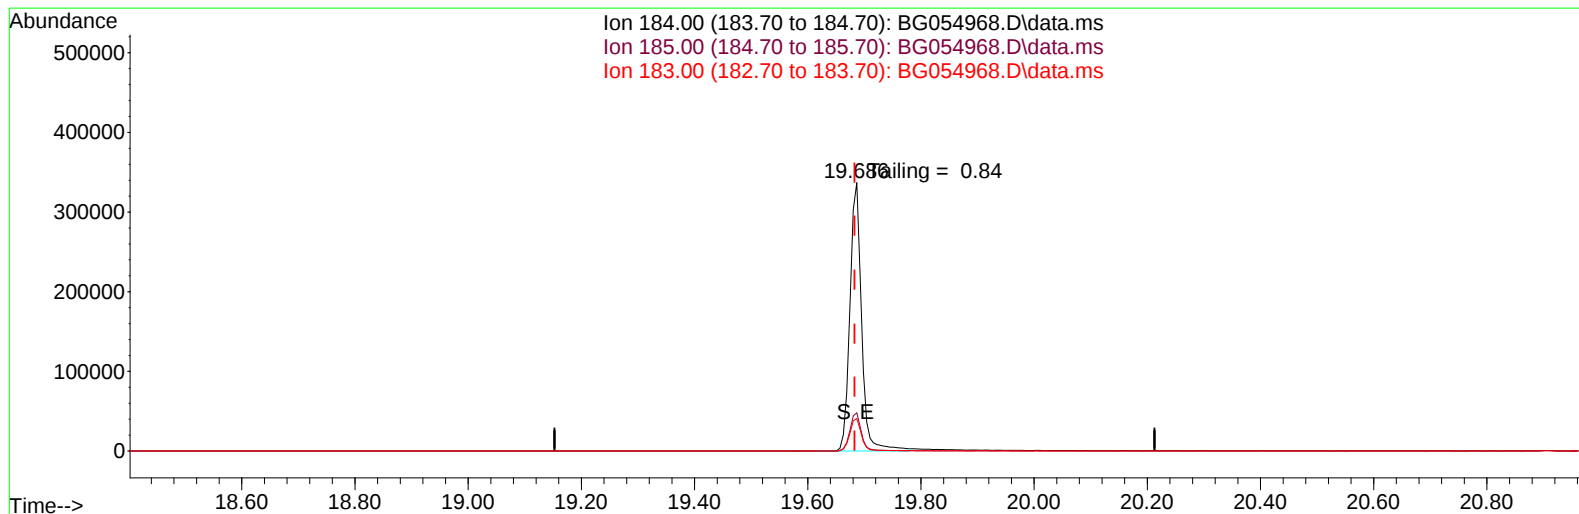

TIC: BG054968.D\data.ms

(77) Benzidine

19.686min (+ 0.004) 0.00 ng

response 494019

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.25
183.00	12.30	12.11
0.00	0.00	0.00