
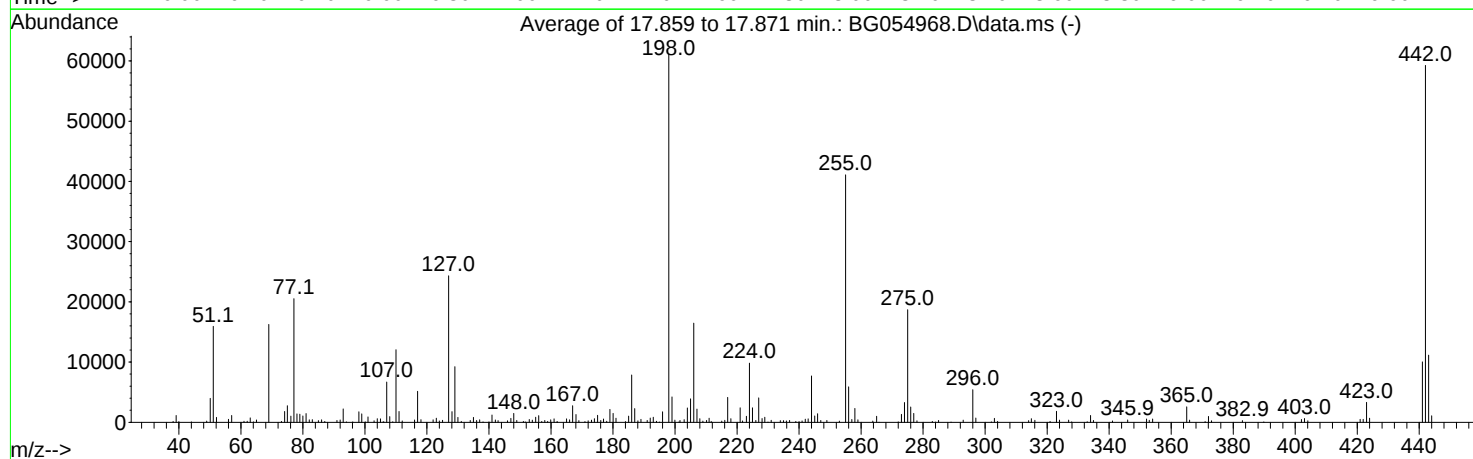


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091922\
 Data File : BG054968.D
 Acq On : 19 Sep 2022 11:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 19 17:41:40 2022

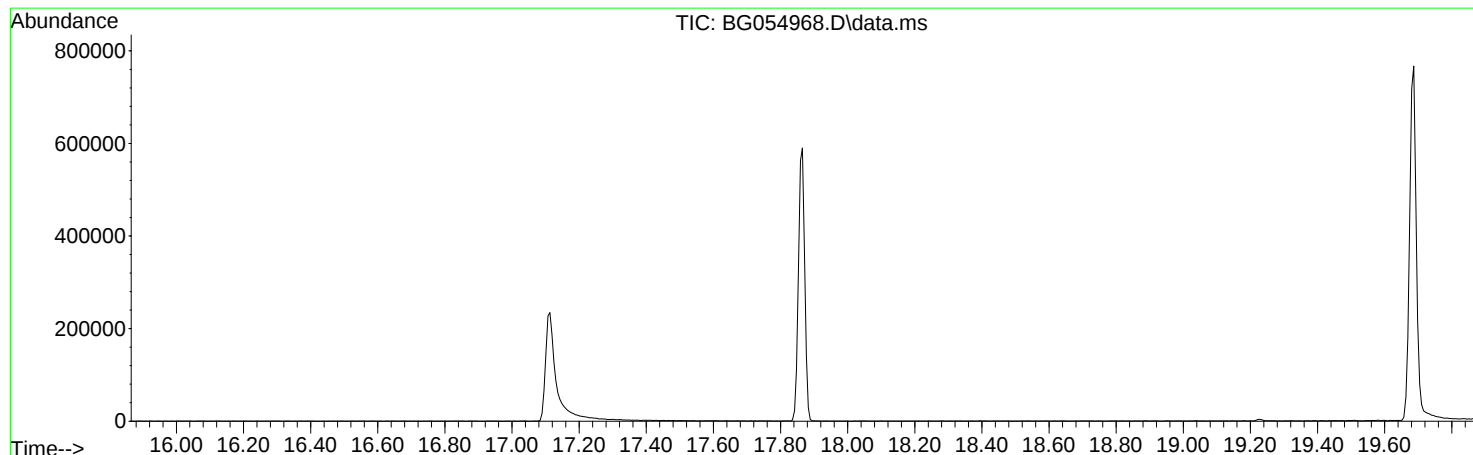




AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.1	15919	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	26.6	16254	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	39.8	24315	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	61080	PASS
199	198	5	9	6.9	4221	PASS
275	198	10	60	30.6	18696	PASS
365	198	1	100	4.2	2564	PASS
441	198	0.01	100	16.4	10042	PASS
442	442	50	100	100.0	59256	PASS
443	442	15	24	18.8	11153	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091922\
Data File : BG054968.D
Acq On : 19 Sep 2022 11:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 19 17:52:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 19 17:41:40 2022
Response via : Initial Calibration

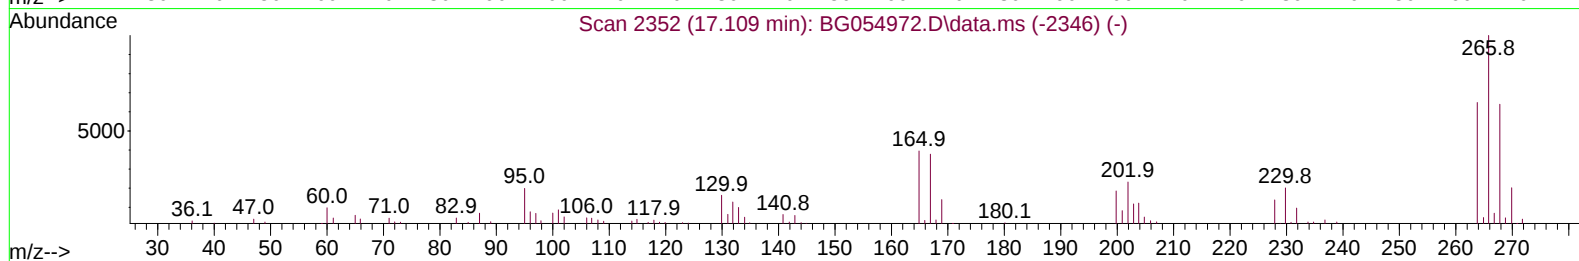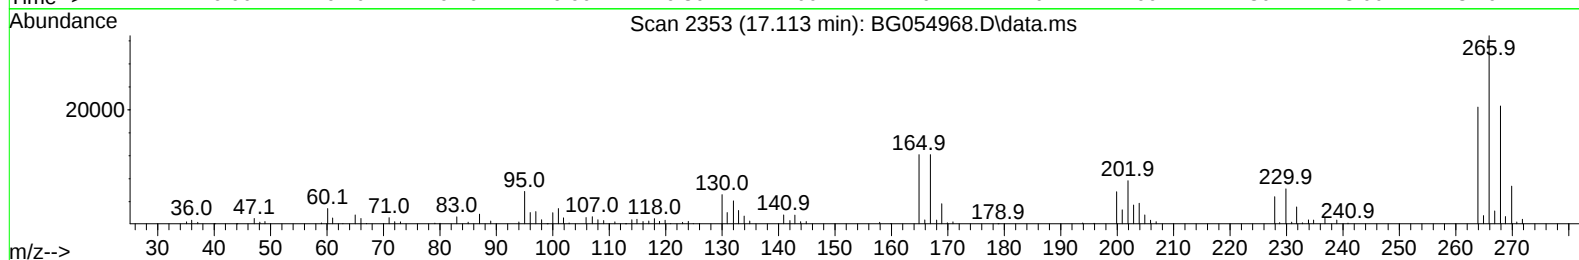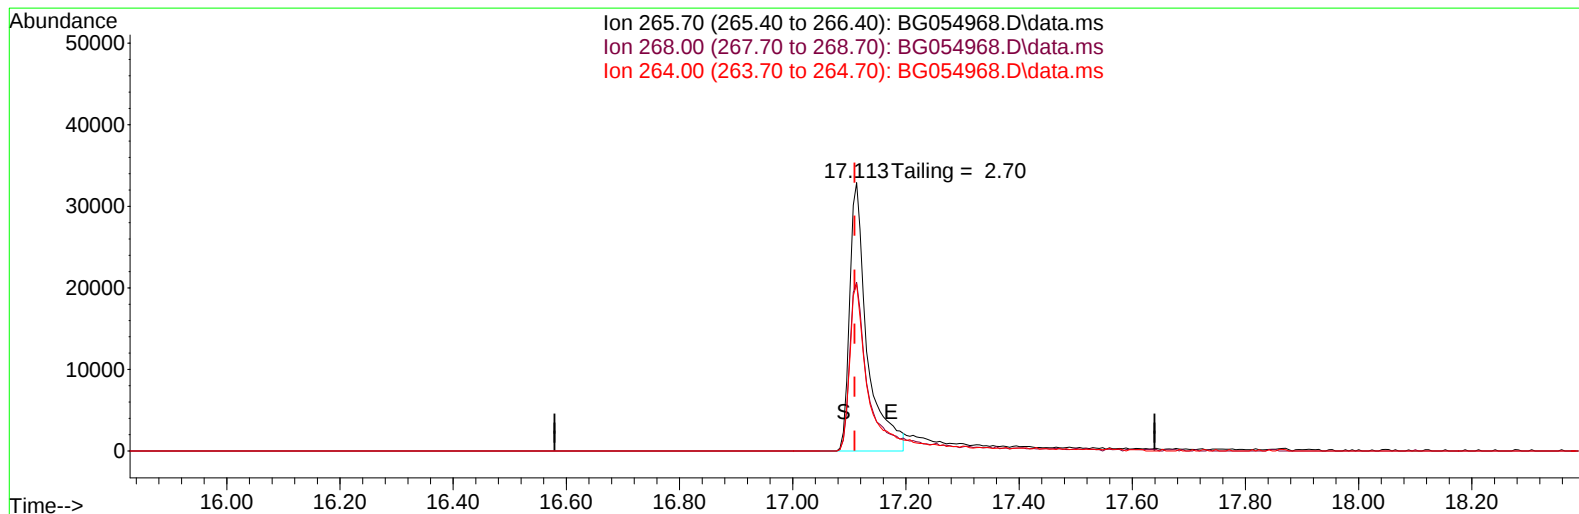

TIC: BG054968.D\data.ms

(70) Pentachlorophenol (C)

17.113min (+ 0.004) 3578.88 ng




response 78288

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	62.85
264.00	61.70	62.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091922\
Data File : BG054968.D
Acq On : 19 Sep 2022 11:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 19 17:52:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 19 17:41:40 2022
Response via : Initial Calibration

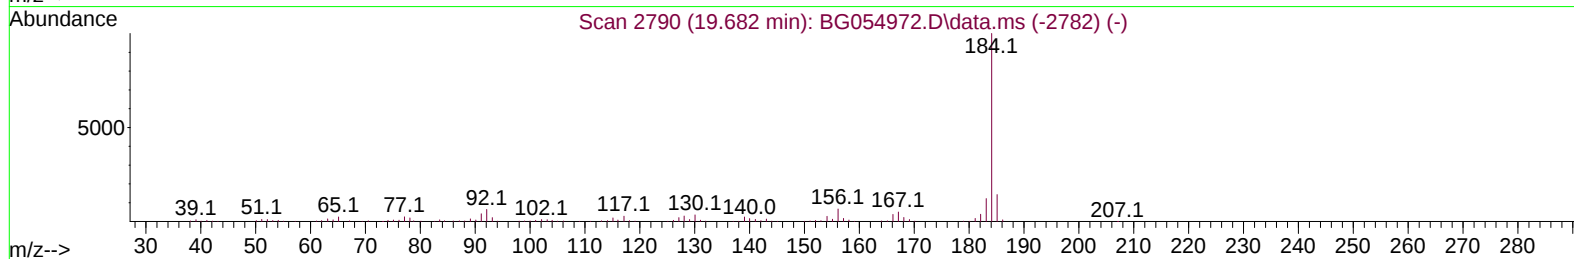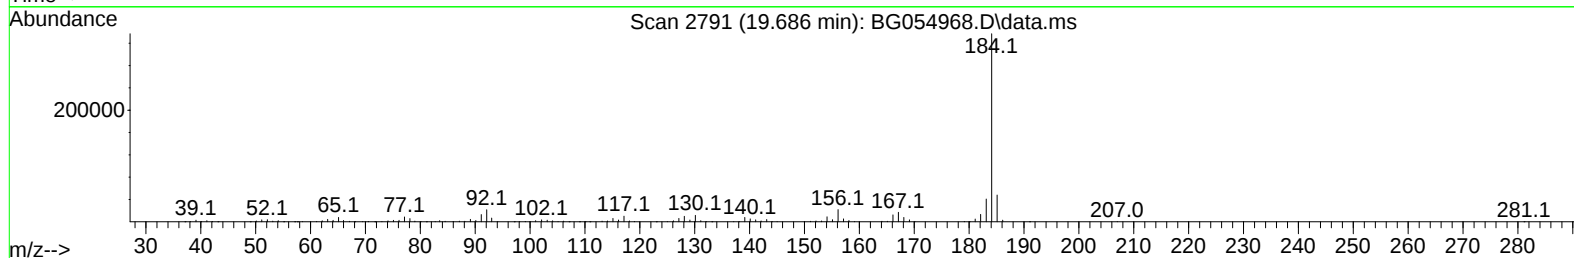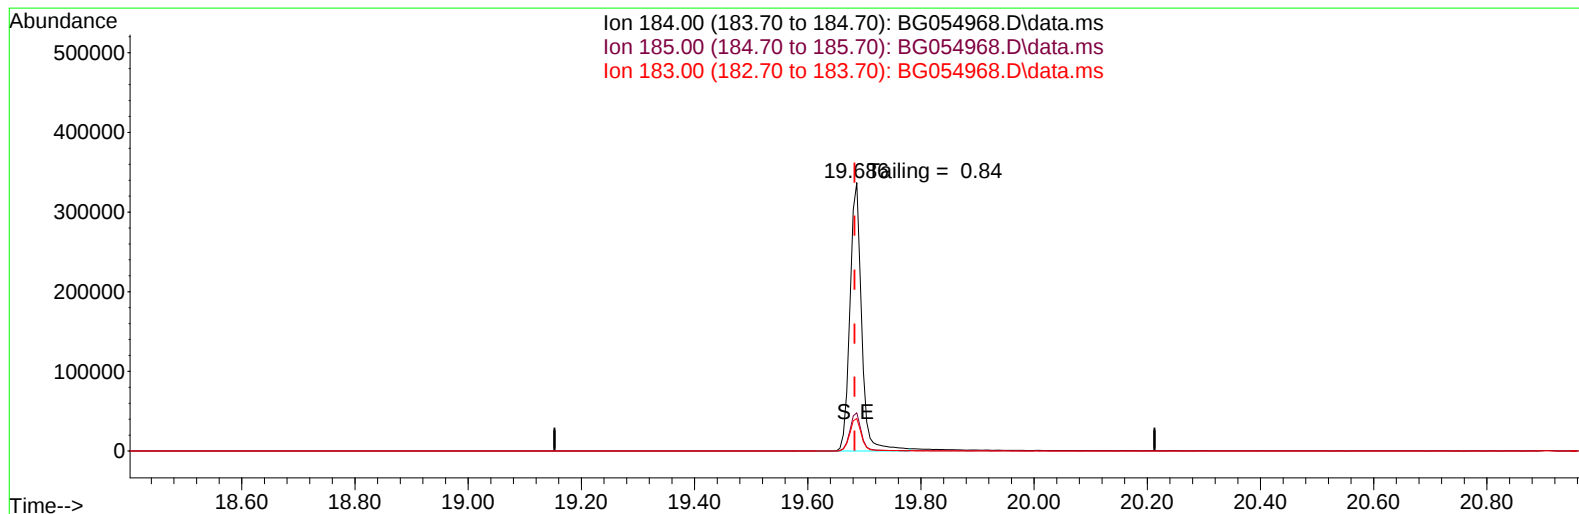

TIC: BG054968.D\data.ms

(77) Benzidine

19.686min (+ 0.004) 0.00 ng

response 494019

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.25
183.00	12.30	12.11
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/19/2022	BNA_G	BG054968.D
Compound Name	Response	Retention Time
DDT	225224	20.9
DDD	3760	20.46
DDE	0	19.9
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3760	228984	1.64

Instrument :
BNA_G
ClientSampleId :
DFTPP