

Data Path : Z:\HPCHEM1\BNA G\DATA\BG092017\
 Data File : BG028846.D
 Acq On : 21 Sep 2017 7:09
 Operator : SJ/JU
 Sample : I5293-09
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SP-A-COMP

Quant Time: Sep 21 08:58:12 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 12 16:57:11 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.29	152	34270	20.00	ng	-0.04
21) Naphthalene-d8	11.11	136	133852	20.00	ng	-0.04
38) Acenaphthene-d10	14.90	164	95385	20.00	ng	-0.04
63) Phenanthrene-d10	17.66	188	262497	20.00	ng	-0.04
75) Chrysene-d12	21.98	240	285009	20.00	ng	-0.05
86) Perylene-d12	25.46	264	273870	20.00	ng	-0.07
System Monitoring Compounds						
5) 2-Fluorophenol	5.86	112	260298	125.33	ng	-0.04
7) Phenol-d6	7.44	99	307915	98.47	ng	-0.05
23) Nitrobenzene-d5	9.46	82	244282	87.30	ng	-0.05
41) 2,4,6-Tribromophenol	16.40	330	205195	130.07	ng	-0.04
44) 2-Fluorobiphenyl	13.52	172	618580	86.47	ng	-0.04
78) Terphenyl-d14	20.24	244	1202289	89.96	ng	-0.04


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG092017\
Data File : BG028846.D
Acq On : 21 Sep 2017 7:09
Operator : SJ/JU
Sample : I5293-09
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SP-A-COMP

Quant Time: Sep 21 08:58:12 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 16:57:11 2017
Response via : Initial Calibration

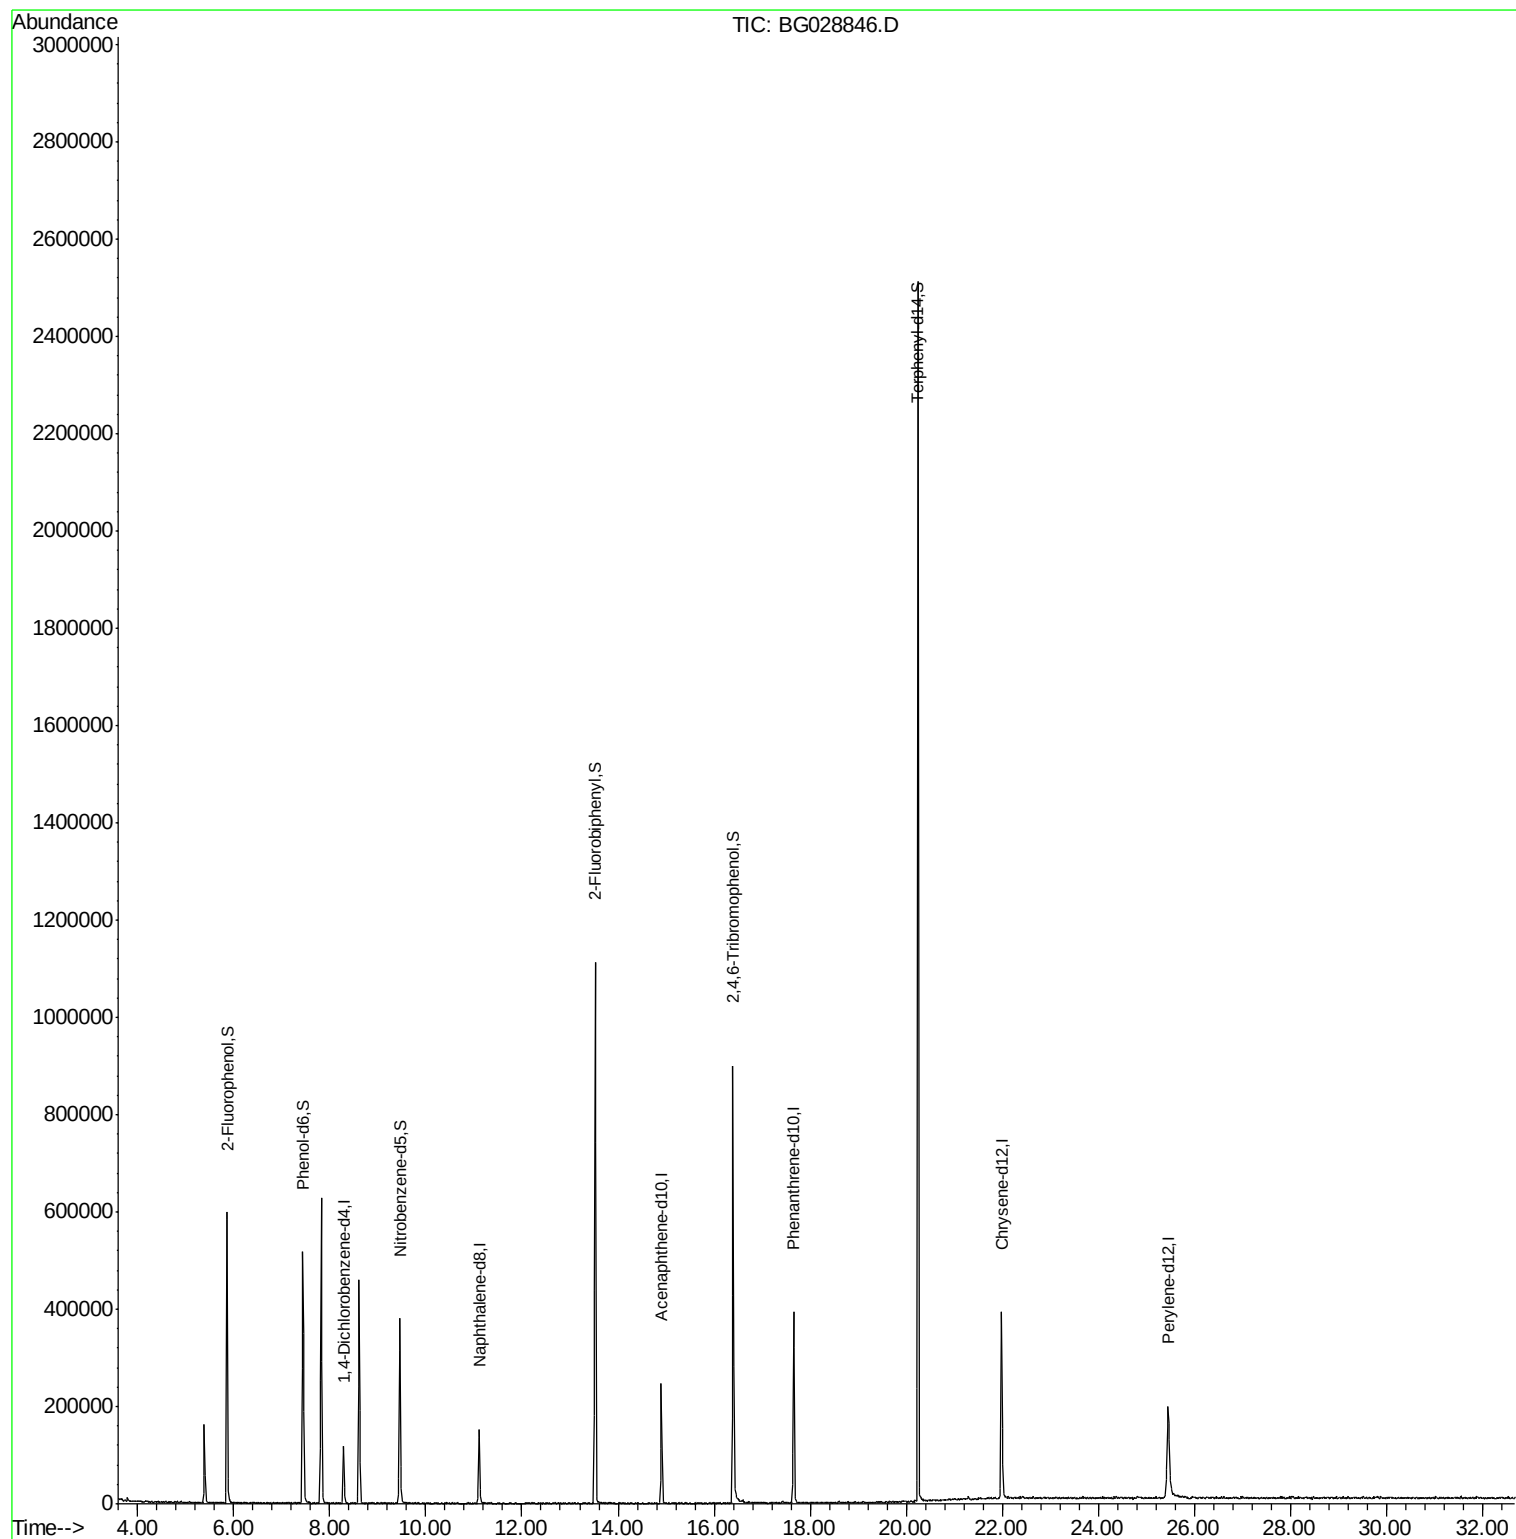

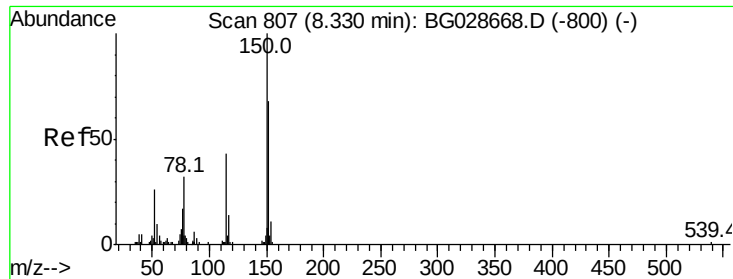

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 8.29 min Scan# 800

Delta R.T. -0.04 min

Lab File: BG028846.D

Acq: 21 Sep 2017 7:09

Instrument :

BNA_G

ClientSampleId :

SP-A-COMP





Tot Ion:152 Resp: 34270

Ion Ratio Lower Upper

152 100

150 154.1 114.0 171.0

115 70.0 48.1 72.1

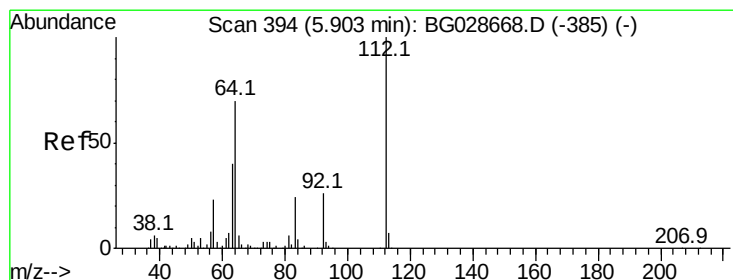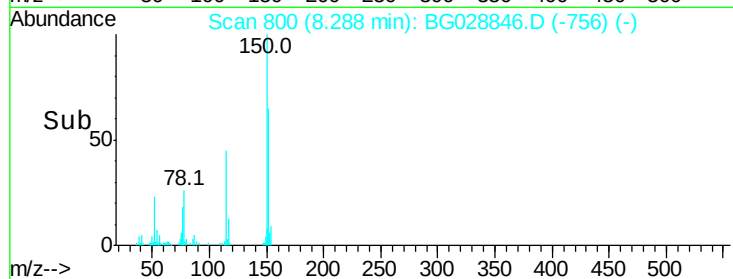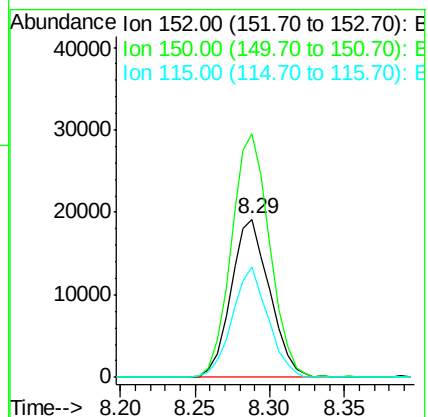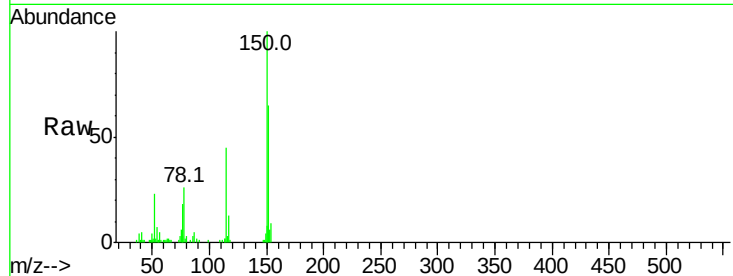

#5

2-Fluorophenol

Concen: 125.330 ng

RT: 5.86 min Scan# 387

Delta R.T. -0.04 min

Lab File: BG028846.D

Acq: 21 Sep 2017 7:09




Tgt Ion:112 Resp: 260298


Ion Ratio Lower Upper

112 100

64 66.6 61.8 92.6

63 37.7 37.2 55.8

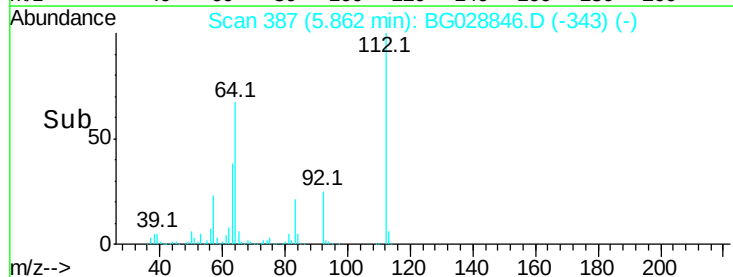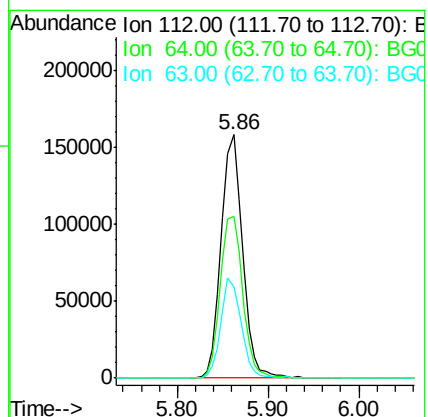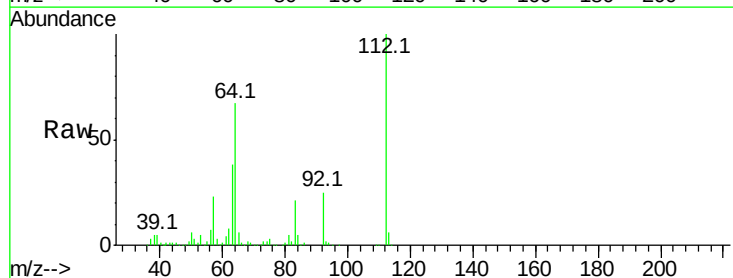

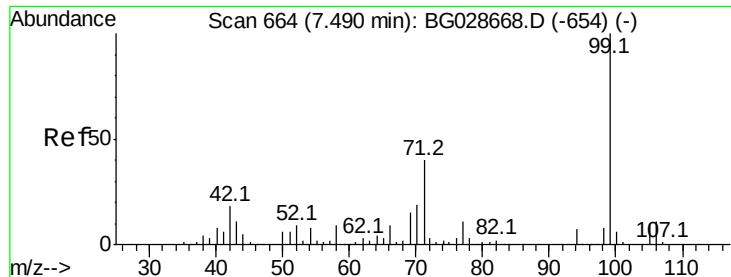

#7

Phenol-d6

Concen: 98.469 ng

RT: 7.44 min Scan# 656

Delta R.T. -0.05 min

Lab File: BG028846.D

Acq: 21 Sep 2017 7:09

Instrument :

BNA_G

ClientSampleId :

SP-A-COMP


Tot Ion: 99 Resp: 307915

Ion Ratio Lower Upper




99 100

42 17.8 20.5 30.7#

71 41.6 37.6 56.4

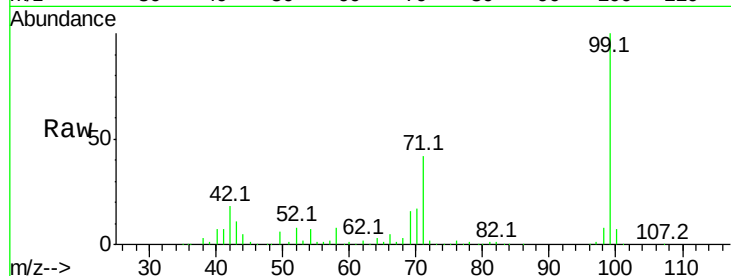

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

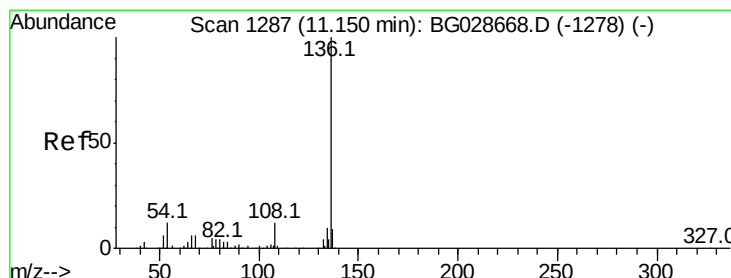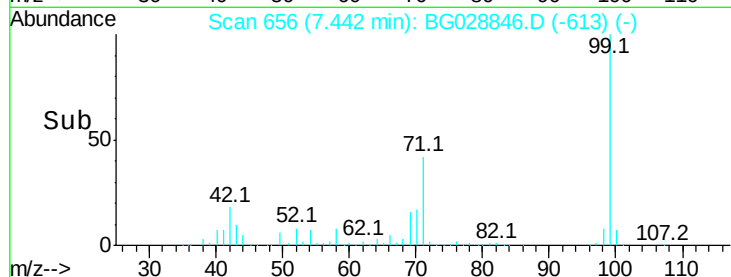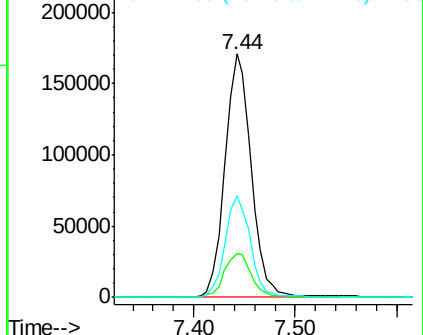

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.11 min Scan# 1280

Delta R.T. -0.04 min

Lab File: BG028846.D

Acq: 21 Sep 2017 7:09

Tgt Ion: 136 Resp: 133852

Ion Ratio Lower Upper




136 100


137 11.7 8.9 13.3

54 9.2 9.3 13.9#

68 5.4 5.1 7.7

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC


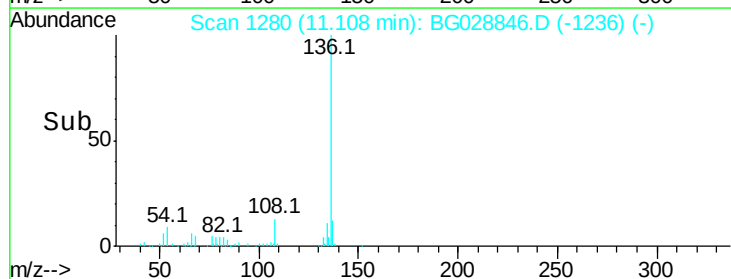
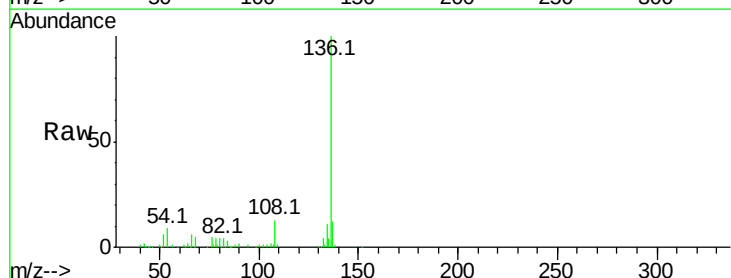
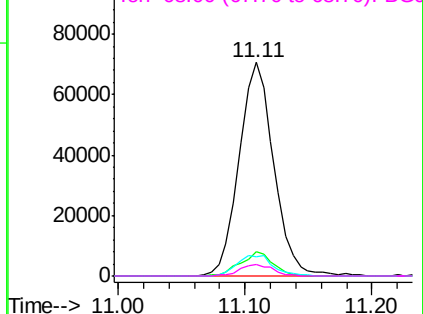


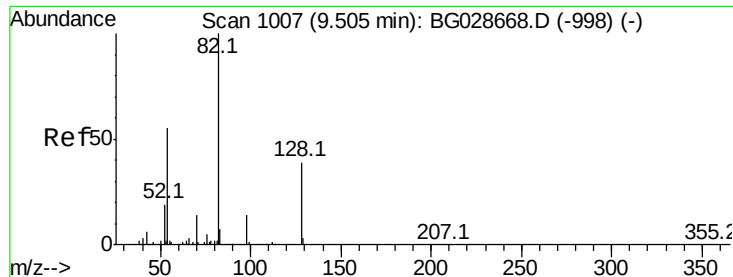

#23
 Nitrobenzene-d5
 Concen: 87.304 ng
 RT: 9.46 min Scan# 999
 Delta R.T. -0.05 min
 Lab File: BG028846.D
 Acq: 21 Sep 2017 7:09




Instrument :
 BNA_G
 ClientSampleId :
 SP-A-COMP


Tot Ion	82	Resp	244282
Ion	Ratio	Lower	Upper
82	100		
128	37.8	26.4	39.6
54	57.5	49.4	74.2

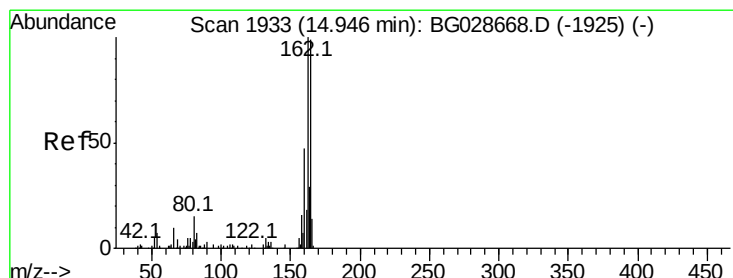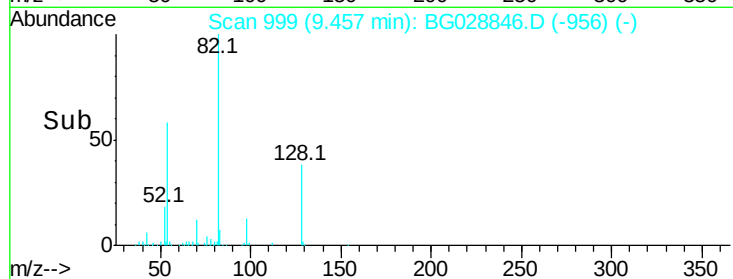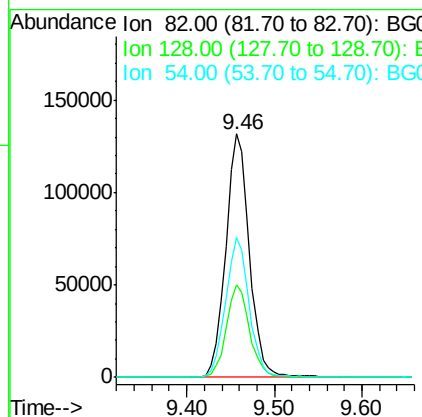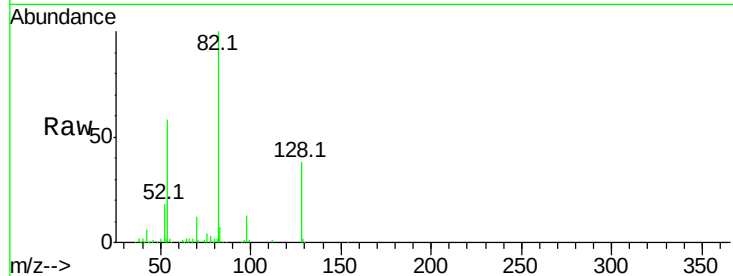

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.90 min Scan# 1926
 Delta R.T. -0.04 min
 Lab File: BG028846.D
 Acq: 21 Sep 2017 7:09

Tgt Ion	164	Resp	95385
Ion	Ratio	Lower	Upper
164	100		
162	96.0	85.1	127.7
160	43.9	34.7	52.1

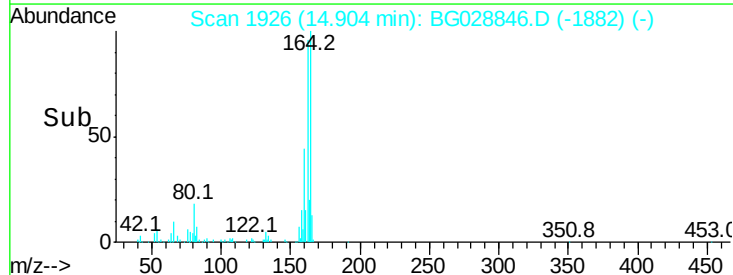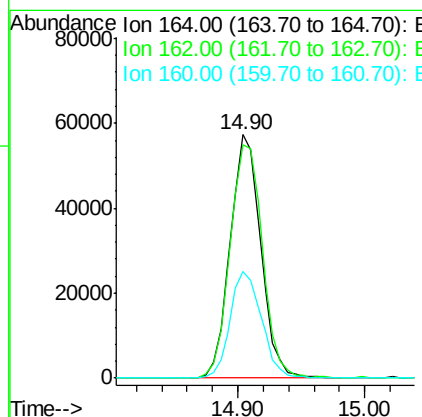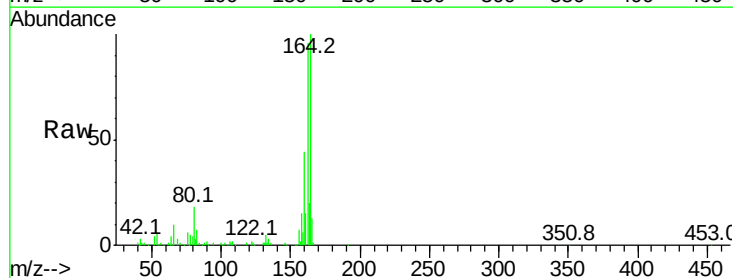


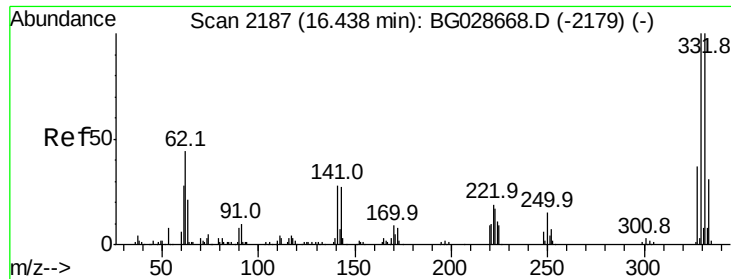




#41
 2,4,6-Tribromophenol
 Concen: 130.067 ng
 RT: 16.40 min Scan# 2180
 Delta R.T. -0.04 min
 Lab File: BG028846.D
 Acq: 21 Sep 2017 7:09

Instrument :
 BNA_G
 ClientSampleId :
 SP-A-COMP

Tot Ion:330 Resp: 205195
 Ion Ratio Lower Upper
 330 100
 332 97.6 77.3 115.9
 141 29.7 32.1 48.1#

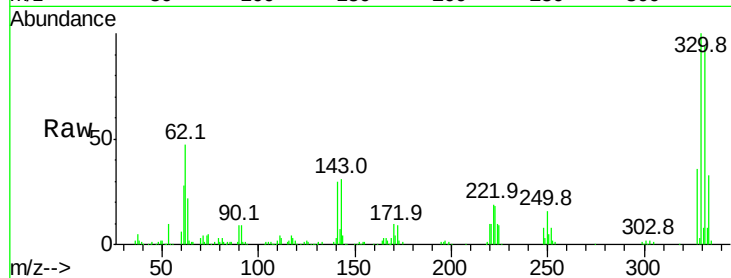


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

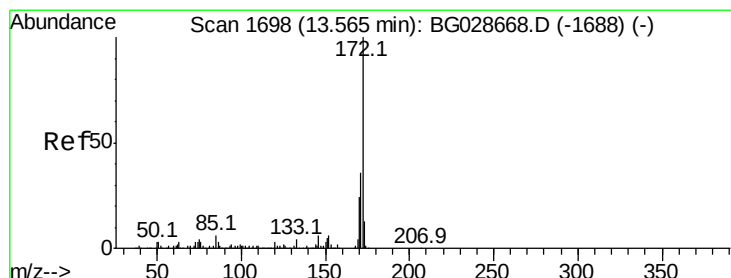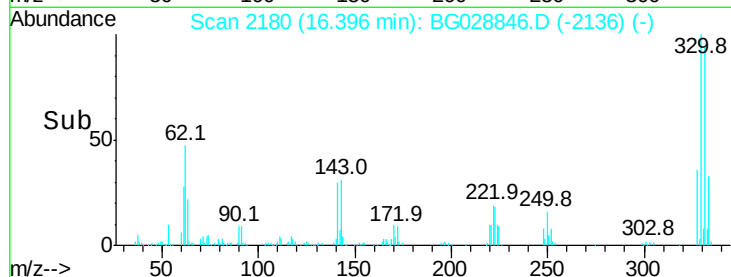
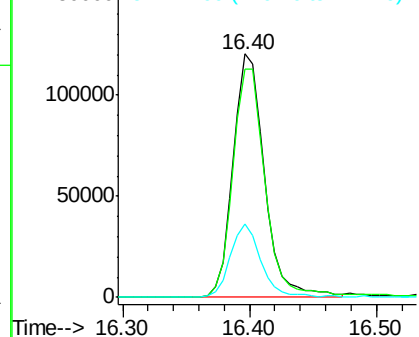



#44
 2-Fluorobiphenyl
 Concen: 86.474 ng
 RT: 13.52 min Scan# 1691
 Delta R.T. -0.04 min
 Lab File: BG028846.D
 Acq: 21 Sep 2017 7:09

Tgt Ion:172 Resp: 618580
 Ion Ratio Lower Upper
 172 100
 171 35.0 32.2 48.2
 170 22.5 21.8 32.6

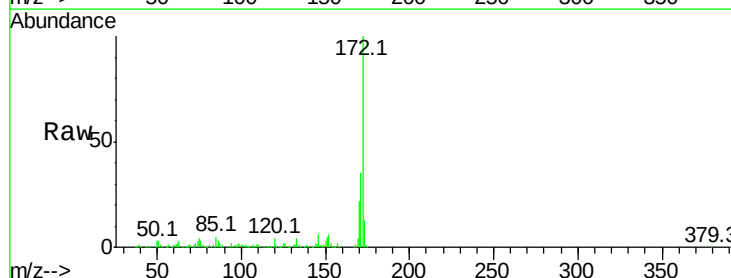

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

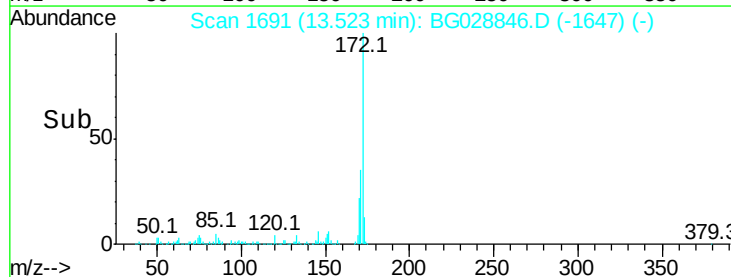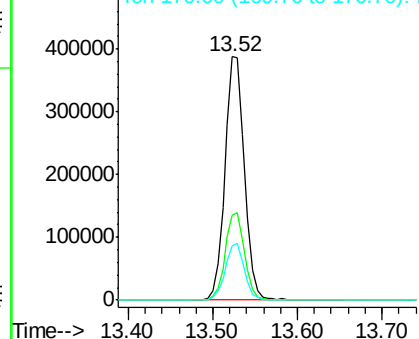

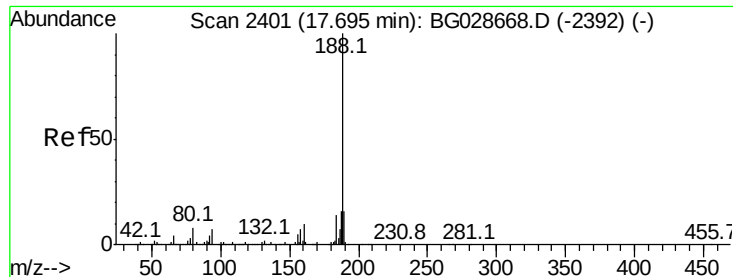

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.66 min Scan# 2395

Delta R.T. -0.04 min

Lab File: BG028846.D

Acq: 21 Sep 2017 7:09

Instrument :

BNA_G

ClientSampleId :

SP-A-COMP


Tot Ion:188 Resp: 262497

Ion Ratio Lower Upper

188 100

94 6.7 5.8 8.8




80 7.4 7.5 11.3#

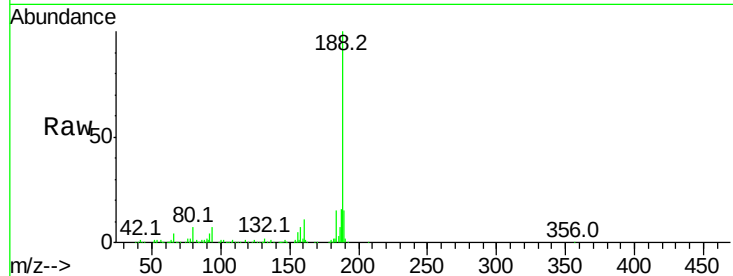

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

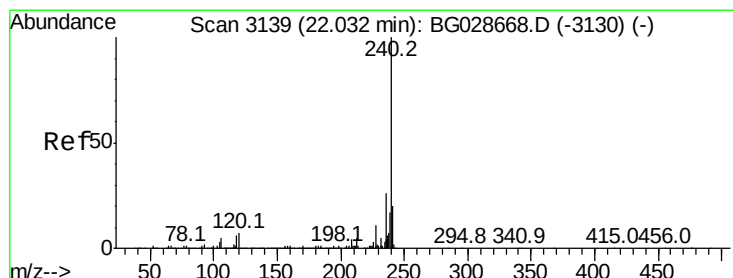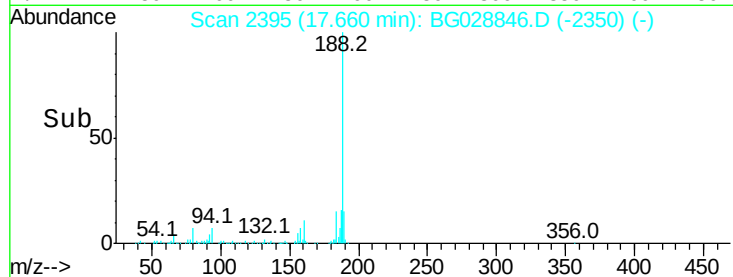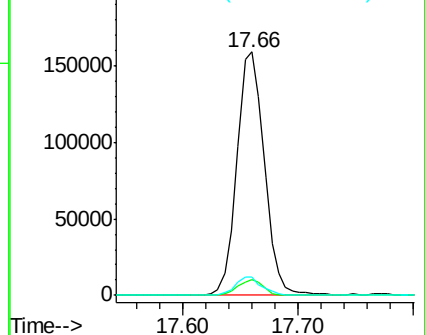

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.98 min Scan# 3131

Delta R.T. -0.05 min

Lab File: BG028846.D

Acq: 21 Sep 2017 7:09


Tgt Ion:240 Resp: 285009

Ion Ratio Lower Upper

240 100

120 6.3 5.7 8.5



236 25.3 22.2 33.4

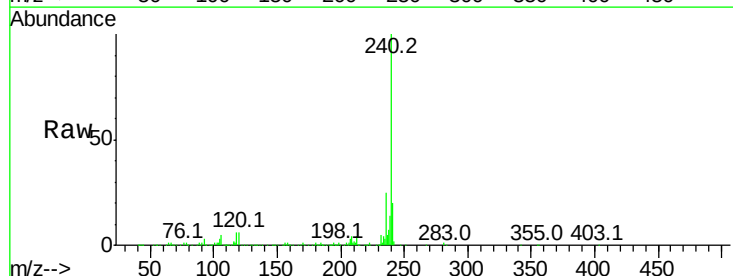


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

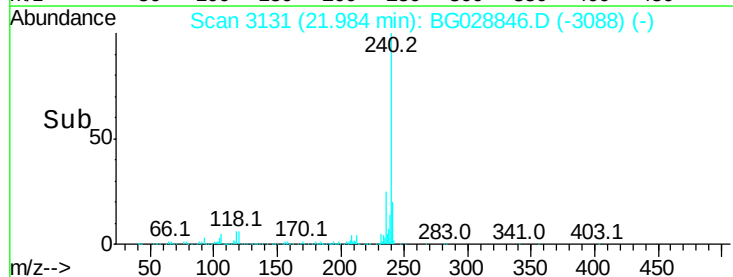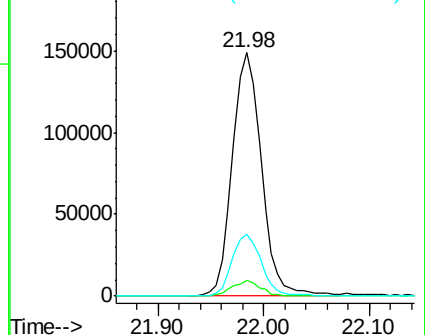

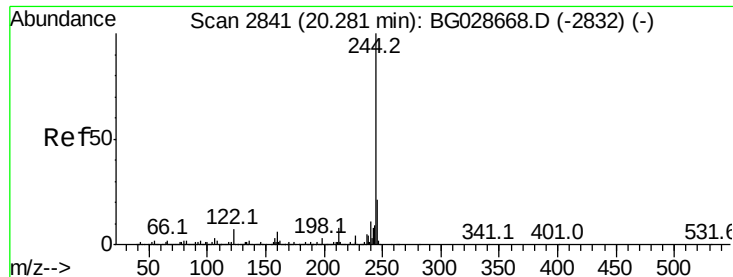

#78

Terphenyl-d14

Concen: 89.961 ng

RT: 20.24 min Scan# 2835

Delta R.T. -0.04 min

Lab File: BG028846.D

Acq: 21 Sep 2017 7:09

Instrument :

BNA_G

ClientSampleId :

SP-A-COMP


Tot Ion:244 Resp: 1202289

Ion Ratio Lower Upper

244 100

212 7.9 10.0 15.0#




122 7.5 8.6 12.8#

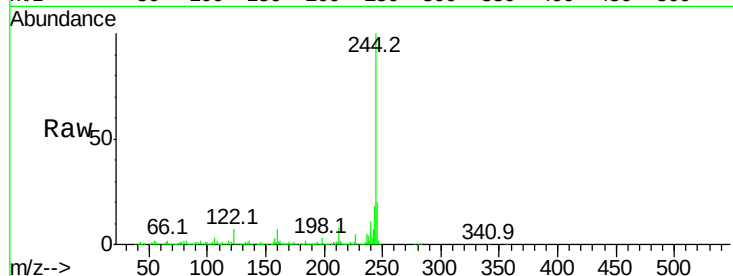

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

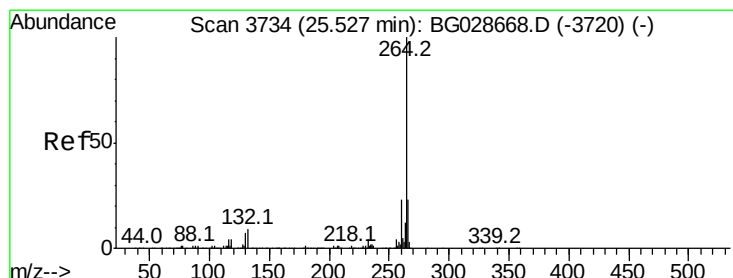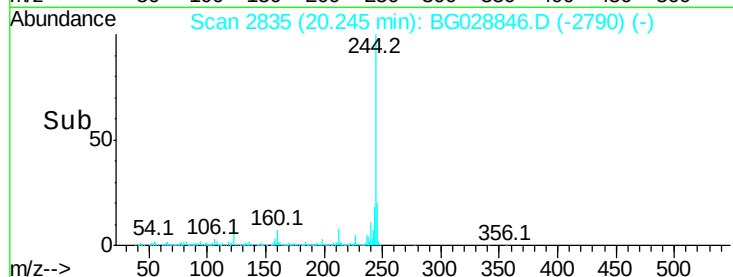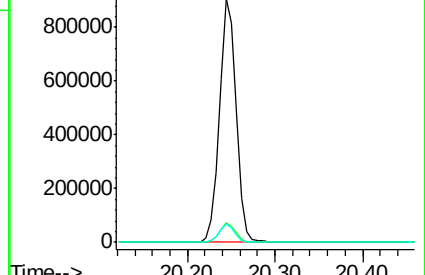

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.46 min Scan# 3722

Delta R.T. -0.07 min

Lab File: BG028846.D

Acq: 21 Sep 2017 7:09


Tgt Ion:264 Resp: 273870

Ion Ratio Lower Upper

264 100

260 23.5 21.8 32.8

265 19.7 18.2 27.4

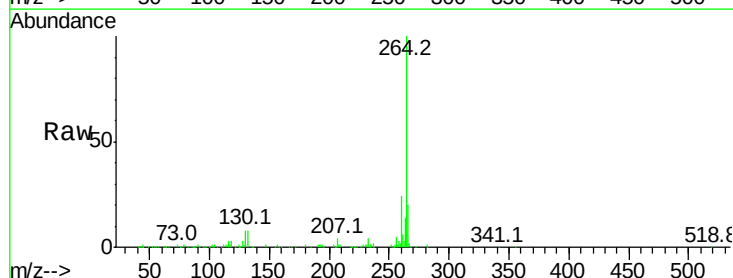

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

