


Data Path : Z:\HPCHEM1\BNA G\DATA\BG092017\
 Data File : BG028823.D
 Acq On : 20 Sep 2017 8:38
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 21 12:57:55 2017

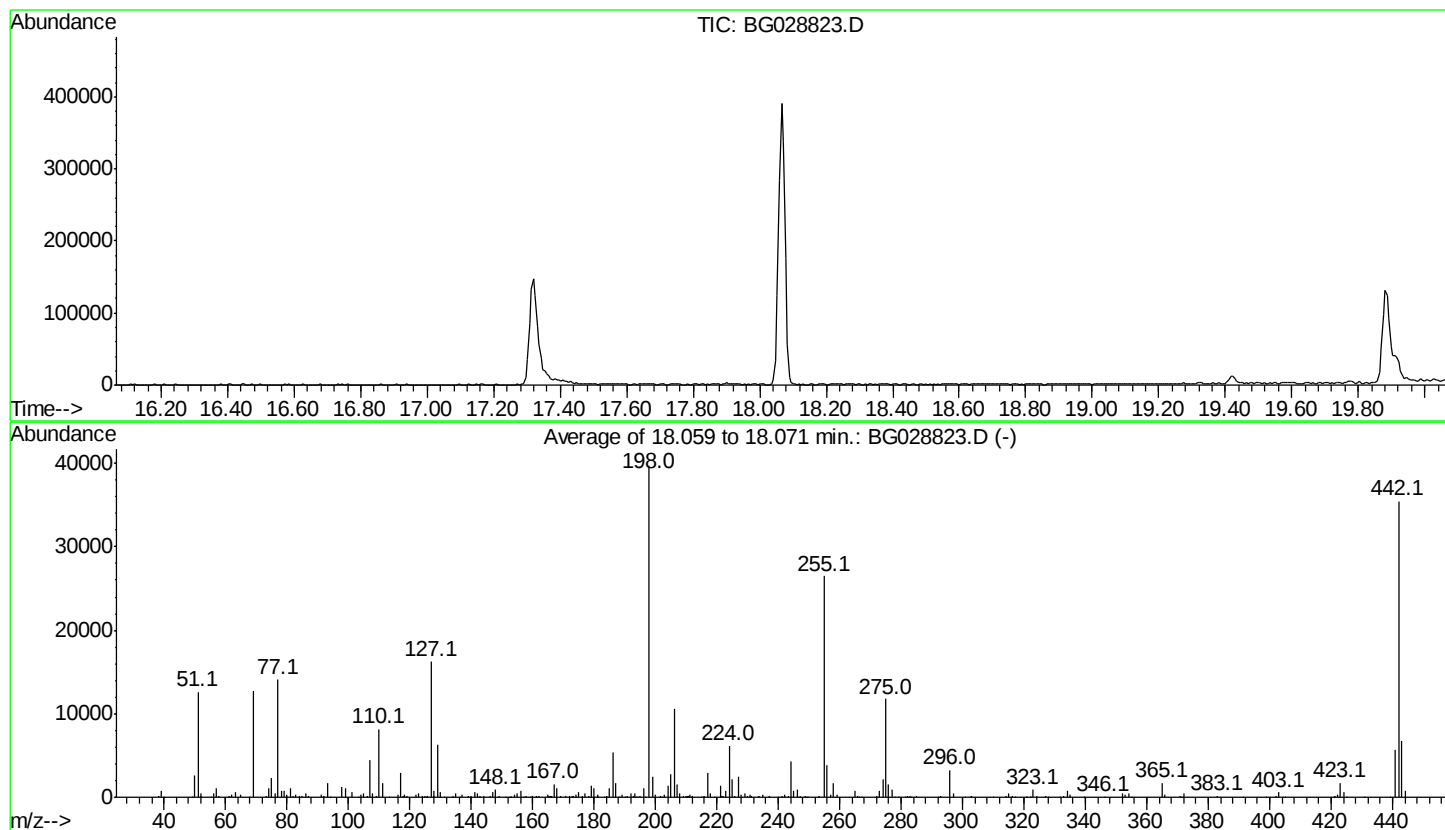

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.8	12640	PASS
68	69	0.00	2	0.6	79	PASS
69	198	0.00	100	32.1	12762	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.9	16250	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	39728	PASS
199	198	5	9	6.3	2516	PASS
275	198	10	60	29.6	11742	PASS
365	198	1	100	4.3	1716	PASS
441	442	0.01	24	16.2	5743	PASS
442	198	50	100	89.4	35506	PASS
443	442	15	24	19.2	6826	PASS