


Data Path : Z:\HPCHEM1\BNA G\DATA\BG092017\
 Data File : BG028842.D
 Acq On : 21 Sep 2017 4:30
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 21 12:57:55 2017

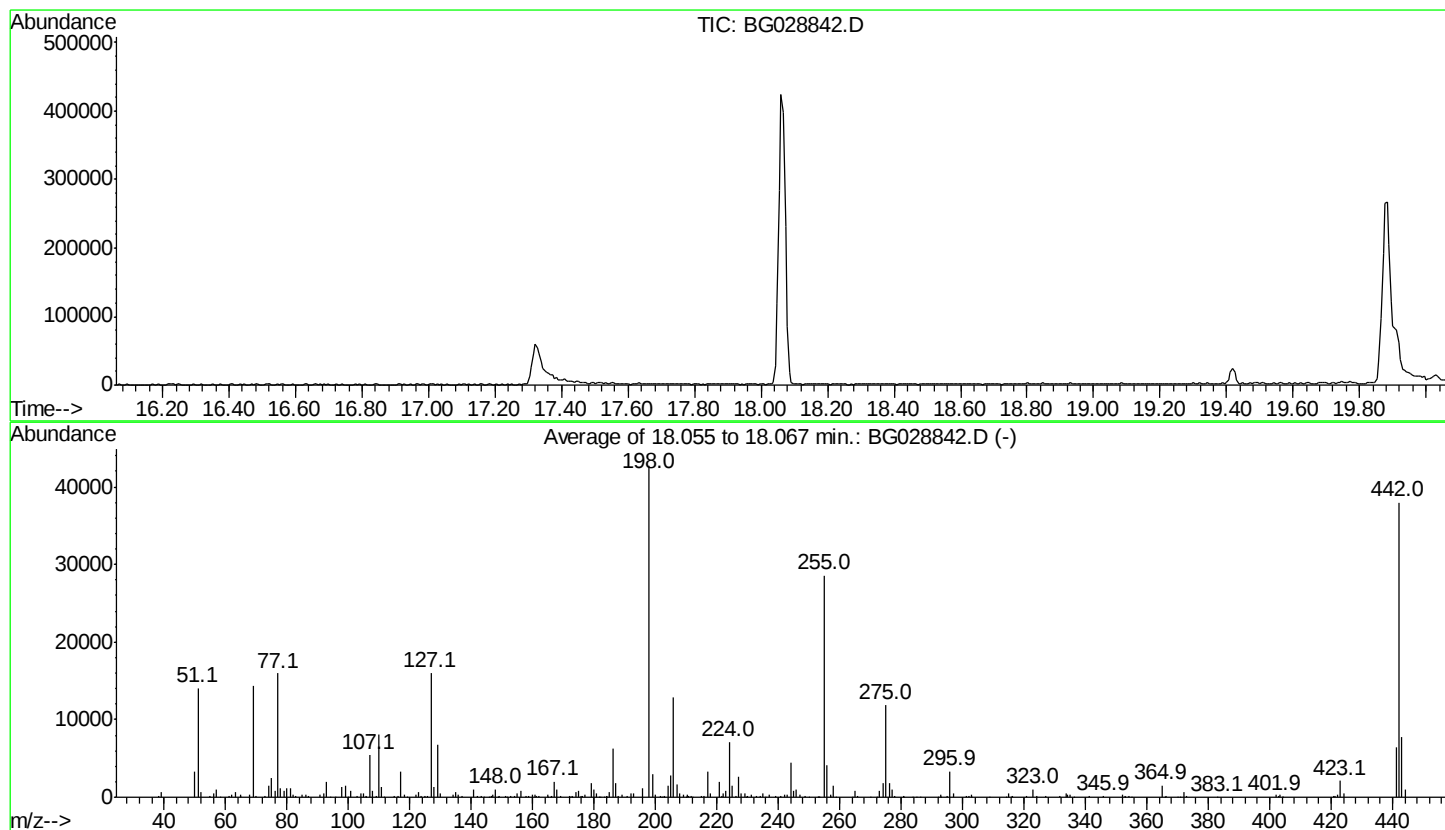

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.9	14058	PASS
68	69	0.00	2	1.9	277	PASS
69	198	0.00	100	33.5	14305	PASS
70	69	0.00	2	0.8	119	PASS
127	198	10	80	37.6	16071	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	42738	PASS
199	198	5	9	6.9	2952	PASS
275	198	10	60	28.0	11954	PASS
365	198	1	100	3.6	1554	PASS
441	442	0.01	24	16.9	6430	PASS
442	198	50	100	88.9	38008	PASS
443	442	15	24	20.3	7705	PASS