


Data Path : Z:\HPCHEM1\BNA G\DATA\BG092115\
Data File : BG018797.D
Acq On : 22 Sep 2015 00:20
Operator : TP
Sample : G3696-18
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AP2

Quant Time: Sep 22 02:53:16 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG091015.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 22 02:06:40 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
9/22/2015 2:14:50 PM

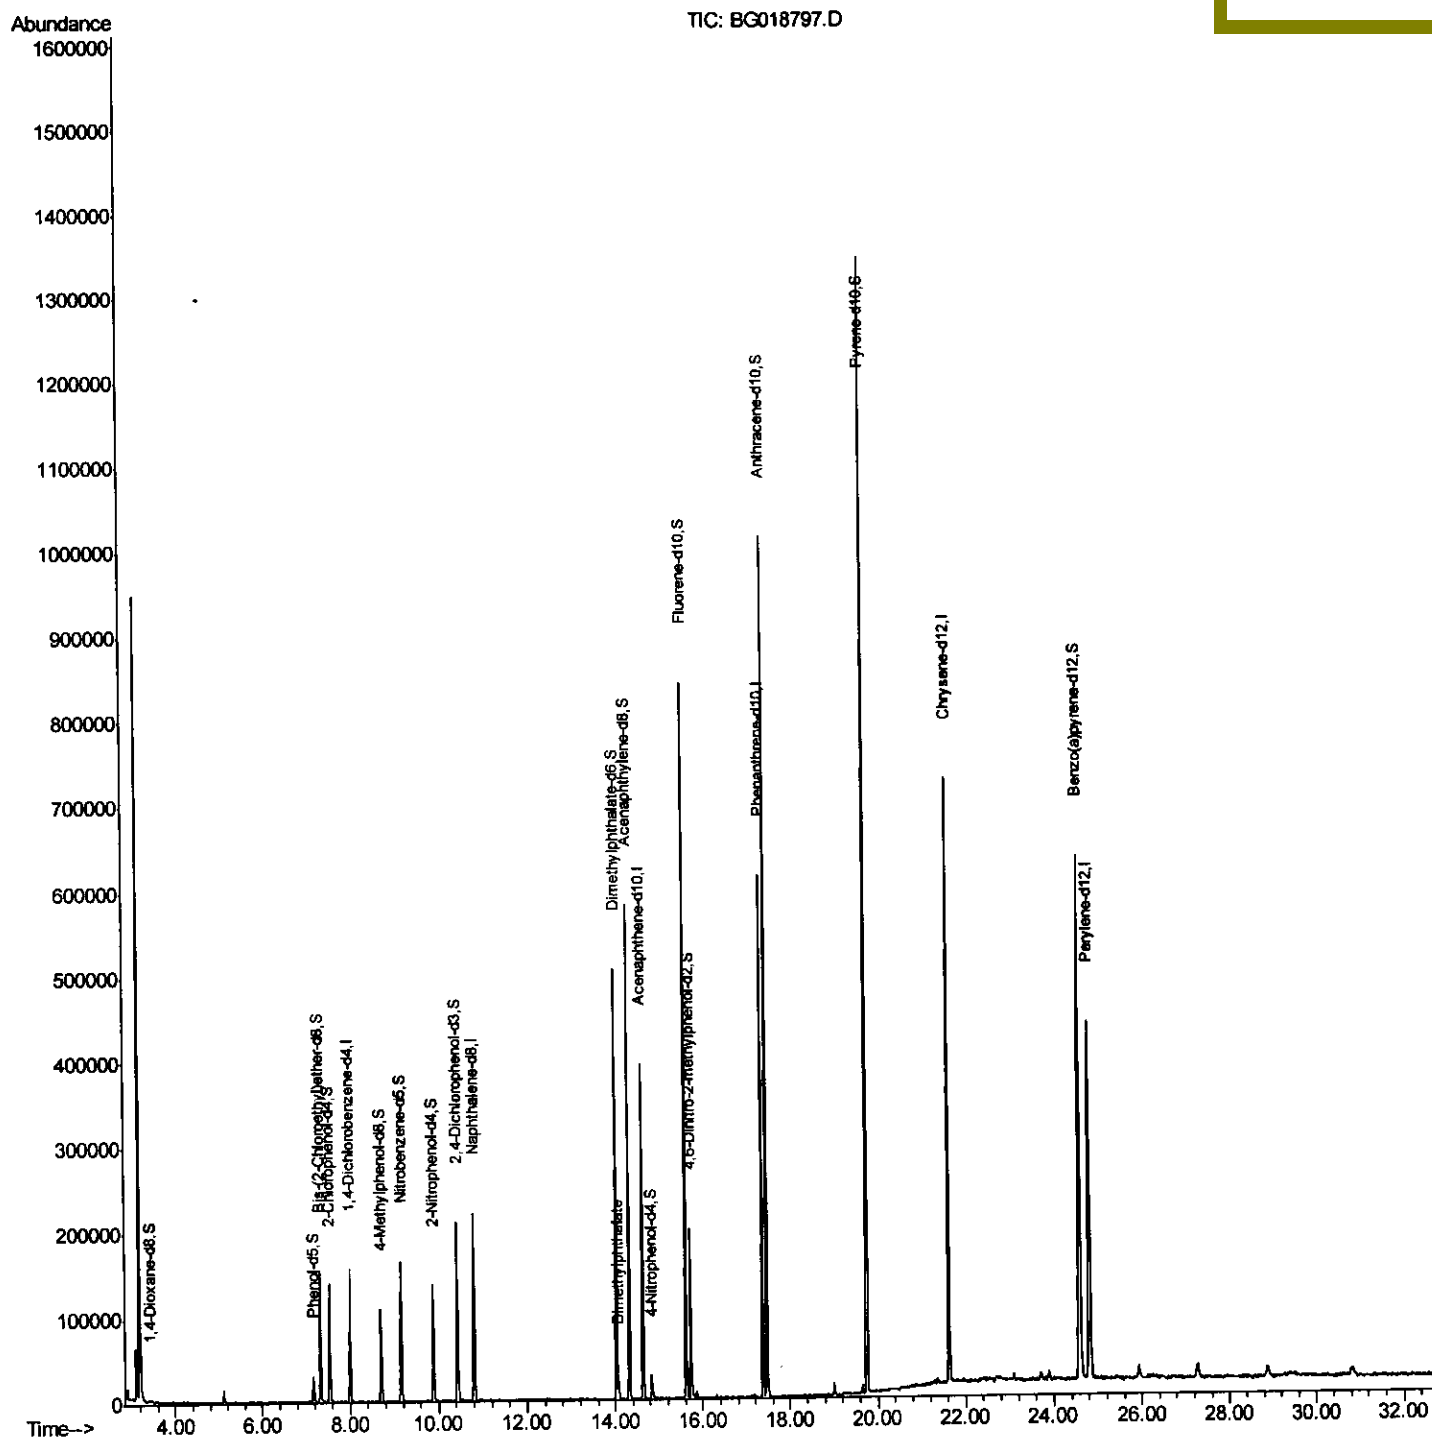

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA G\DATA\BG092115\
 Data File : BG018797.D
 Acq On : 22 Sep 2015 00:20
 Operator : TP
 Sample : G3696-18
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AP2

Quant Time: Sep 22 02:09:43 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG091015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 22 02:06:40 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 9/22/2015 2:14:50 PM

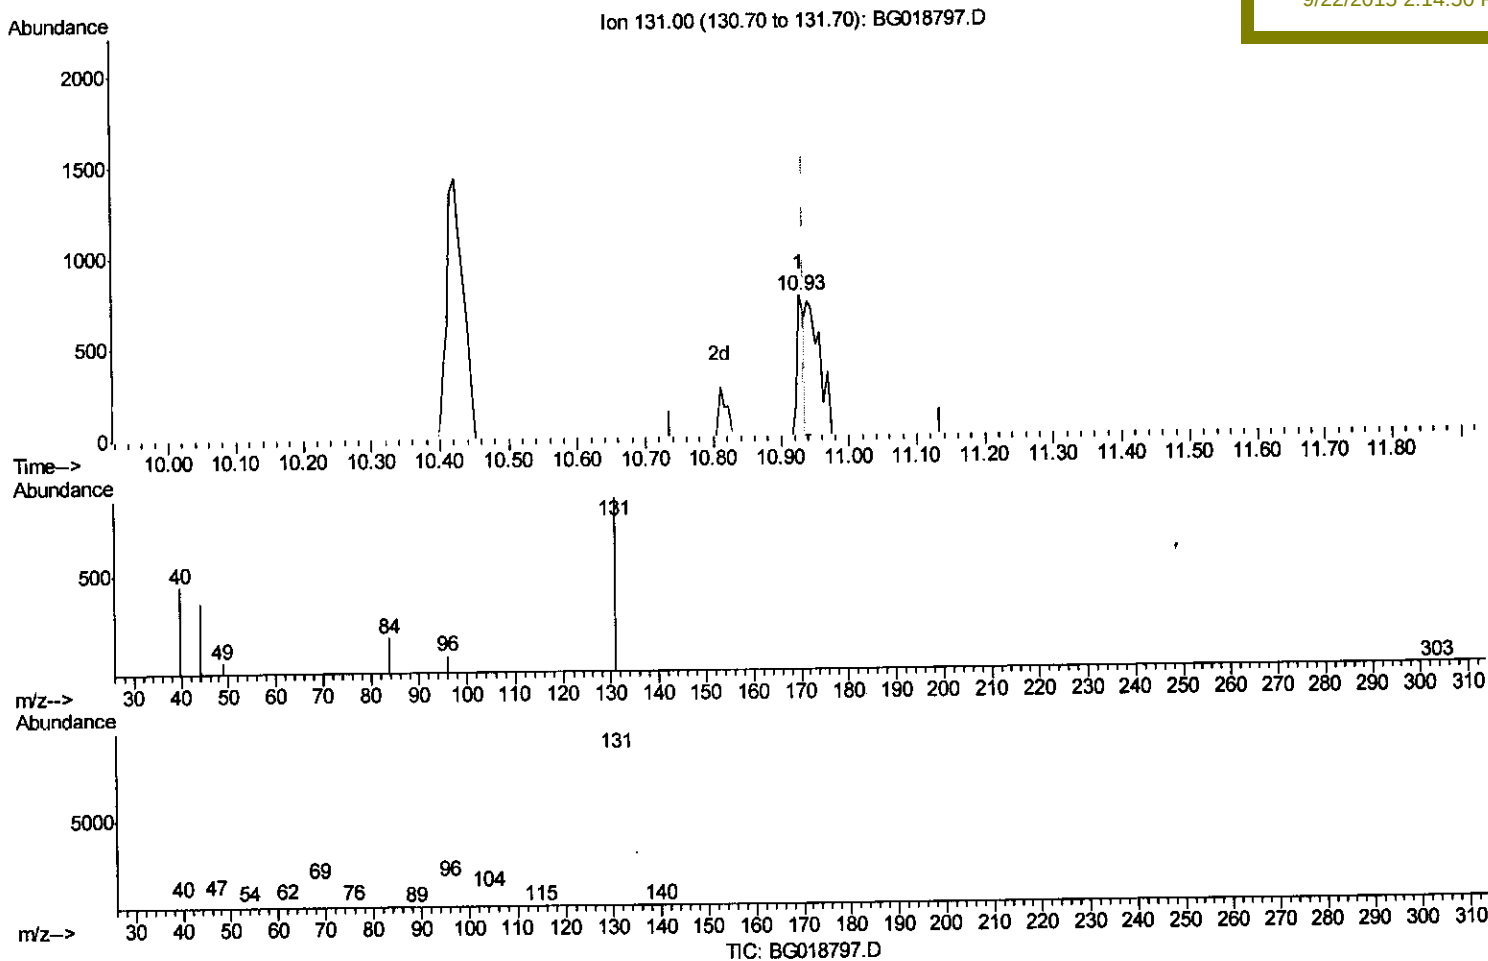

(29) 4-Chloroaniline-d4 (S)

10.928min (-0.008) 0.15ng/ul

response 555

Ion	Exp%	Act%
131.00	100	100
133.00	32.00	0.00#
69.00	18.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA G\DATA\BG092115\
 Data File : BG018797.D
 Acq On : 22 Sep 2015 00:20
 Operator : TP
 Sample : G3696-18
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AP2

Quant Time: Sep 22 02:09:43 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG091015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 22 02:06:40 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 9/22/2015 2:14:50 PM

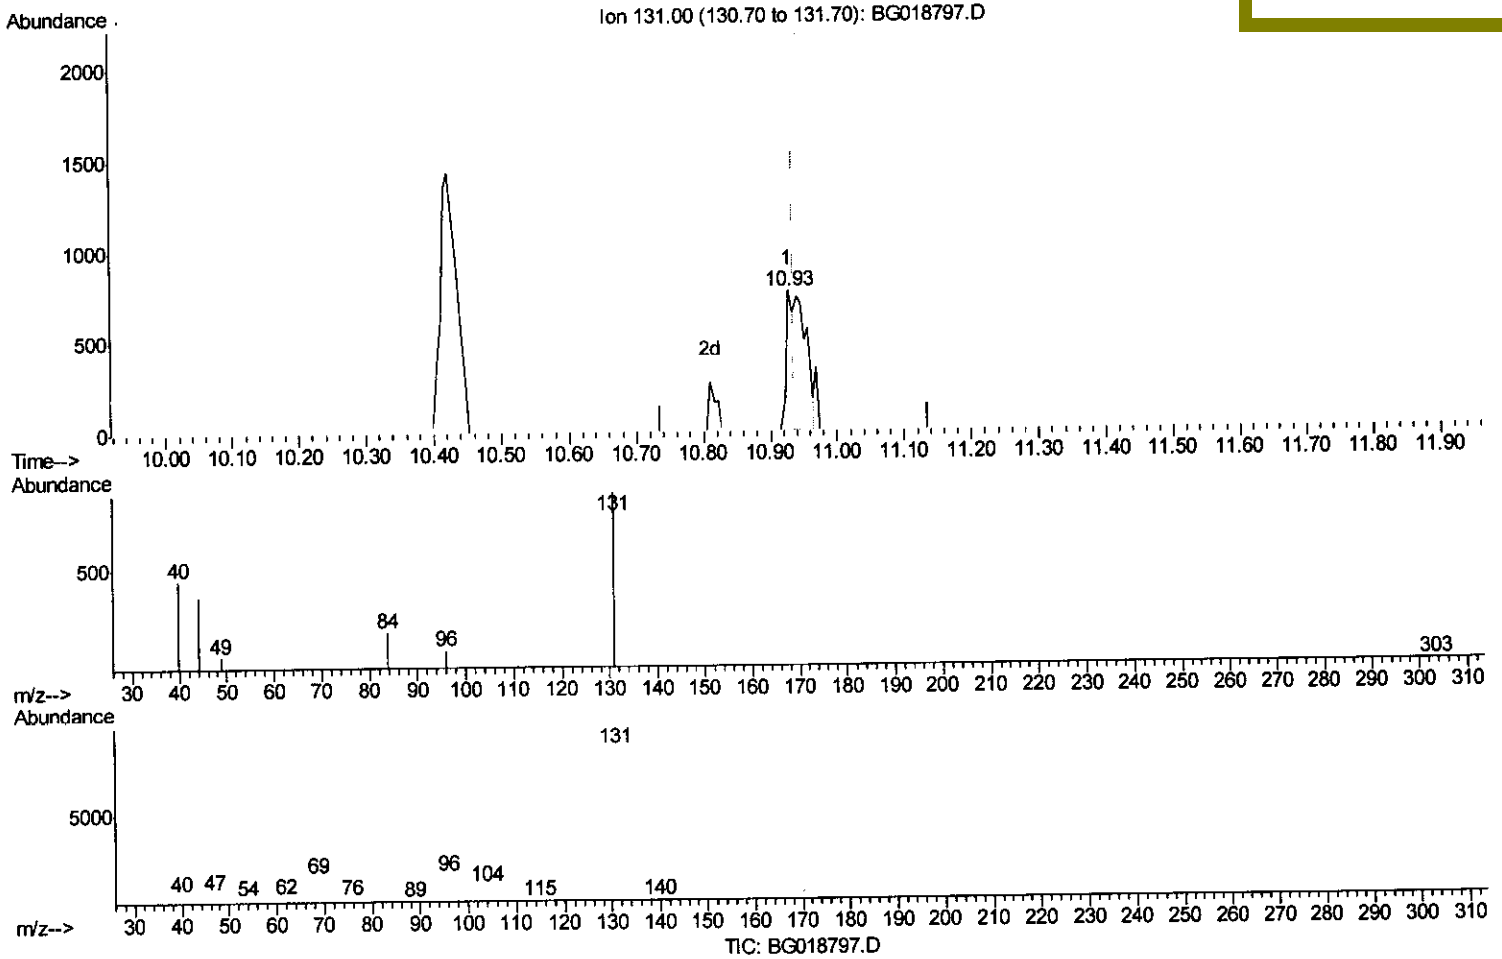

(29) 4-Chloroaniline-d4 (S)

10.928min (-0.008) 0.39ng/ul m

response 1491

Ion Exp% Act%

131.00	100	100
133.00	32.00	0.00#
69.00	18.90	0.00#
0.00	0.00	0.00

T.P
 9/23/15

Data Path : Z:\HPCHEM1\BNA G\DATA\BG092115\
 Data File : BG018797.D
 Acq On : 22 Sep 2015 00:20
 Operator : TP
 Sample : G3696-18
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AP2

Quant Time: Sep 22 02:53:16 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG091015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 22 02:06:40 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 9/22/2015 2:14:50 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.00	152	49839	20.00	ng/ul	0.00
18) Naphthalene-d8	10.80	136	204346	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.62	164	139904	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.37	188	381055	20.00	ng/ul	0.00
78) Chrysene-d12	21.63	240	434299	20.00	ng/ul	0.00
86) Perylene-d12	24.81	264	434430	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.44	96	1042	1.01	ng/uL	0.00
5) Phenol-d5	7.17	99	22229	5.43	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.32	67	71069	29.97	ng/ul	0.00
9) 2-Chlorophenol-d4	7.53	132	75314	24.30	ng/ul	0.00
13) 4-Methylphenol-d8	8.71	113	47186	14.21	ng/ul	0.00
19) Nitrobenzene-d5	9.16	128	51098	33.01	ng/ul	0.00
22) 2-Nitrophenol-d4	9.88	143	53437	34.32	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.42	165	91646	27.96	ng/ul	0.00
29) 4-Chloroaniline-d4	10.93	131	1491m	0.39	ng/ul	0.00
44) Dimethylphthalate-d6	14.02	166	384526	34.15	ng/ul	0.00
47) Acenaphthylene-d8	14.32	160	445417	33.38	ng/ul	0.00
52) 4-Nitrophenol-d4	14.83	143	10070	4.66	ng/ul	0.00
58) Fluorene-d10	15.62	176	341739	34.71	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.73	200	54946	30.46	ng/ul	0.00
71) Anthracene-d10	17.47	188	600270	35.78	ng/ul	0.00
79) Pyrene-d10	19.75	212	706436	35.36	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.59	264	654017	30.93	ng/ul	0.00

Target Compounds				Ovalue
45) Dimethylphthalate	14.07	163	13230	1.21 ng/ul# 94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

T.P
 9/23/15