

Data Path : Z:\HPCHEM1\BNA G\DATA\BG092115\
 Data File : BG018783.D
 Acq On : 21 Sep 2015 15:28
 Operator : TP
 Sample : G3696-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AP4

Quant Time: Sep 21 16:26:24 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG091015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 21 15:50:58 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.00	152	42411	20.00	ng/ul	0.00
18) Naphthalene-d8	10.80	136	179185	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.63	164	126306	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.37	188	360957	20.00	ng/ul	0.00
78) Chrysene-d12	21.63	240	435796	20.00	ng/ul	-0.01
86) Perylene-d12	24.82	264	439358	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.44	96	860	0.97	ng/uL	0.00
5) Phenol-d5	7.17	99	16619	4.77	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.32	67	42383	21.00	ng/ul	0.00
9) 2-Chlorophenol-d4	7.53	132	45082	17.09	ng/ul	0.00
13) 4-Methylphenol-d8	8.71	113	30325	10.73	ng/ul	0.00
19) Nitrobenzene-d5	9.16	128	27750	20.44	ng/ul	0.00
22) 2-Nitrophenol-d4	9.88	143	30203	22.12	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.42	165	54766	19.05	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	6267	1.87	ng/ul	0.00
44) Dimethylphthalate-d6	14.02	166	231905	22.81	ng/ul	0.00
47) Acenaphthylene-d8	14.32	160	258366	21.45	ng/ul	0.00
52) 4-Nitrophenol-d4	14.84	143	8169	4.19	ng/ul	0.00
58) Fluorene-d10	15.62	176	199861	22.49	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.73	200	28102	16.45	ng/ul	0.00
71) Anthracene-d10	17.47	188	349661	22.00	ng/ul	0.00
79) Pyrene-d10	19.75	212	417945	20.85	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.59	264	357628	16.73	ng/ul	-0.03


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.07	163	36391	3.69	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG092115\
Data File : BG018783.D
Acq On : 21 Sep 2015 15:28
Operator : TP
Sample : G3696-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AP4

Quant Time: Sep 21 16:26:24 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG091015.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 21 15:50:58 2015
Response via : Initial Calibration

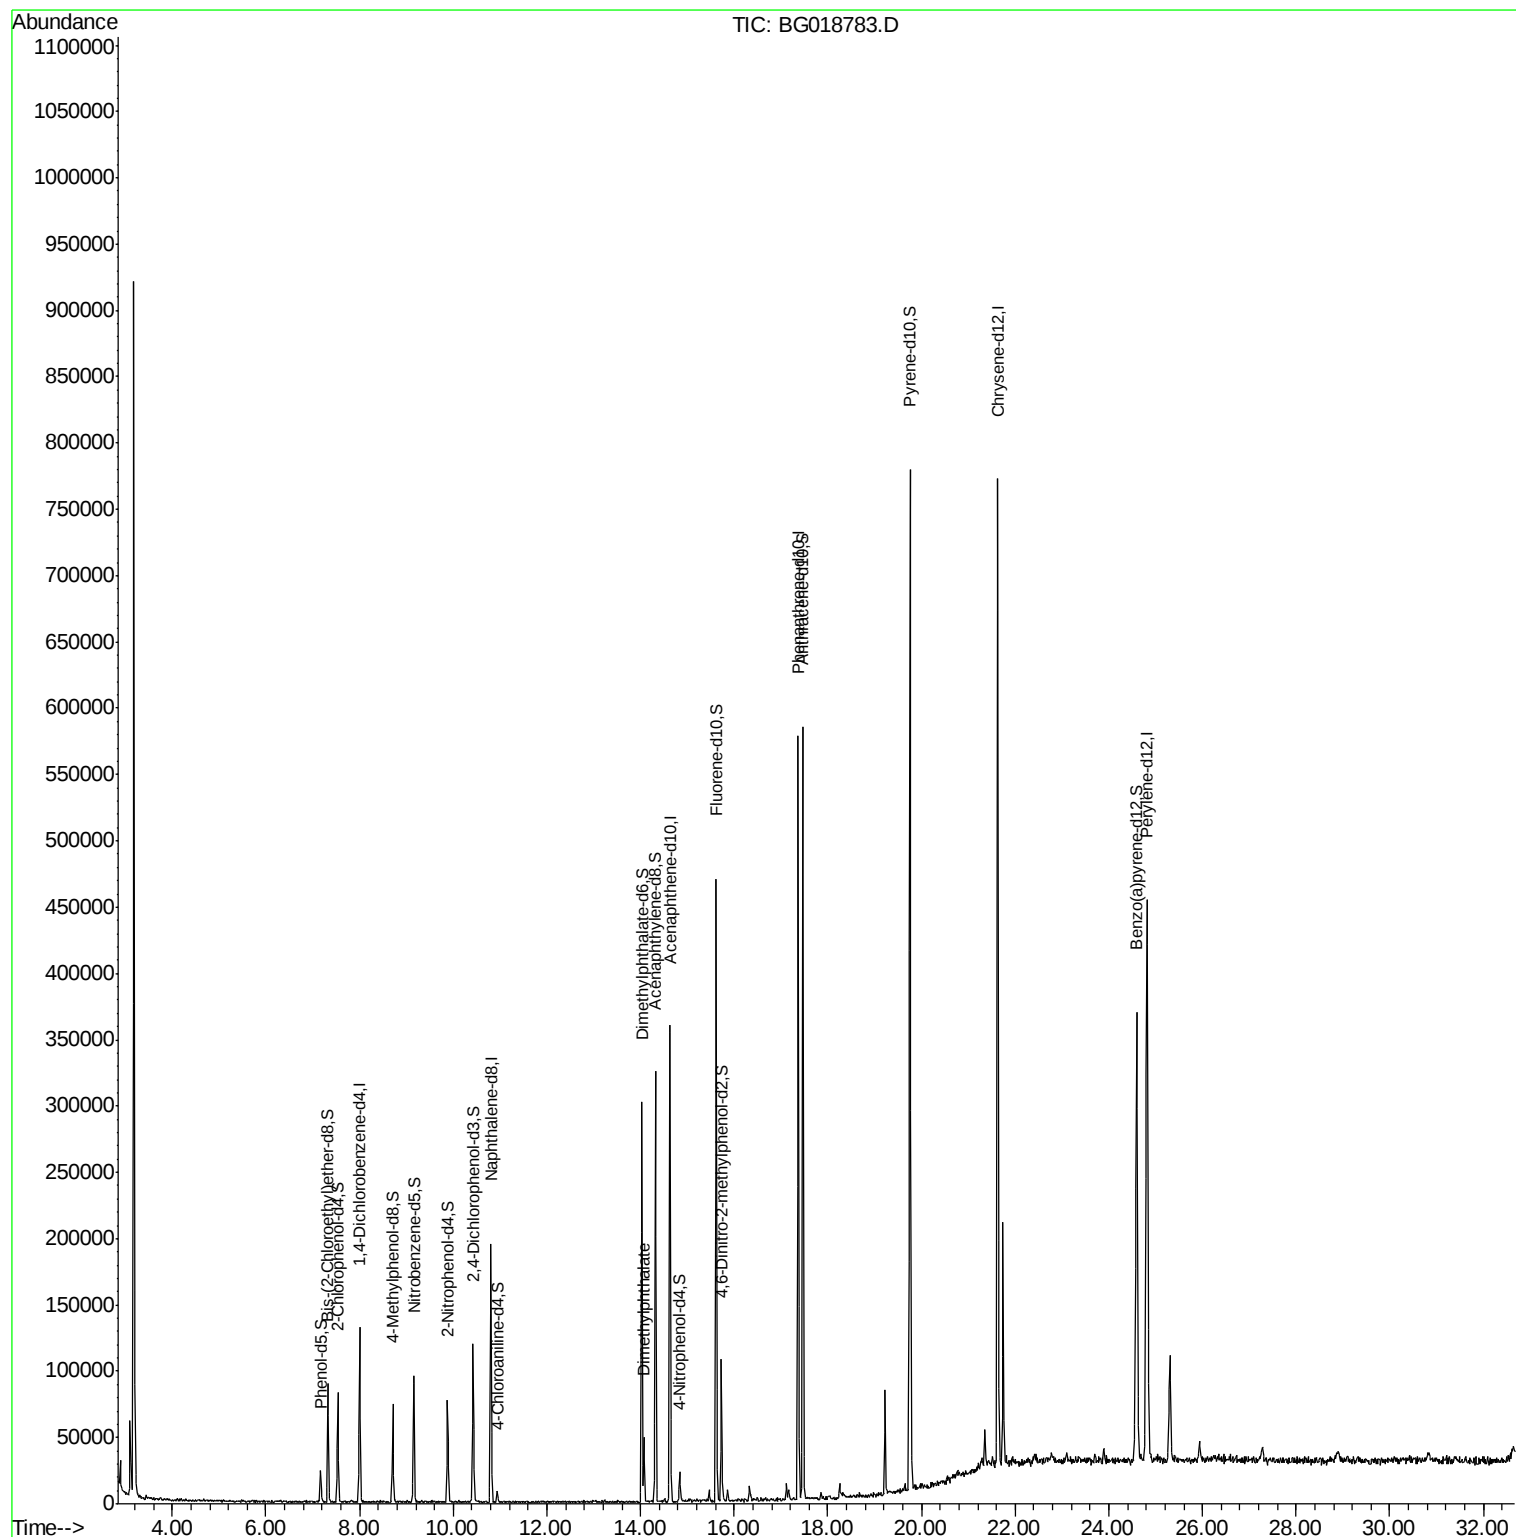

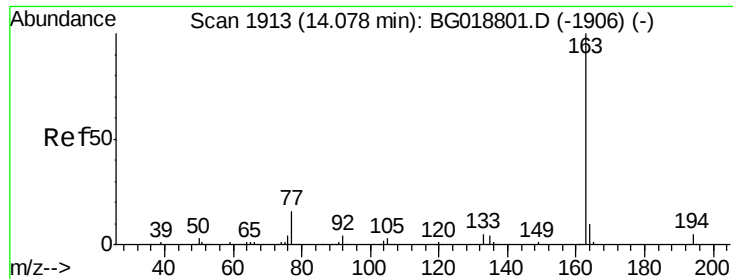

#45

Dimethylphthalate

Concen: 3.69 ng/ul

RT: 14.07 min Scan# 1912

Delta R.T. -0.01 min

Lab File: BG018783.D

Acq: 21 Sep 2015 15:28

Instrument :

BNA_G

ClientSampleId :

C0AP4


Tot Ion:163 Resp: 36391

Ion Ratio Lower Upper

163 100

194 3.8 2.9 4.3

164 9.8 7.7 11.5

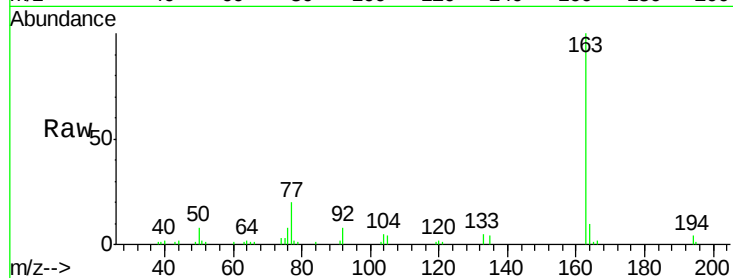

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

