

Data Path : Z:\HPCHEM1\BNA G\DATA\BG092115\
 Data File : BG018784.D
 Acq On : 21 Sep 2015 16:06
 Operator : TP
 Sample : G3696-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AQ6

Manual Integrations
 APPROVED

MMDadoda
 9/22/2015 2:14:15 PM

Quant Time: Sep 21 16:44:14 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG091015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 21 15:50:58 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.00	152	41821	20.00	ng/ul	0.00
18) Naphthalene-d8	10.80	136	180846	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.62	164	124066	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.37	188	367914	20.00	ng/ul	0.00
78) Chrysene-d12	21.63	240	420421	20.00	ng/ul	-0.01
86) Perylene-d12	24.81	264	424794	20.00	ng/ul	-0.03

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.44	96	1341	1.54	ng/uL	0.00
5) Phenol-d5	7.16	99	22525	6.56	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.32	67	63685	32.00	ng/ul	0.00
9) 2-Chlorophenol-d4	7.53	132	68842	26.47	ng/ul	0.00
13) 4-Methylphenol-d8	8.71	113	45624	16.37	ng/ul	0.00
19) Nitrobenzene-d5	9.16	128	46213	33.73	ng/ul	0.00
22) 2-Nitrophenol-d4	9.88	143	48685	35.34	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.42	165	84928	29.27	ng/ul	0.00
29) 4-Chloroaniline-d4	10.93	131	1174m	0.35	ng/ul	0.00
44) Dimethylphthalate-d6	14.03	166	364720	36.53	ng/ul	0.00
47) Acenaphthylene-d8	14.32	160	399692	33.78	ng/ul	0.00
52) 4-Nitrophenol-d4	14.83	143	11861	6.19	ng/ul	0.00
58) Fluorene-d10	15.62	176	311752	35.71	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.73	200	50347	28.91	ng/ul	0.00
71) Anthracene-d10	17.47	188	556619	34.36	ng/ul	0.00
79) Pyrene-d10	19.75	212	673148	34.80	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.60	264	512404	24.79	ng/ul	-0.03

Target Compounds					Ovalue
45) Dimethylphthalate	14.07	163	11625	1.20 ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG092115\
Data File : BG018784.D
Acq On : 21 Sep 2015 16:06
Operator : TP
Sample : G3696-04
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
C0AQ6

Manual Integrations
APPROVED

MMDadoda
9/22/2015 2:14:15 PM

Quant Time: Sep 21 16:44:14 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG091015.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 21 15:50:58 2015
Response via : Initial Calibration

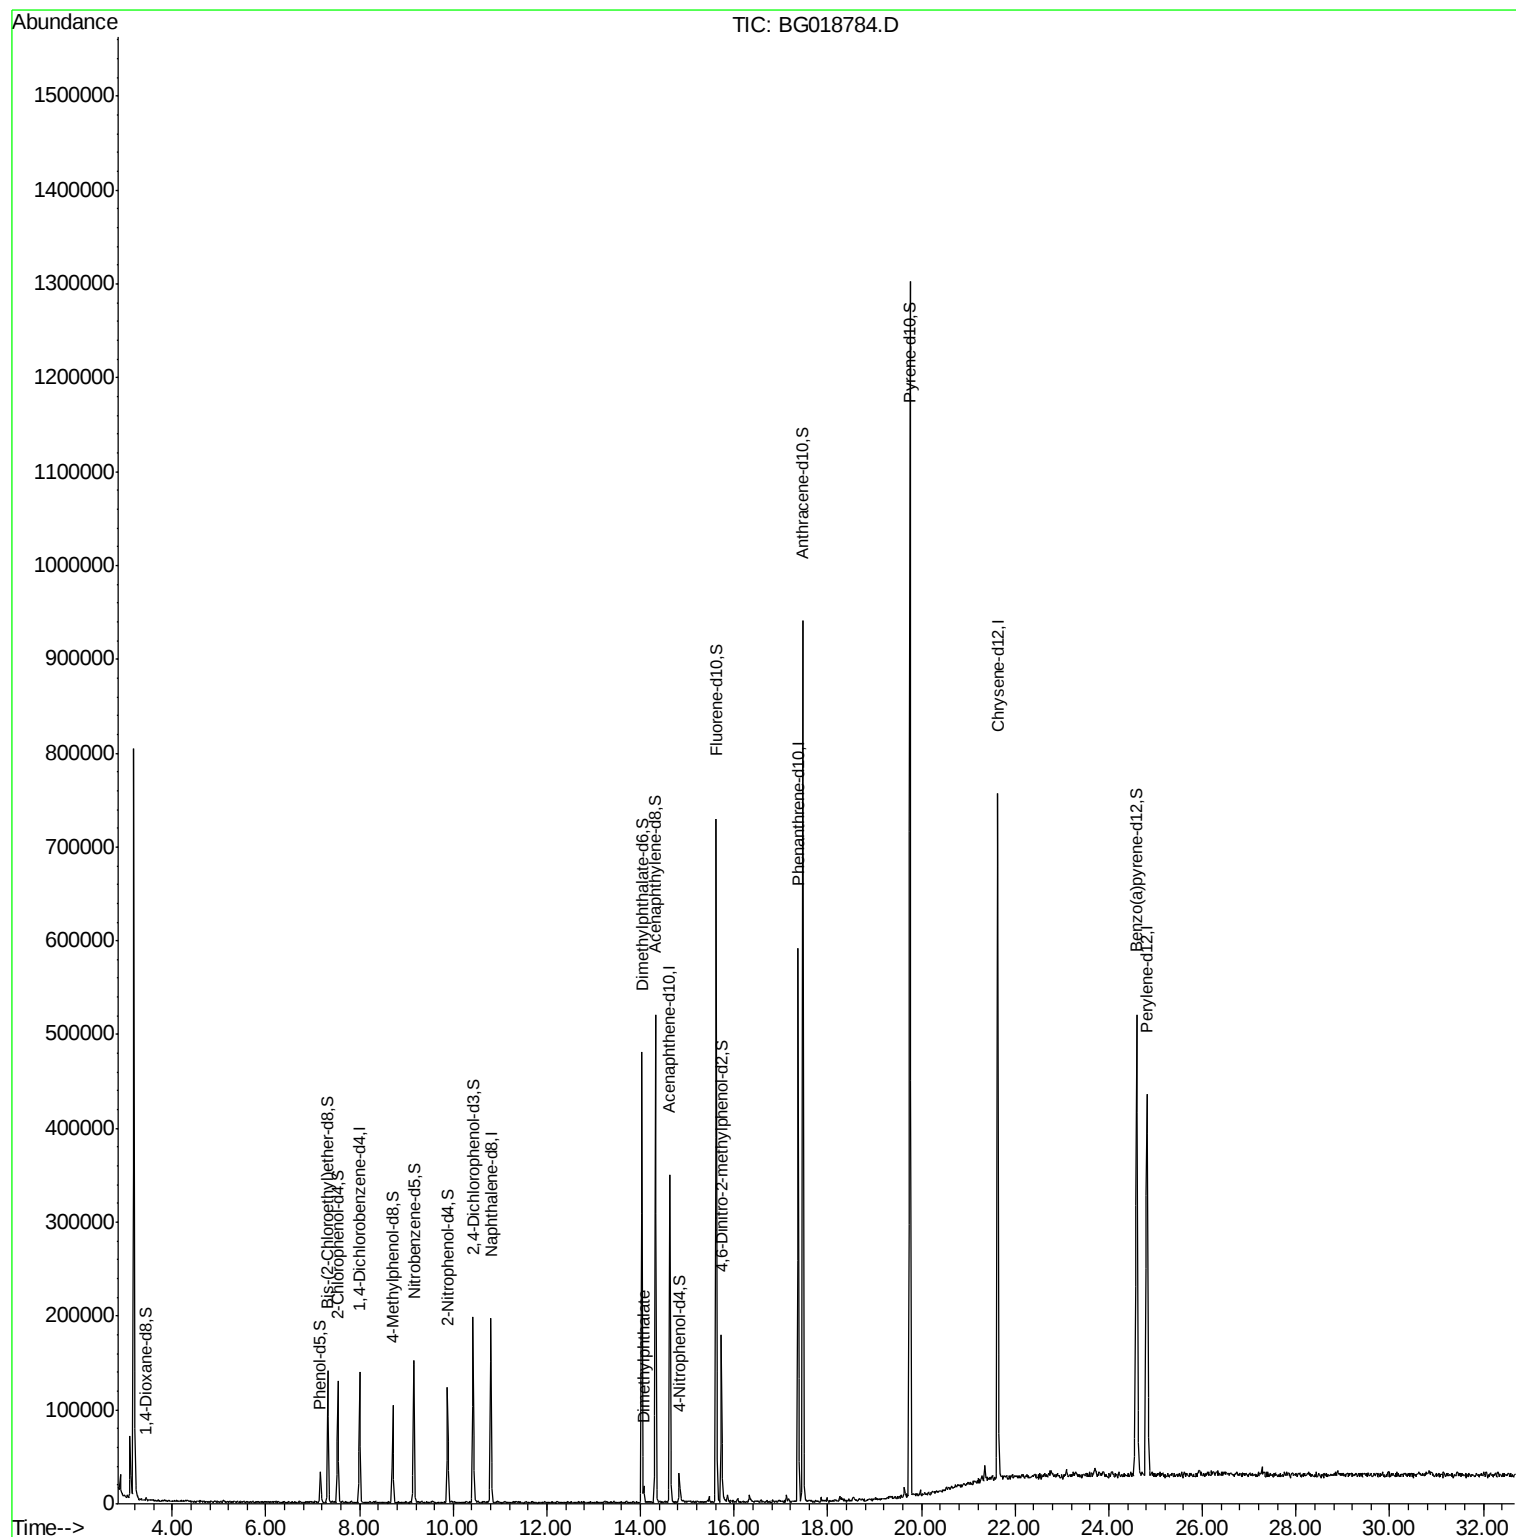

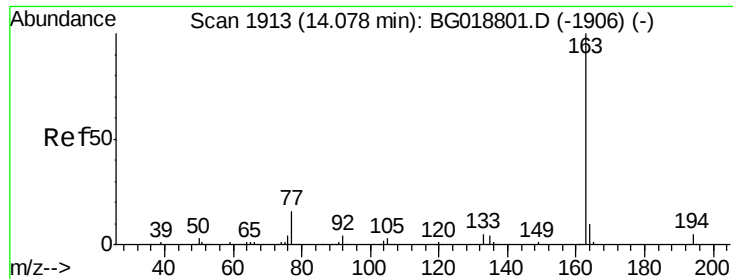


#45
 Dimethylphthalate
 Concen: 1.20 ng/ul
 RT: 14.07 min Scan# 1912
 Delta R.T. -0.01 min
 Lab File: BG018784.D
 Acq: 21 Sep 2015 16:06

Instrument :
 BNA_G
 ClientSampleId :
 C0AQ6

Tot Ion	Ratio	Resp Lower	Resp Upper
163	100		
194	3.7	2.9	4.3
164	8.7	7.7	11.5

Manual Integrations
 APPROVED

MMDadoda
 9/22/2015 2:14:15 PM

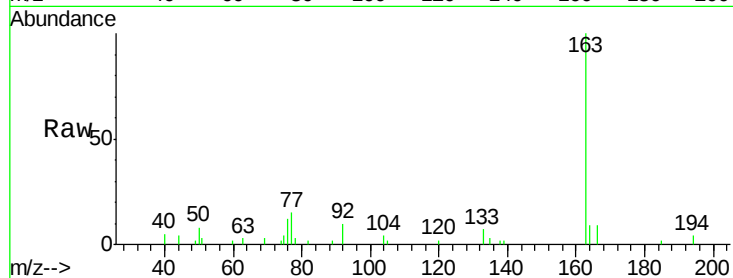

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

