

Data Path : Z:\HPCHEM1\BNA G\DATA\BG092115\
 Data File : BG018789.D
 Acq On : 21 Sep 2015 19:17
 Operator : TP
 Sample : G3696-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AR1

Quant Time: Sep 22 02:08:50 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG091015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 22 02:06:40 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.00	152	45032	20.00	ng/ul	0.00
18) Naphthalene-d8	10.80	136	200770	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.62	164	139291	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.37	188	383181	20.00	ng/ul	0.00
78) Chrysene-d12	21.63	240	424315	20.00	ng/ul	0.00
86) Perylene-d12	24.81	264	431673	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.44	96	1158	1.24	ng/uL	0.00
5) Phenol-d5	7.16	99	23426	6.34	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.32	67	62700	29.26	ng/ul	0.00
9) 2-Chlorophenol-d4	7.53	132	66723	23.82	ng/ul	0.00
13) 4-Methylphenol-d8	8.71	113	45039	15.01	ng/ul	0.00
19) Nitrobenzene-d5	9.16	128	44604	29.32	ng/ul	0.00
22) 2-Nitrophenol-d4	9.88	143	47976	31.37	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.42	165	83185	25.83	ng/ul	0.00
29) 4-Chloroaniline-d4	10.93	131	5960	1.59	ng/ul	0.00
44) Dimethylphthalate-d6	14.03	166	356910	31.84	ng/ul	0.00
47) Acenaphthylene-d8	14.32	160	405190	30.50	ng/ul	0.00
52) 4-Nitrophenol-d4	14.84	143	11961	5.56	ng/ul	0.00
58) Fluorene-d10	15.62	176	308648	31.49	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.73	200	47492	26.18	ng/ul	0.00
71) Anthracene-d10	17.47	188	530193	31.43	ng/ul	0.00
79) Pyrene-d10	19.75	212	628424	32.19	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.59	264	577894	27.51	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.07	163	37110	3.41	ng/ul	98




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG092115\
Data File : BG018789.D
Acq On : 21 Sep 2015 19:17
Operator : TP
Sample : G3696-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AR1

Quant Time: Sep 22 02:08:50 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG091015.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 22 02:06:40 2015
Response via : Initial Calibration

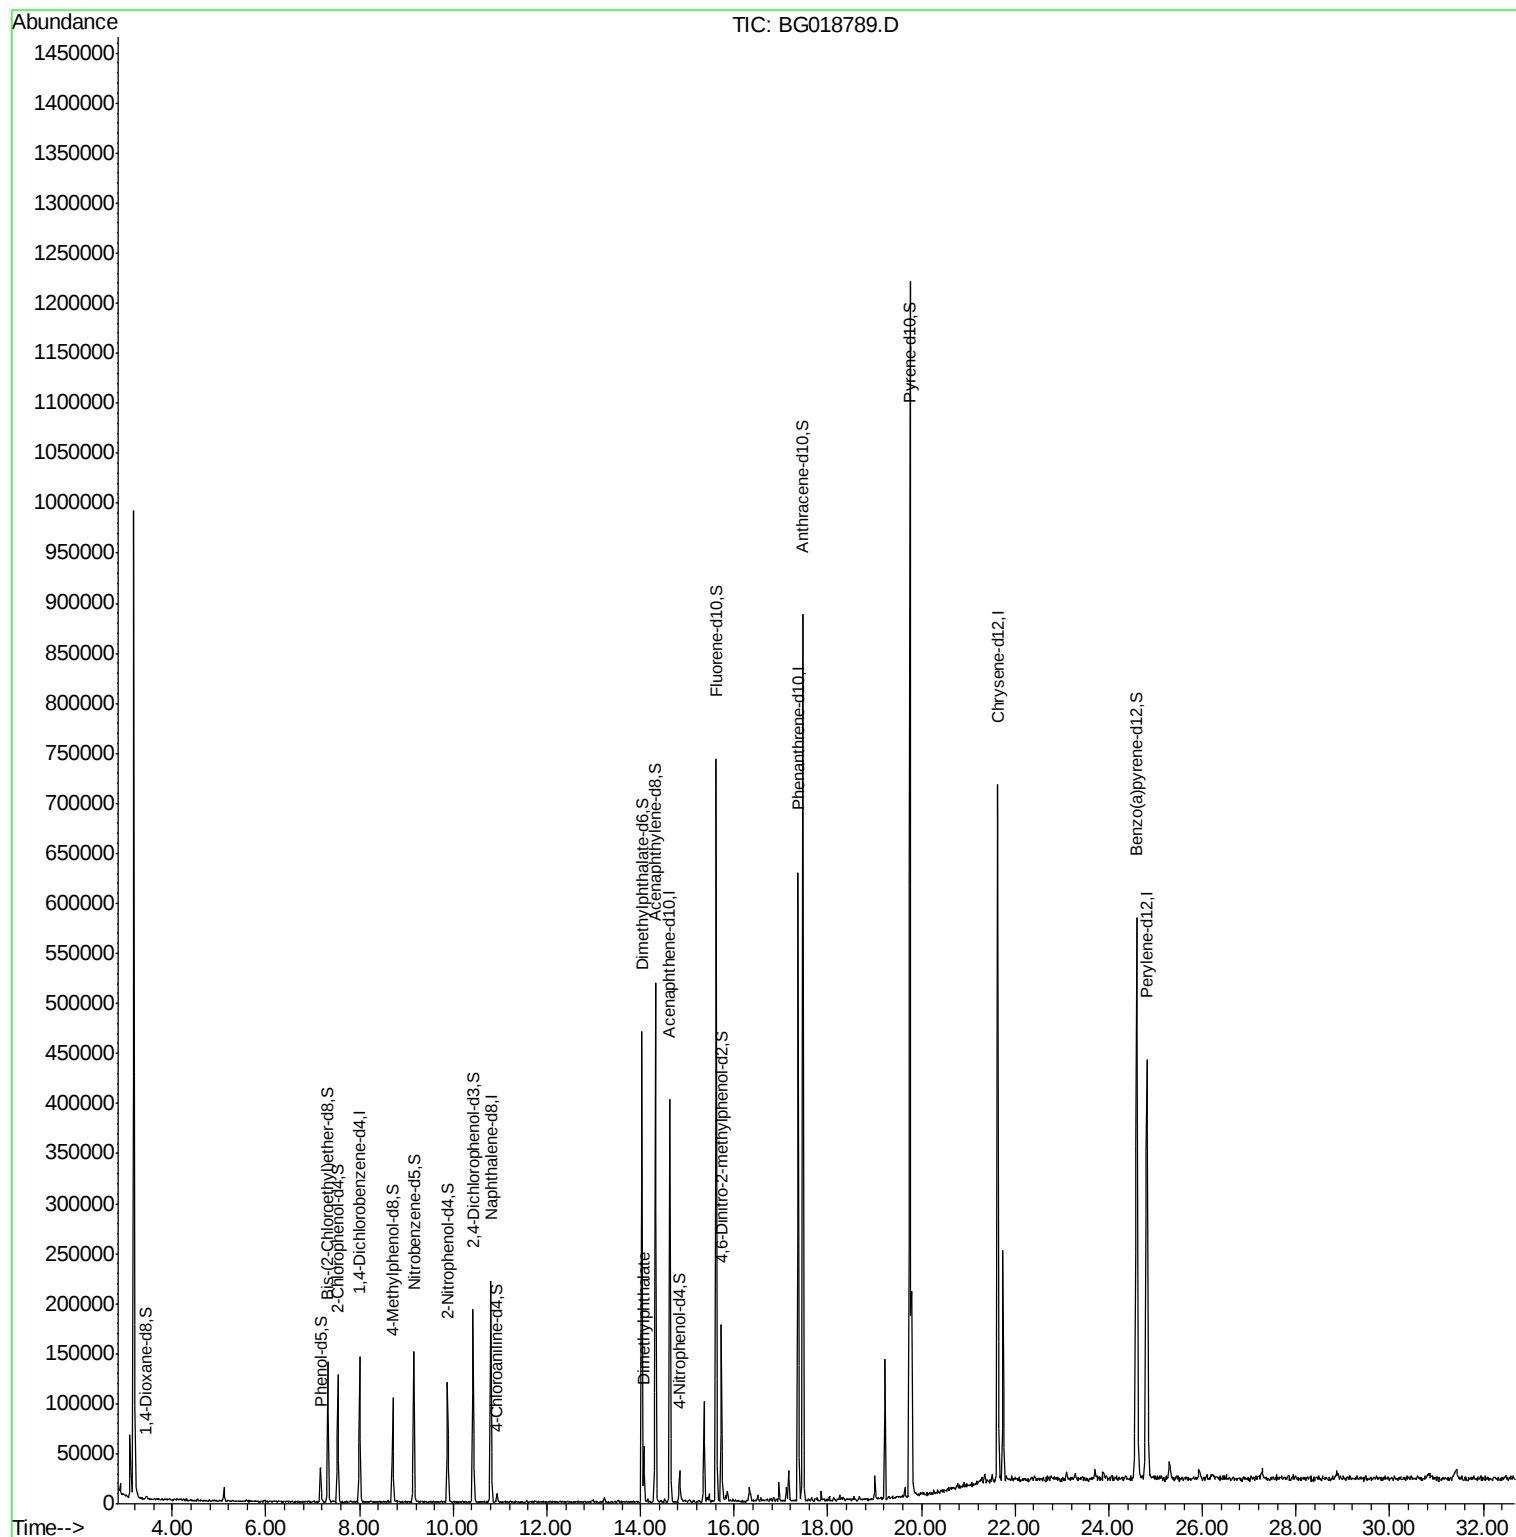

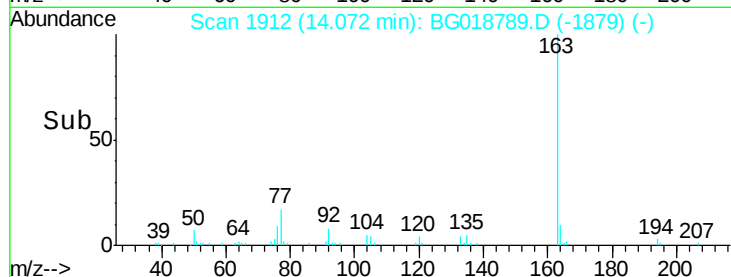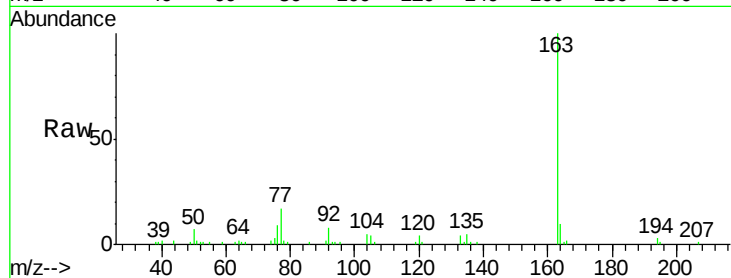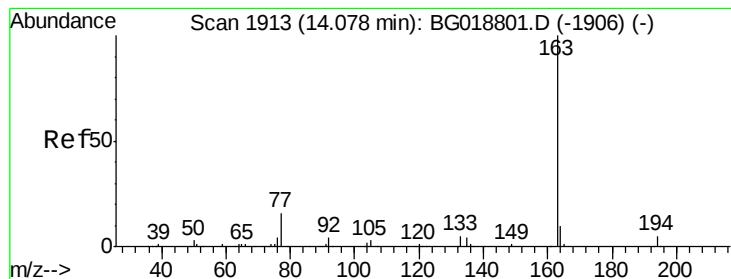

#45

Dimethylphthalate

Concen: 3.41 ng/ul

RT: 14.07 min Scan# 1912

Delta R.T. -0.01 min

Lab File: BG018789.D

Acq: 21 Sep 2015 19:17

Instrument :

BNA_G

ClientSampleId :

C0AR1

Tot Ion:163 Resp: 37110

Ion Ratio Lower Upper

163 100

194 3.2 2.9 4.3

164 10.2 7.7 11.5

