

Data Path : Z:\HPCHEM1\BNA G\DATA\BG092115\
 Data File : BG018797.D
 Acq On : 22 Sep 2015 00:20
 Operator : TP
 Sample : G3696-18
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AP2

Manual Integrations
 APPROVED

MMDadoda
 9/22/2015 2:14:50 PM

Quant Time: Sep 22 02:53:16 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG091015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 22 02:06:40 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.00	152	49839	20.00	ng/ul	0.00
18) Naphthalene-d8	10.80	136	204346	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.62	164	139904	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.37	188	381055	20.00	ng/ul	0.00
78) Chrysene-d12	21.63	240	434299	20.00	ng/ul	0.00
86) Perylene-d12	24.81	264	434430	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.44	96	1042	1.01	ng/uL	0.00
5) Phenol-d5	7.17	99	22229	5.43	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.32	67	71069	29.97	ng/ul	0.00
9) 2-Chlorophenol-d4	7.53	132	75314	24.30	ng/ul	0.00
13) 4-Methylphenol-d8	8.71	113	47186	14.21	ng/ul	0.00
19) Nitrobenzene-d5	9.16	128	51098	33.01	ng/ul	0.00
22) 2-Nitrophenol-d4	9.88	143	53437	34.32	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.42	165	91646	27.96	ng/ul	0.00
29) 4-Chloroaniline-d4	10.93	131	1491m	0.39	ng/ul	0.00
44) Dimethylphthalate-d6	14.02	166	384526	34.15	ng/ul	0.00
47) Acenaphthylene-d8	14.32	160	445417	33.38	ng/ul	0.00
52) 4-Nitrophenol-d4	14.83	143	10070	4.66	ng/ul	0.00
58) Fluorene-d10	15.62	176	341739	34.71	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.73	200	54946	30.46	ng/ul	0.00
71) Anthracene-d10	17.47	188	600270	35.78	ng/ul	0.00
79) Pyrene-d10	19.75	212	706436	35.36	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.59	264	654017	30.93	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.07	163	13230	1.21	ng/ul#	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG092115\
Data File : BG018797.D
Acq On : 22 Sep 2015 00:20
Operator : TP
Sample : G3696-18
Misc :
ALS Vial : 22 Sample Multiplier: 1




Instrument :
BNA_G
ClientSampleId :
C0AP2

Manual Integrations
APPROVED

MMDadoda
9/22/2015 2:14:50 PM

Quant Time: Sep 22 02:53:16 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG091015.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 22 02:06:40 2015
Response via : Initial Calibration

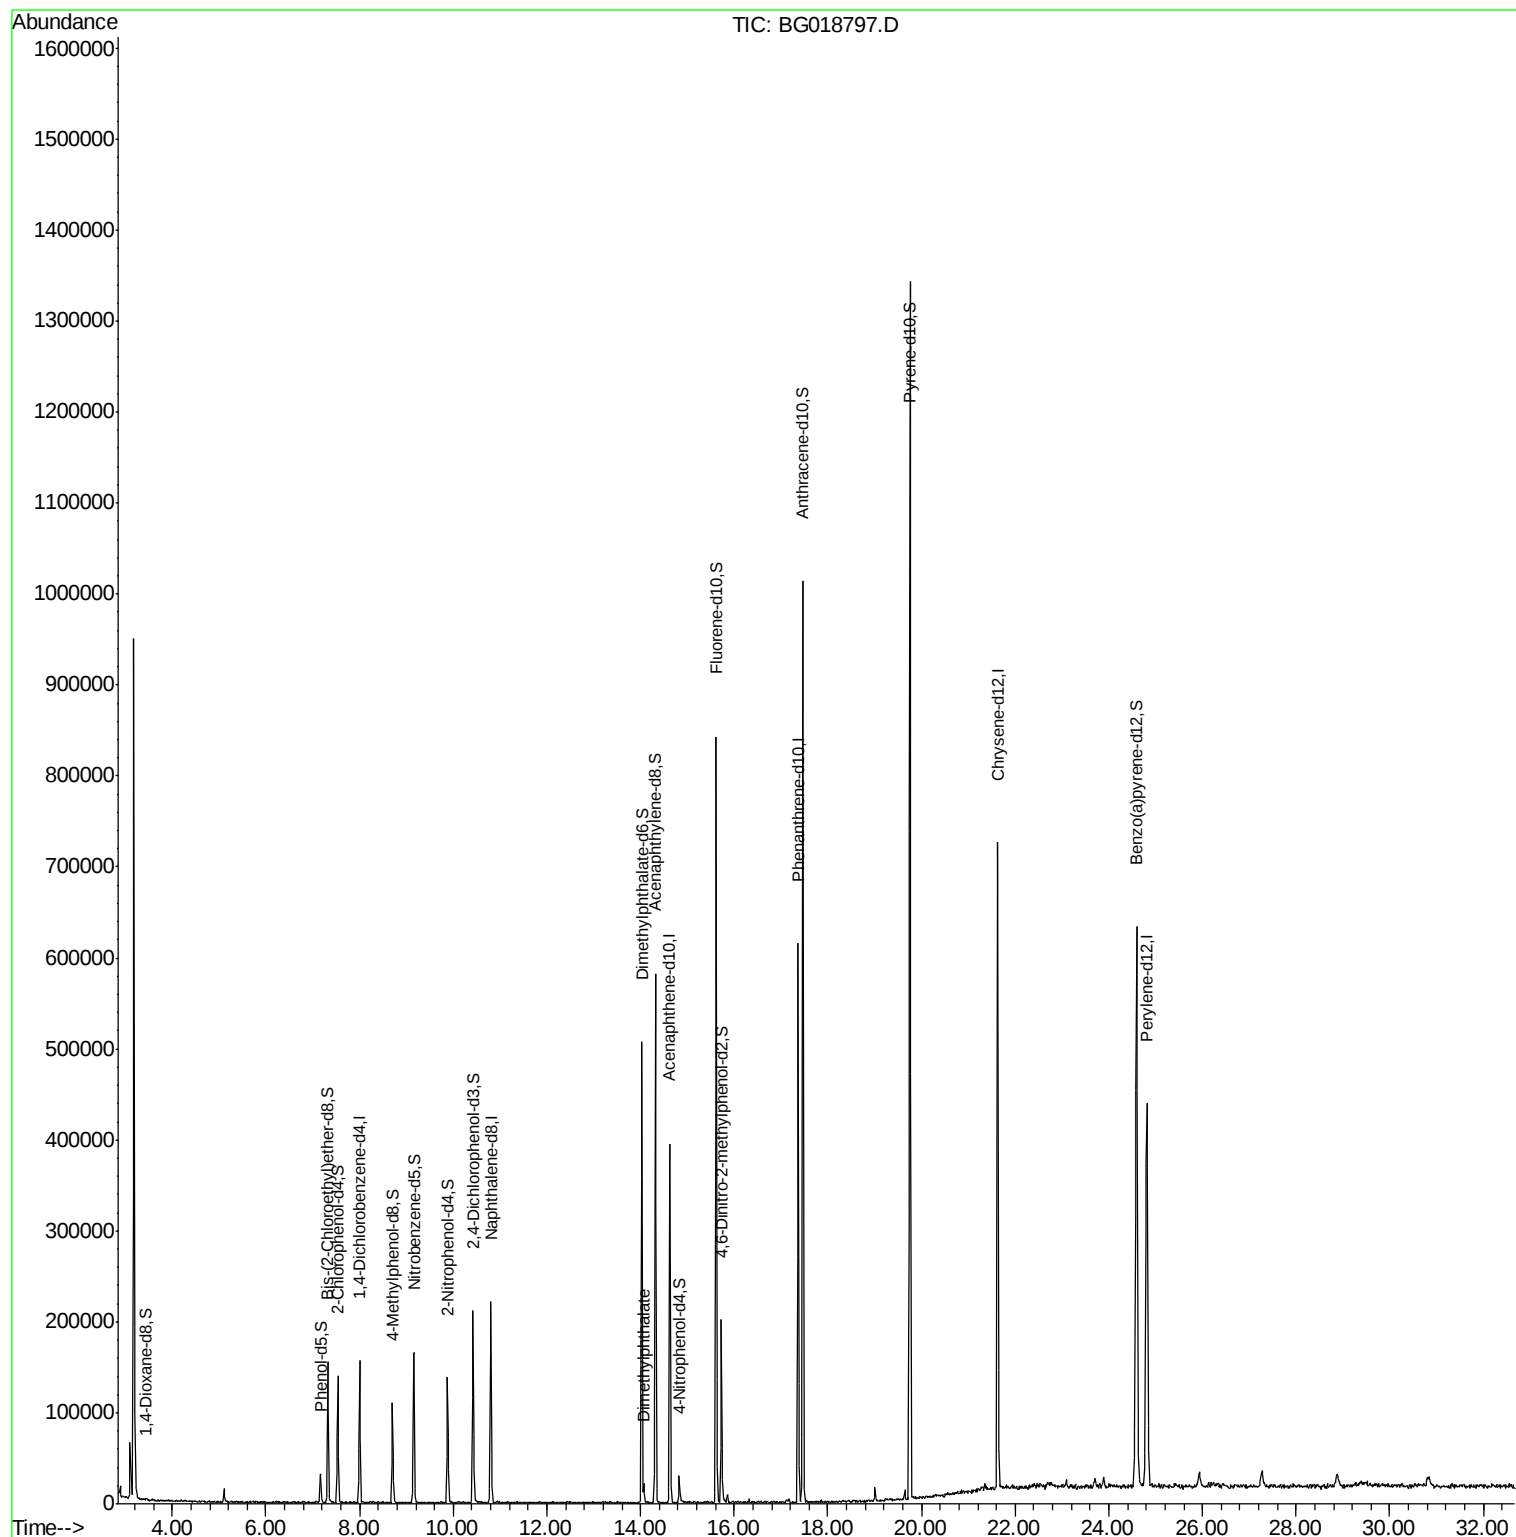

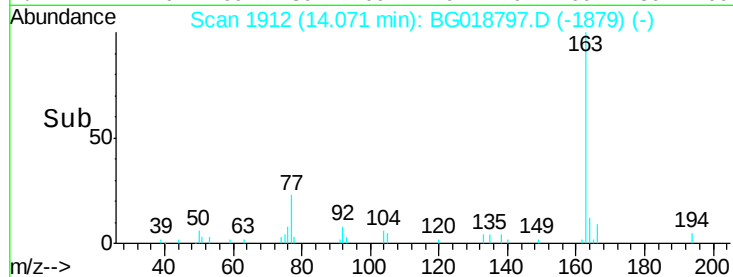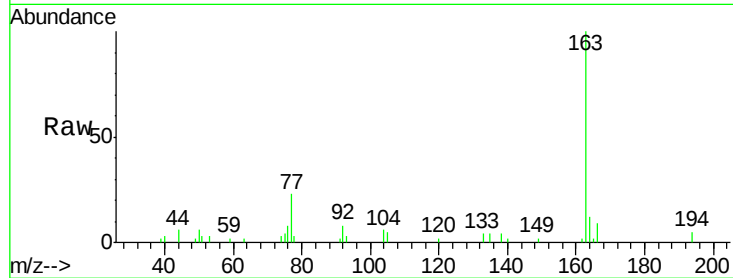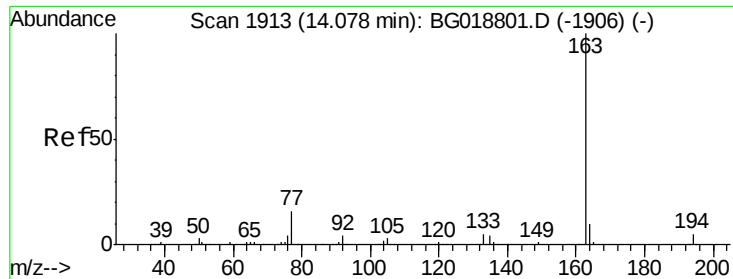

#45
 Dimethylphthalate
 Concen: 1.21 ng/ul
 RT: 14.07 min Scan# 1912
 Delta R.T. -0.01 min
 Lab File: BG018797.D
 Acq: 22 Sep 2015 00:20

Instrument :
 BNA_G
 ClientSampleId :
 C0AP2

Tot Ion	Ratio	Resp	Lower	Upper
163	100			
194	5.1	2.9	4.3#	
164	12.2	7.7	11.5#	

Manual Integrations
 APPROVED

MMDadoda
 9/22/2015 2:14:50 PM

