

Data Path : Z:\HPCHEM1\BNA G\DATA\BG092115\
 Data File : BG018800.D
 Acq On : 22 Sep 2015 2:14
 Operator : TP
 Sample : G3696-21
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AQ1

Quant Time: Sep 22 03:38:14 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG091015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 22 02:06:40 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.00	152	47065	20.00	ng/ul	0.00
18) Naphthalene-d8	10.80	136	200378	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.63	164	135683	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.37	188	377140	20.00	ng/ul	0.00
78) Chrysene-d12	21.63	240	430207	20.00	ng/ul	0.00
86) Perylene-d12	24.81	264	436987	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.44	96	841	0.86	ng/uL	0.00
5) Phenol-d5	7.16	99	21634	5.60	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	65086	29.06	ng/ul	0.00
9) 2-Chlorophenol-d4	7.53	132	70061	23.94	ng/ul	0.00
13) 4-Methylphenol-d8	8.70	113	43047	13.73	ng/ul	0.00
19) Nitrobenzene-d5	9.16	128	46035	30.32	ng/ul	0.00
22) 2-Nitrophenol-d4	9.88	143	49166	32.21	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.42	165	84066	26.15	ng/ul	0.00
29) 4-Chloroaniline-d4	10.93	131	6053	1.62	ng/ul	0.00
44) Dimethylphthalate-d6	14.02	166	371876	34.06	ng/ul	0.00
47) Acenaphthylene-d8	14.32	160	419764	32.44	ng/ul	0.00
52) 4-Nitrophenol-d4	14.83	143	11376	5.43	ng/ul	0.00
58) Fluorene-d10	15.62	176	332379	34.81	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.73	200	54781	30.69	ng/ul	0.00
71) Anthracene-d10	17.47	188	593120	35.72	ng/ul	0.00
79) Pyrene-d10	19.75	212	709447	35.84	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.59	264	584293	27.47	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.07	163	15596	1.47	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG092115\
Data File : BG018800.D
Acq On : 22 Sep 2015 2:14
Operator : TP
Sample : G3696-21
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AQ1

Quant Time: Sep 22 03:38:14 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG091015.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 22 02:06:40 2015
Response via : Initial Calibration

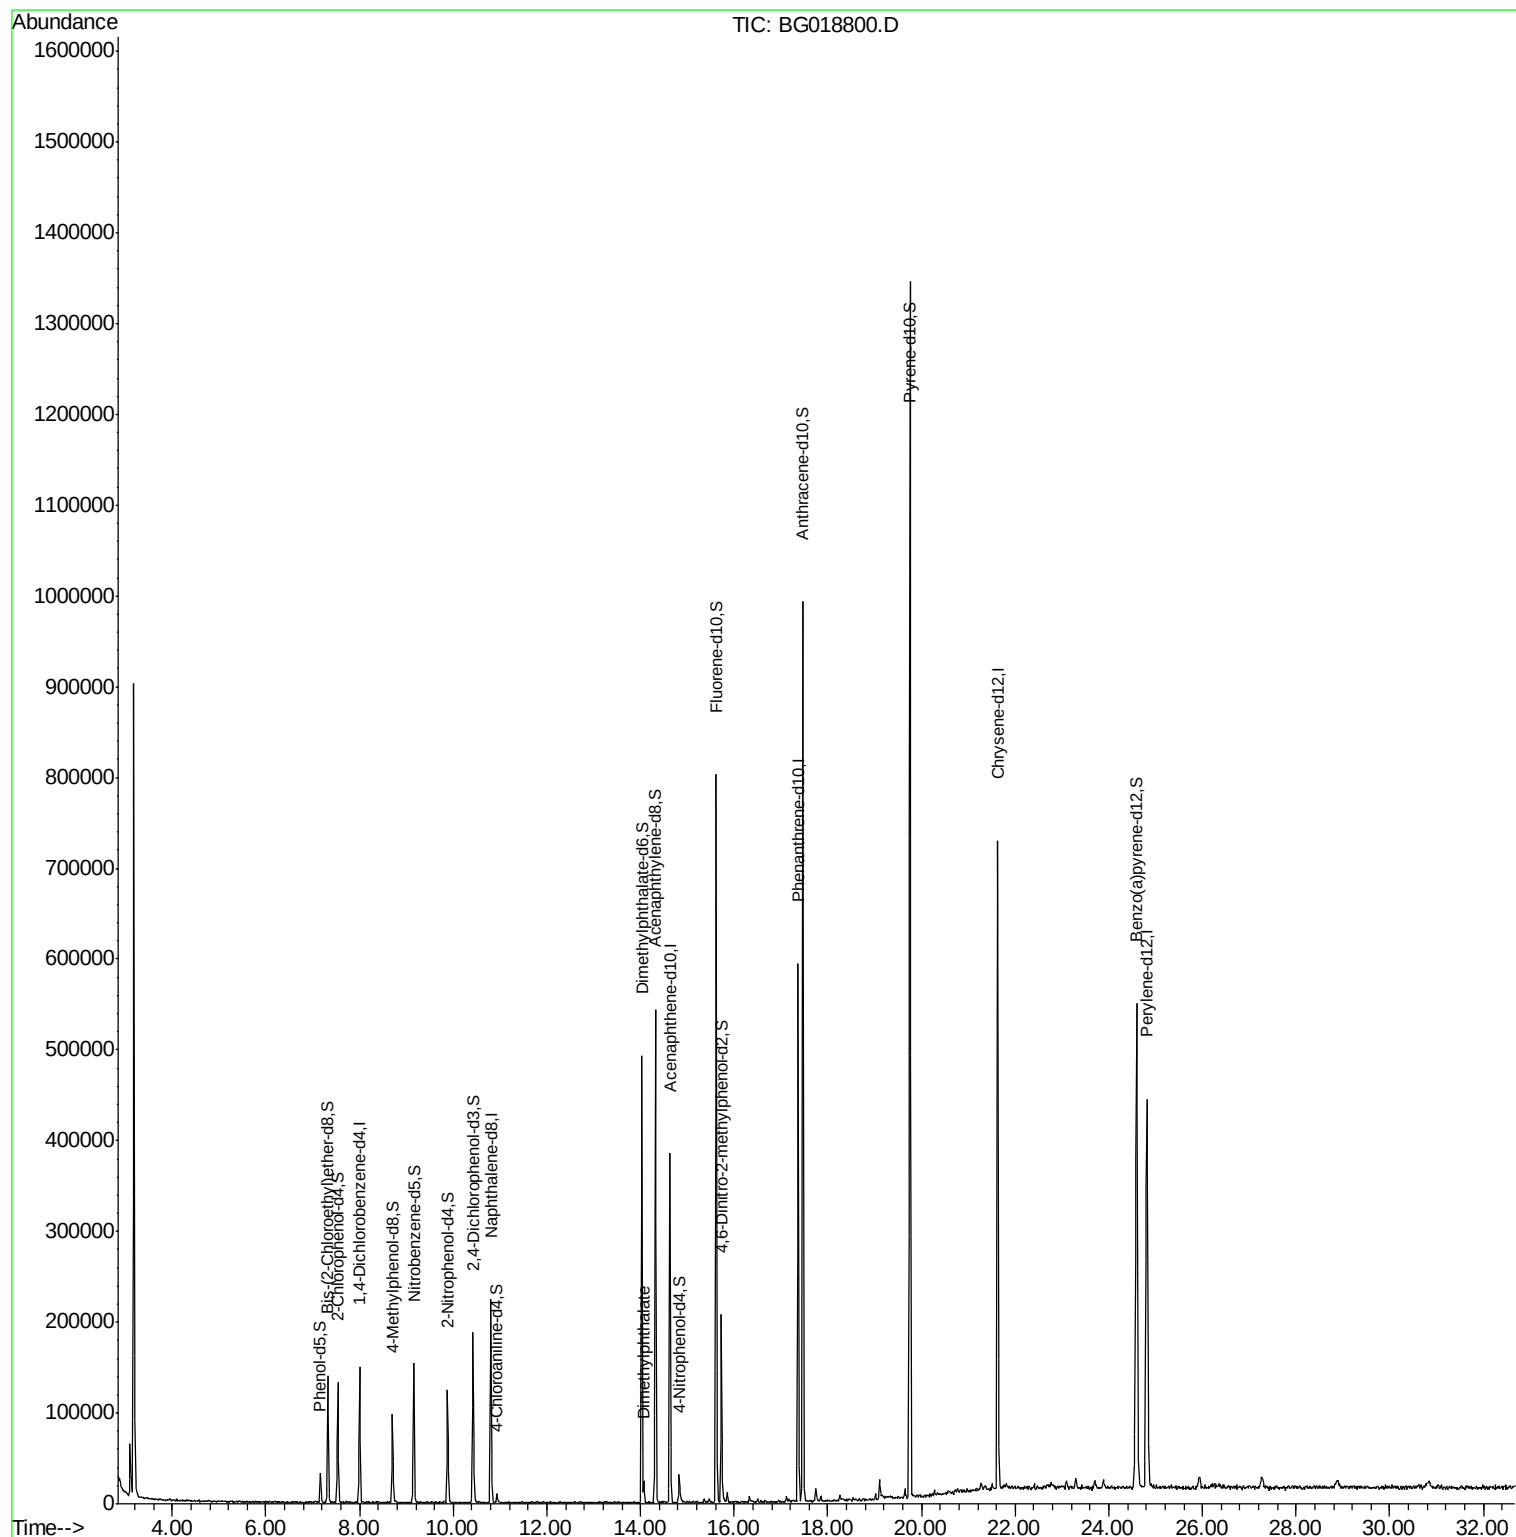

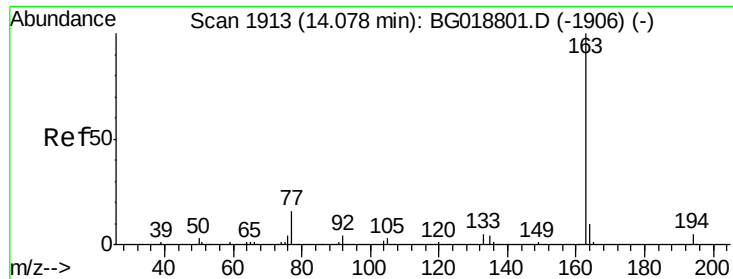

#45

Dimethylphthalate

Concen: 1.47 ng/ul

RT: 14.07 min Scan# 1912

Delta R.T. -0.01 min

Lab File: BG018800.D

Acq: 22 Sep 2015 2:14

Instrument :

BNA_G

ClientSampleId :

C0AQ1


Tot Ion:163 Resp: 15596

Ion Ratio Lower Upper

163 100

194 4.0 2.9 4.3

164 9.5 7.7 11.5

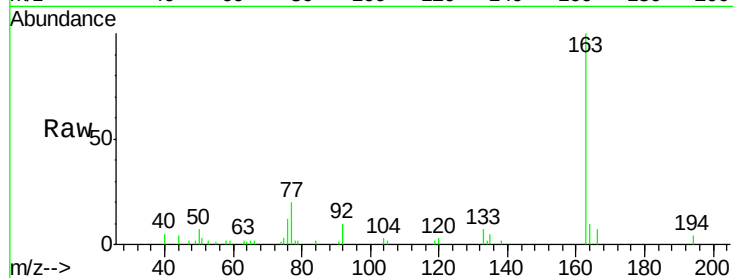

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

