
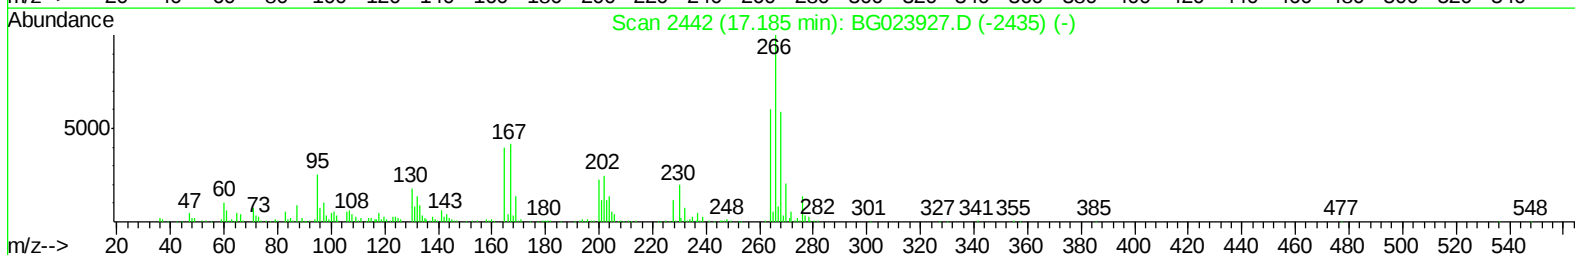
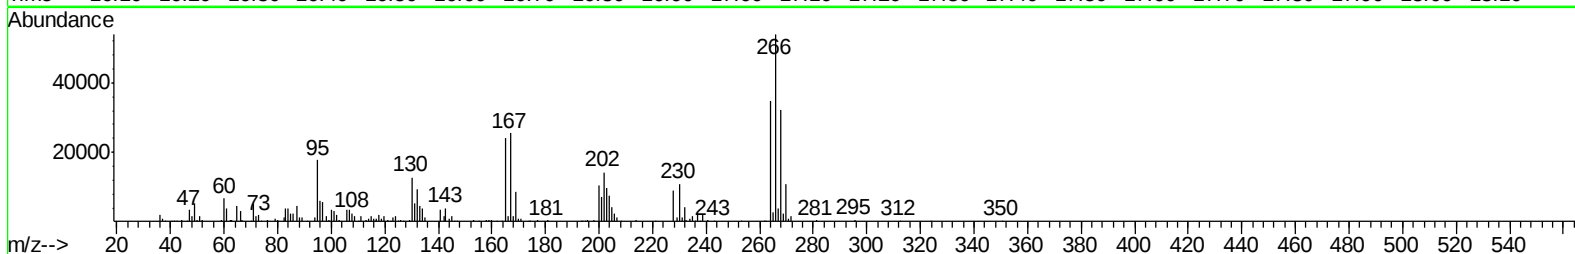


Data Path : Z:\HPCHEM1\BNA G\DATA\BG092116\
Data File : BG024049.D
Acq On : 21 Sep 2016 11:15
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 22 19:03:53 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 19:01:00 2016
Response via : Initial Calibration

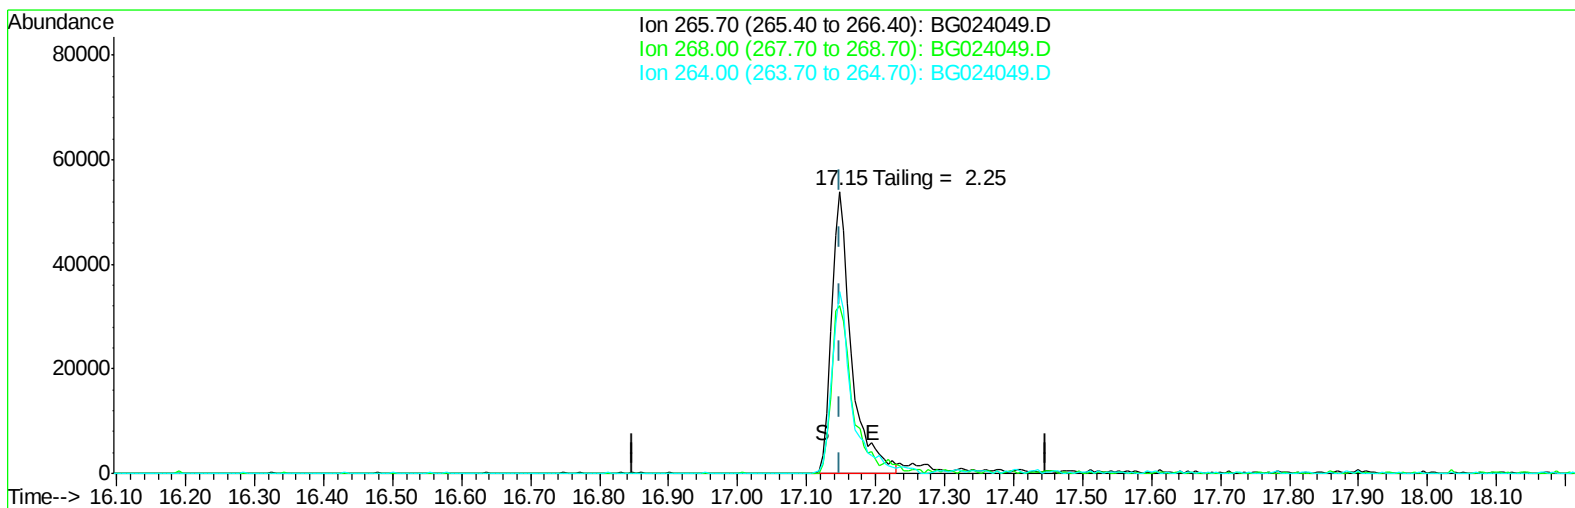

TIC: BG024049.D

(69) Pentachlorophenol (C)




17.147min (-0.001) 205136.29ng

response 105714

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	59.55
264.00	63.20	64.38
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG092116\
Data File : BG024049.D
Acq On : 21 Sep 2016 11:15
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 22 19:03:53 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 19:01:00 2016
Response via : Initial Calibration

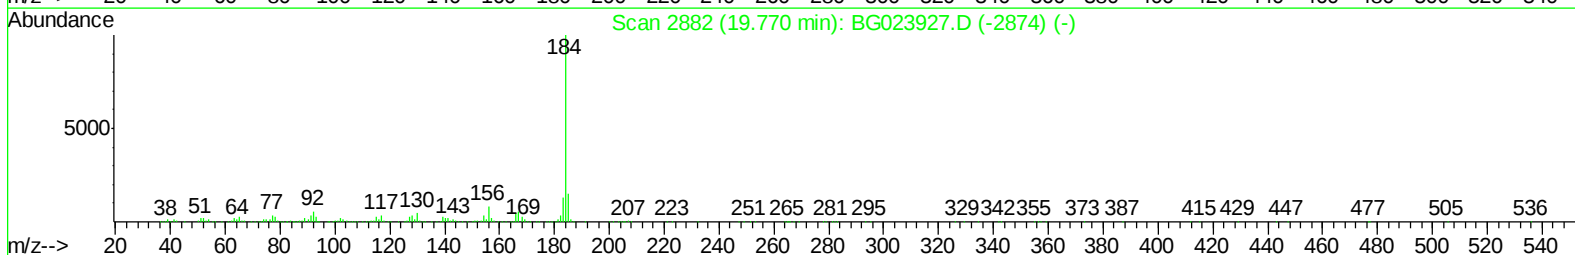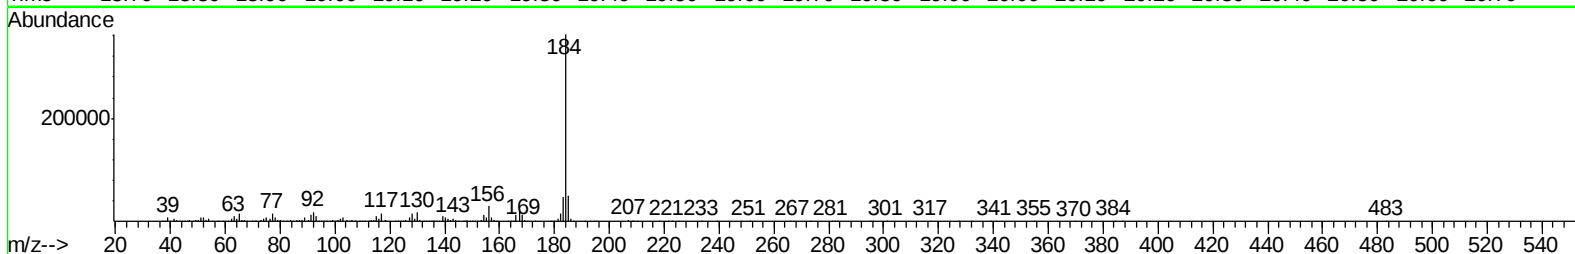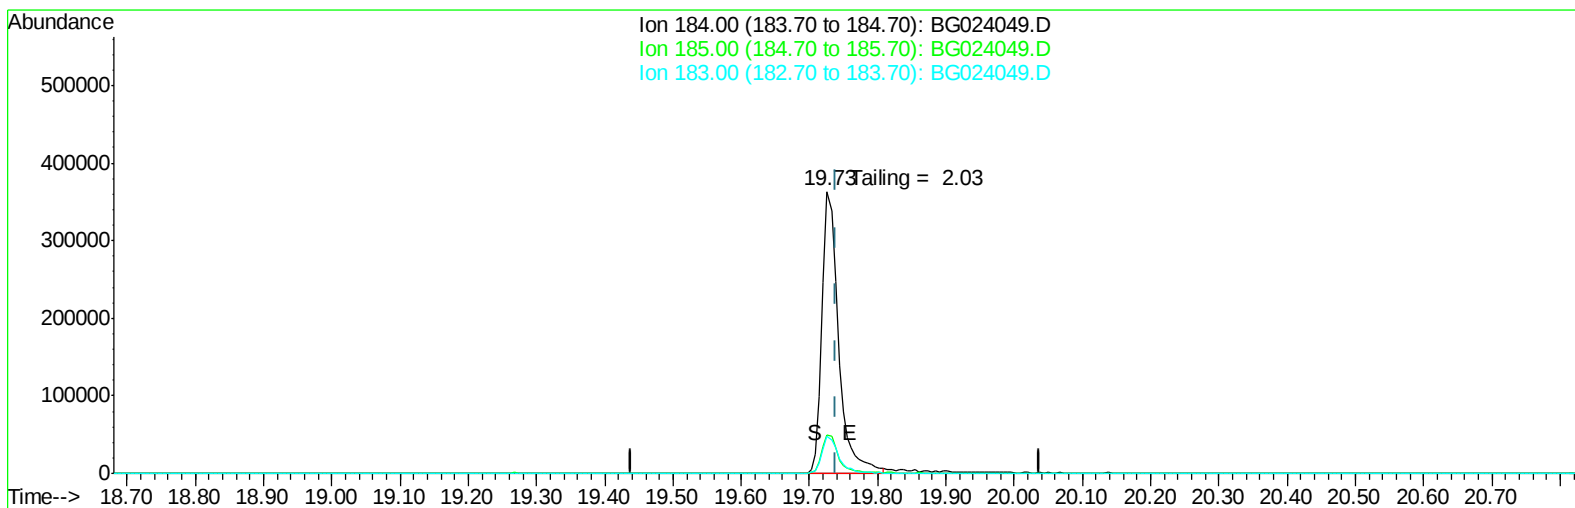

TIC: BG024049.D

(76) Benzidine

19.726min (-0.013) 154682.84ng

response 613104

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	13.77
183.00	13.40	13.02
0.00	0.00	0.00