
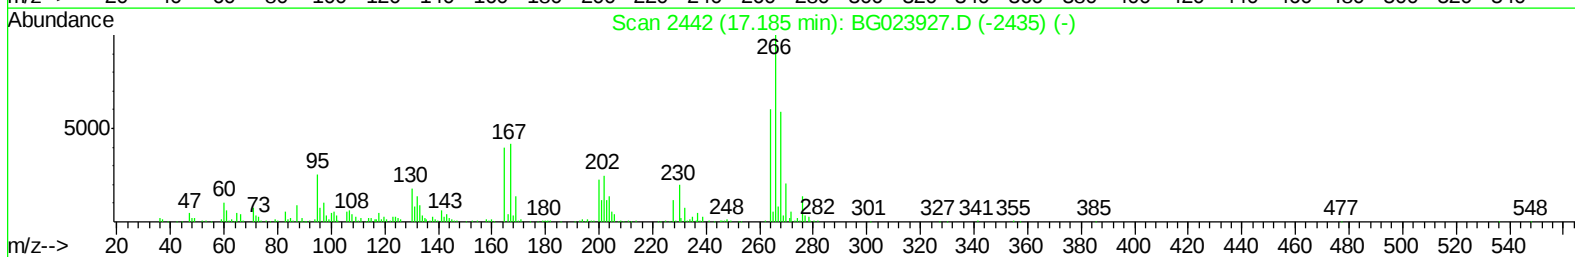
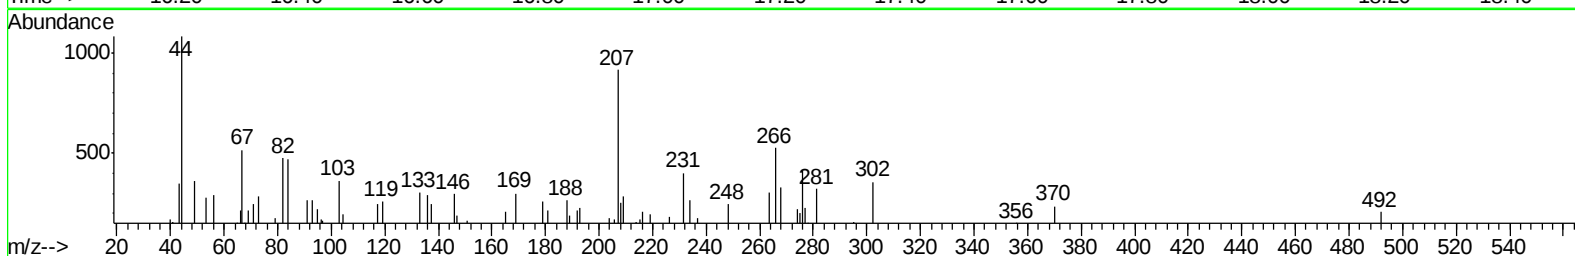


Data Path : Z:\HPCHEM1\BNA G\DATA\BG092116\
 Data File : BG024066.D
 Acq On : 22 Sep 2016 1:25
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 22 19:04:58 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG083116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 19:01:00 2016
 Response via : Initial Calibration

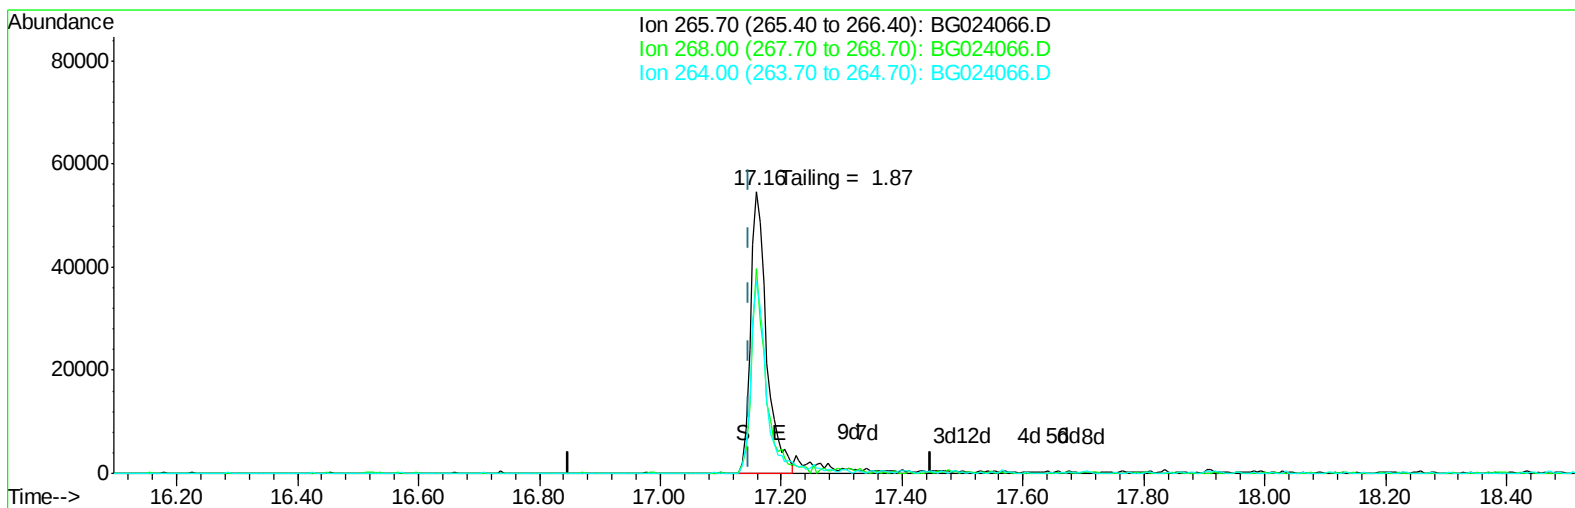

TIC: BG024066.D

(69) Pentachlorophenol (C)




17.500min (+0.352) 721.46ng

response 421

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	63.00
264.00	63.20	58.25
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG092116\
 Data File : BG024066.D
 Acq On : 22 Sep 2016 1:25
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 22 19:04:58 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG083116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 19:01:00 2016
 Response via : Initial Calibration

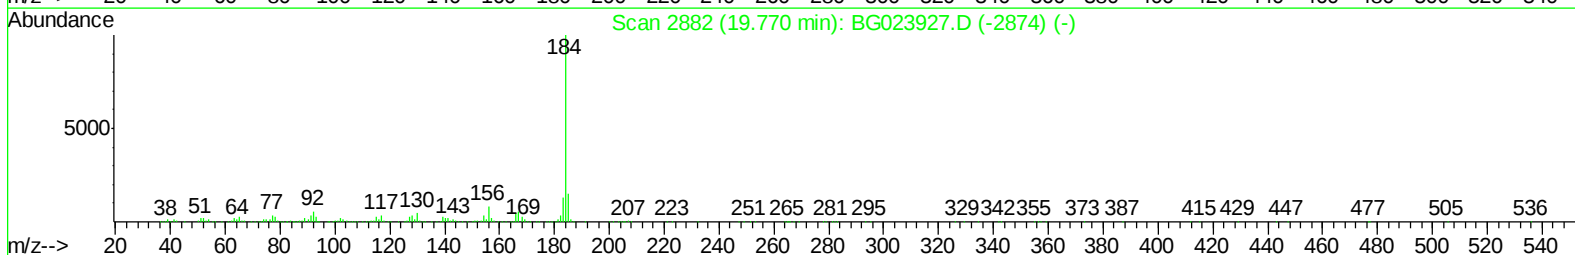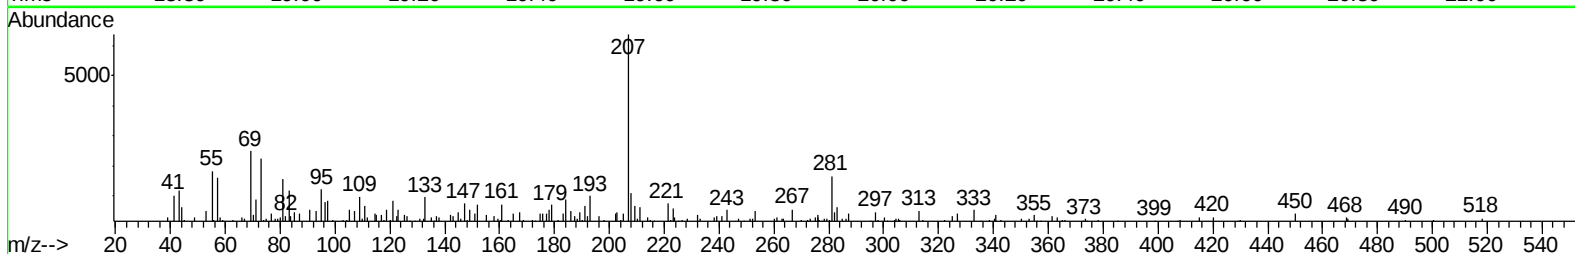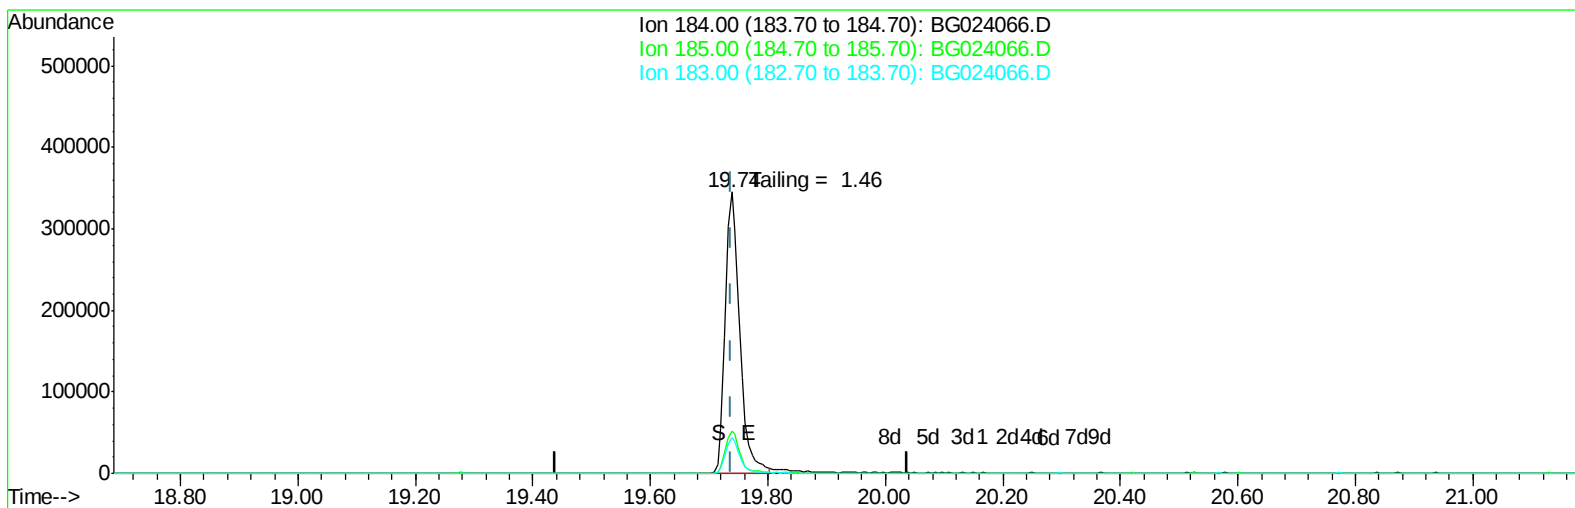

TIC: BG024066.D

(76) Benzidine

20.167min (+0.428) 35.34ng

response 336

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	0.00#
183.00	13.40	48.45#
0.00	0.00	0.00