


Data Path : Z:\HPCHEM1\BNA G\DATA\BG092116\
Data File : BG024049.D
Acq On : 21 Sep 2016 11:15
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG083116.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Sep 20 19:01:00 2016

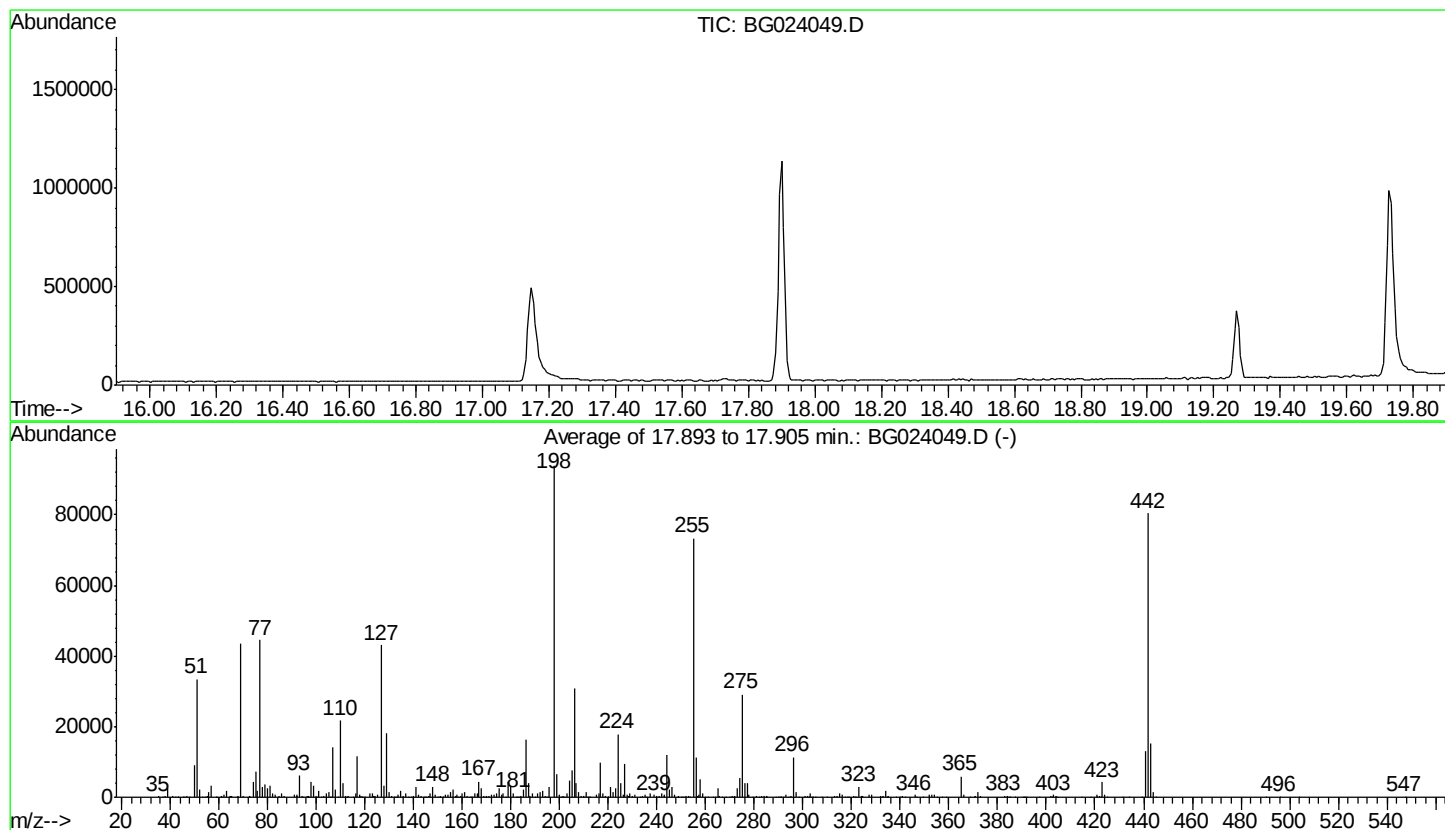

AutoFind: Scans 2563, 2564, 2565; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	33377	PASS
68	69	0.00	2	0.8	330	PASS
69	198	0.00	100	46.3	43517	PASS
70	69	0.00	2	1.0	455	PASS
127	198	10	80	45.8	43032	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	93965	PASS
199	198	5	9	6.8	6370	PASS
275	198	10	60	31.0	29138	PASS
365	198	1	100	6.2	5811	PASS
441	442	0.01	24	16.2	12989	PASS
442	198	50	100	85.6	80418	PASS
443	442	15	24	19.1	15369	PASS