


Data Path : Z:\HPCHEM1\BNA G\DATA\BG092116\
 Data File : BG024066.D
 Acq On : 22 Sep 2016 1:25
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG083116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 20 19:01:00 2016

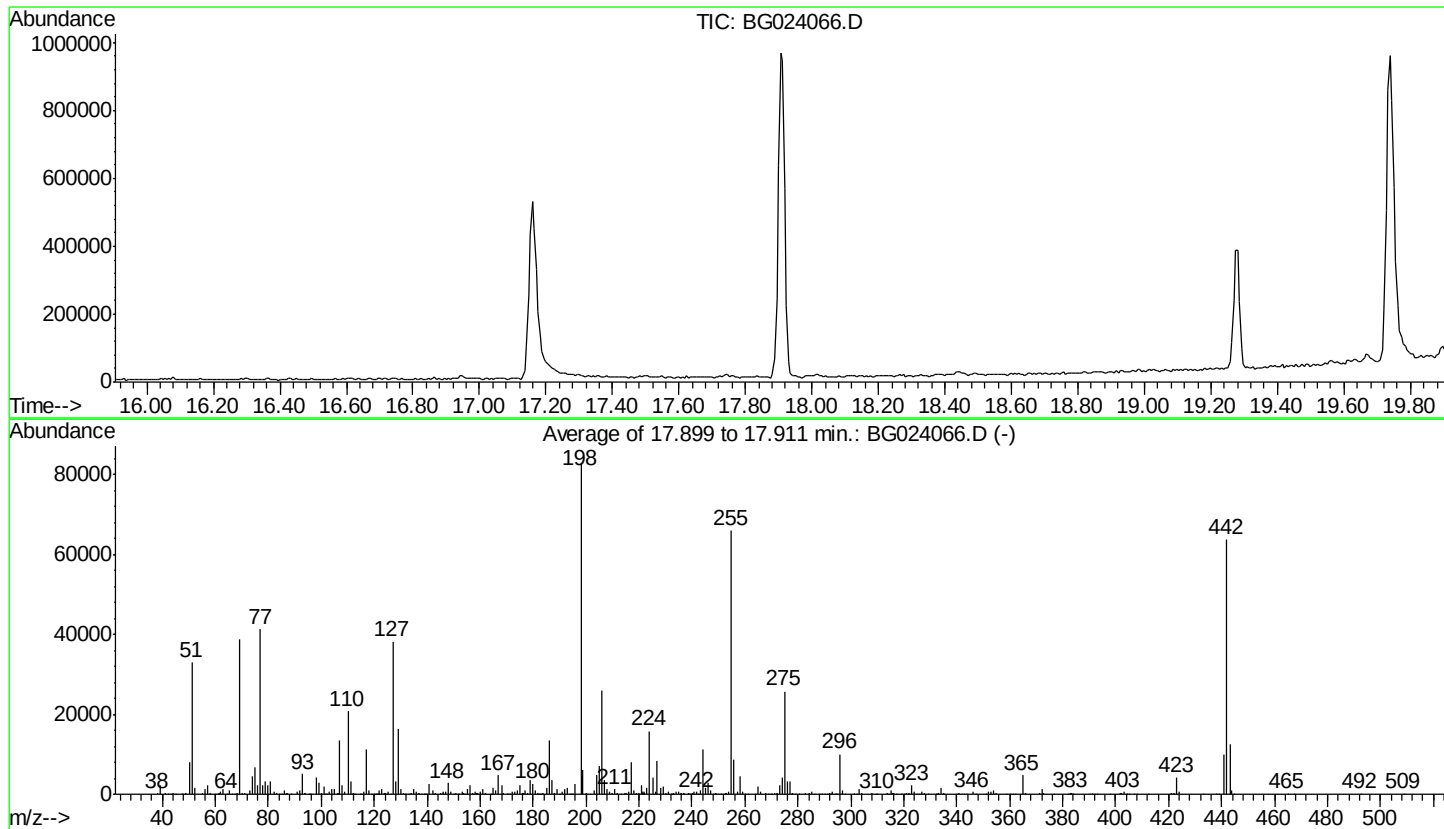

AutoFind: Scans 2564, 2565, 2566; Background Corrected with Scan 2558

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.6	32877	PASS
68	69	0.00	2	0.8	304	PASS
69	198	0.00	100	46.8	38824	PASS
70	69	0.00	2	0.5	175	PASS
127	198	10	80	46.1	38277	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	83029	PASS
199	198	5	9	7.4	6112	PASS
275	198	10	60	30.9	25685	PASS
365	198	1	100	5.7	4707	PASS
441	442	0.01	24	15.5	9853	PASS
442	198	50	100	76.8	63736	PASS
443	442	15	24	19.6	12475	PASS