
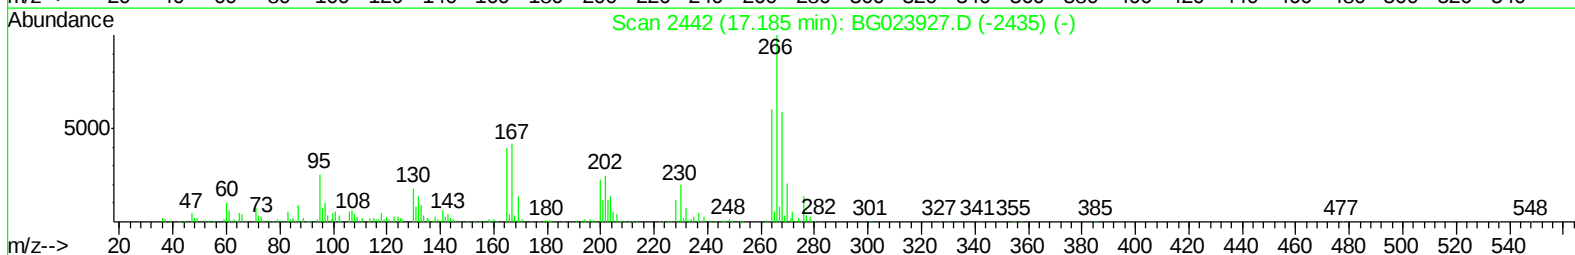
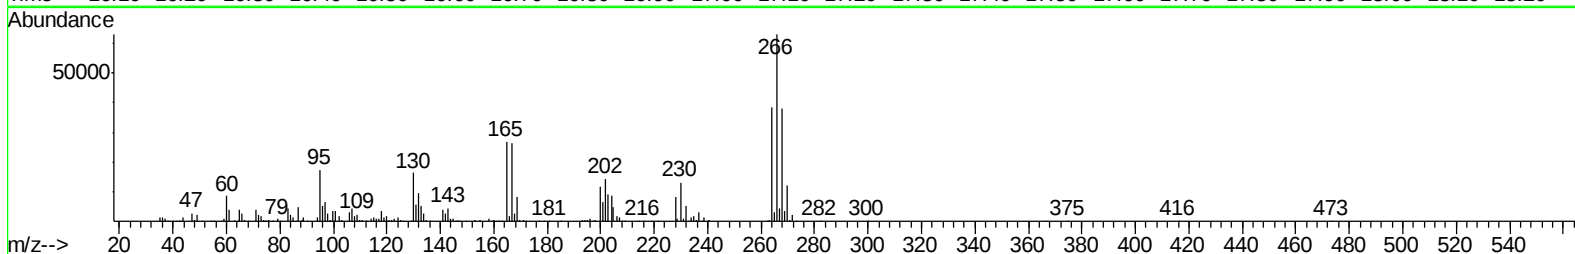


Data Path : Z:\HPCHEM1\BNA_G\Data\BG092216\
Data File : BG024071.D
Acq On : 22 Sep 2016 13:59
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 23 08:05:28 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 19:01:00 2016
Response via : Initial Calibration

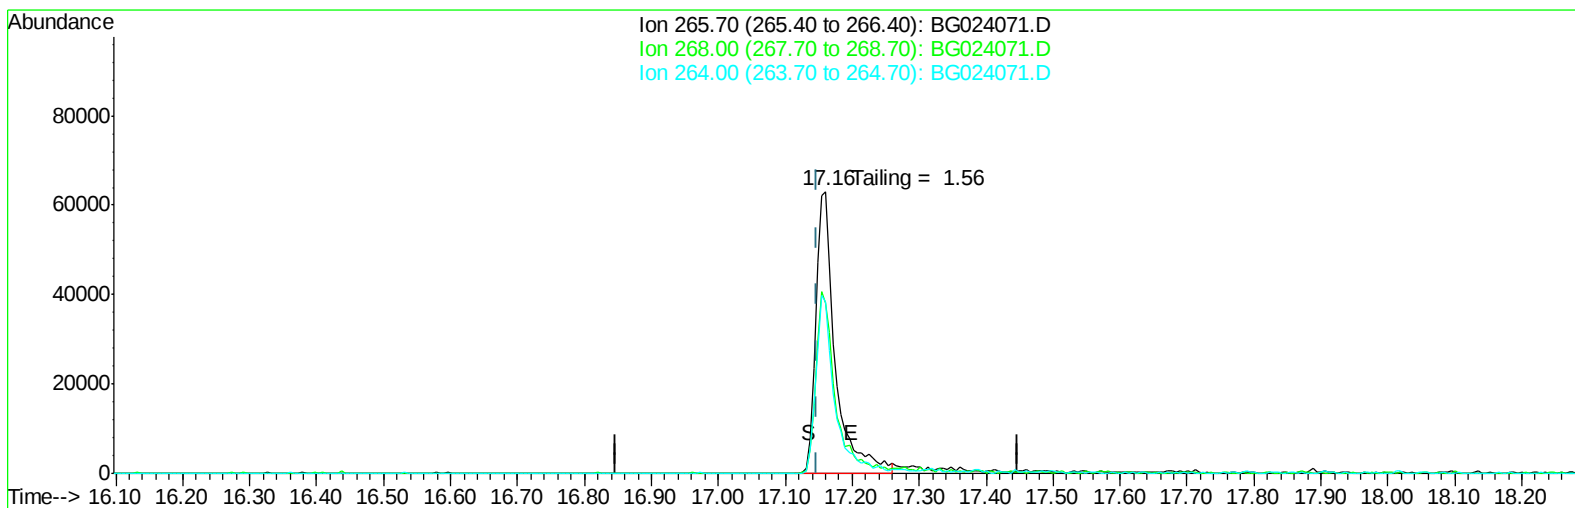

TIC: BG024071.D

(69) Pentachlorophenol (C)




17.160min (+0.012) 5027.07ng

response 131703

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	60.41
264.00	63.20	61.13
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG092216\
 Data File : BG024071.D
 Acq On : 22 Sep 2016 13:59
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 23 08:05:28 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG083116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 19:01:00 2016
 Response via : Initial Calibration

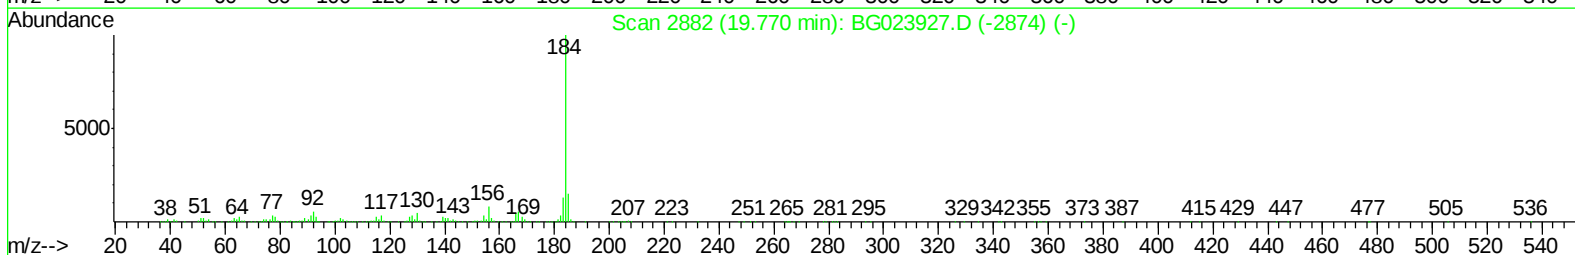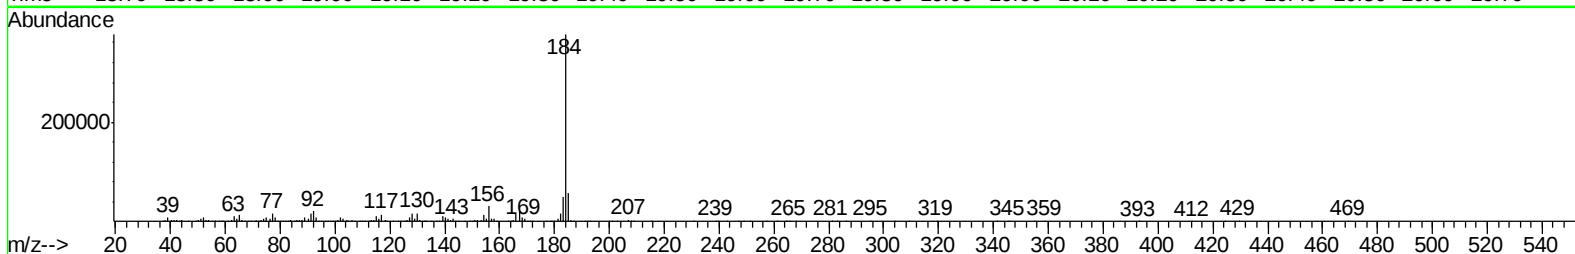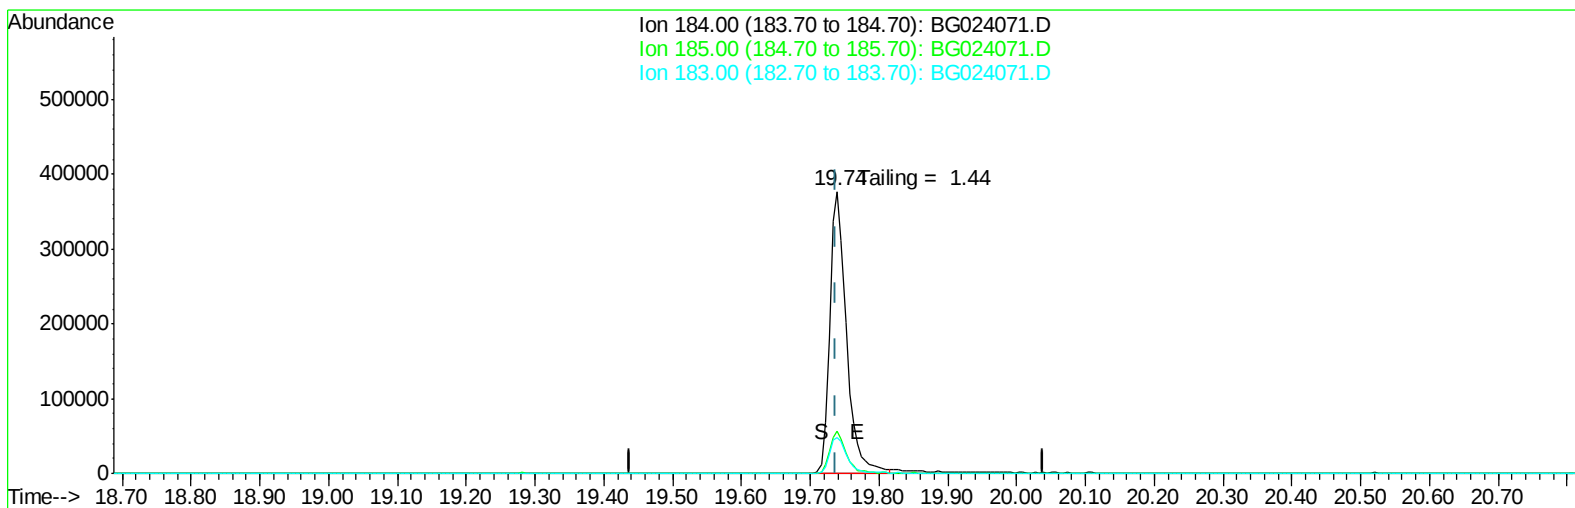

TIC: BG024071.D

(76) Benzidine

19.739min (+0.000) 3126.91ng

response 632185

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	14.99
183.00	13.40	12.94
0.00	0.00	0.00