


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG092216\
 Data File : BG024071.D
 Acq On : 22 Sep 2016 13:59
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG083116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 20 19:01:00 2016

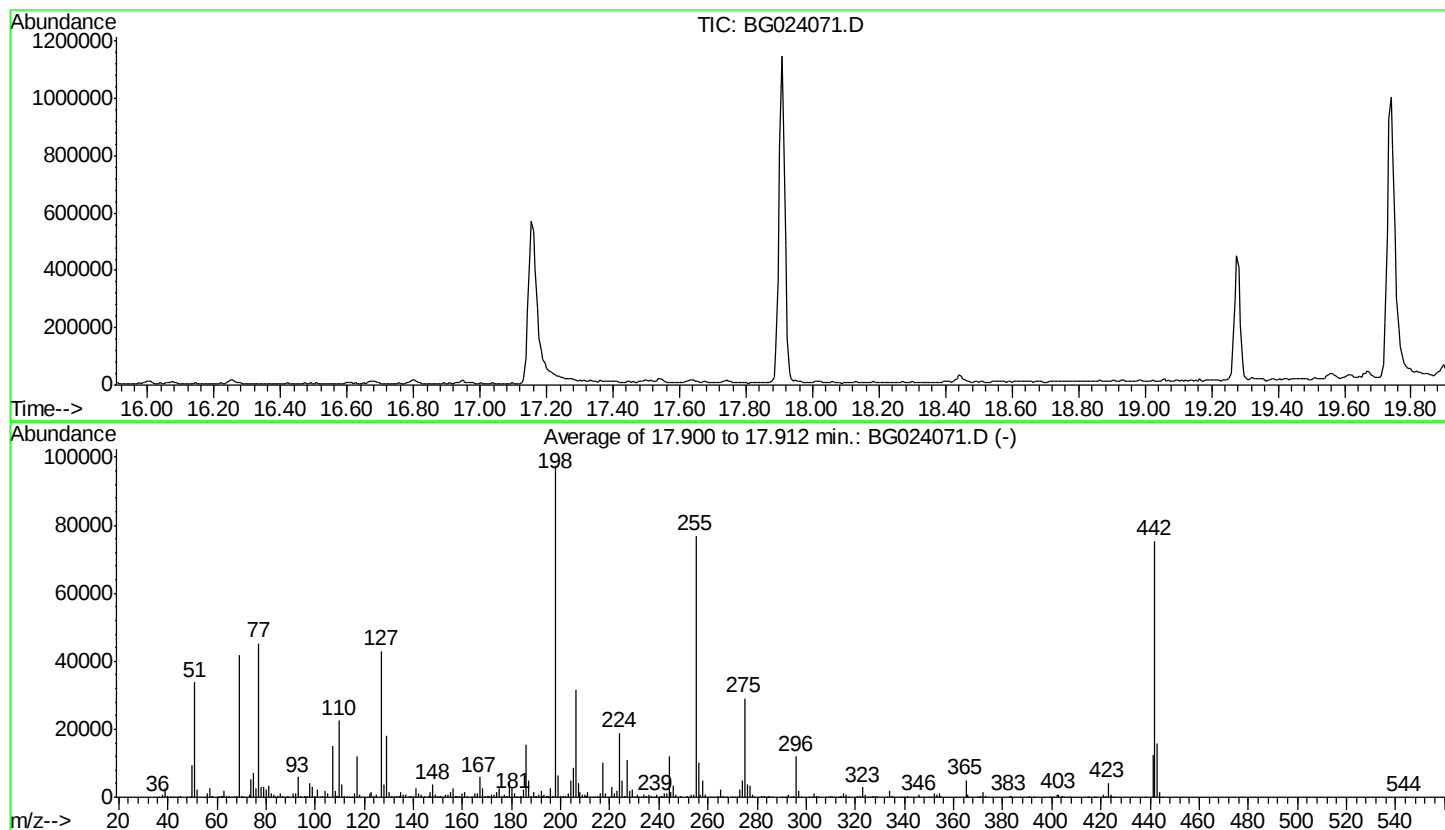

AutoFind: Scans 2564, 2565, 2566; Background Corrected with Scan 2557

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	33869	PASS
68	69	0.00	2	0.6	267	PASS
69	198	0.00	100	42.7	41681	PASS
70	69	0.00	2	0.8	331	PASS
127	198	10	80	44.0	42957	PASS
197	198	0.00	2	0.4	397	PASS
198	198	100	100	100.0	97549	PASS
199	198	5	9	6.4	6282	PASS
275	198	10	60	29.7	29016	PASS
365	198	1	100	5.0	4902	PASS
441	442	0.01	24	16.5	12456	PASS
442	198	50	100	77.3	75448	PASS
443	442	15	24	21.2	15992	PASS