
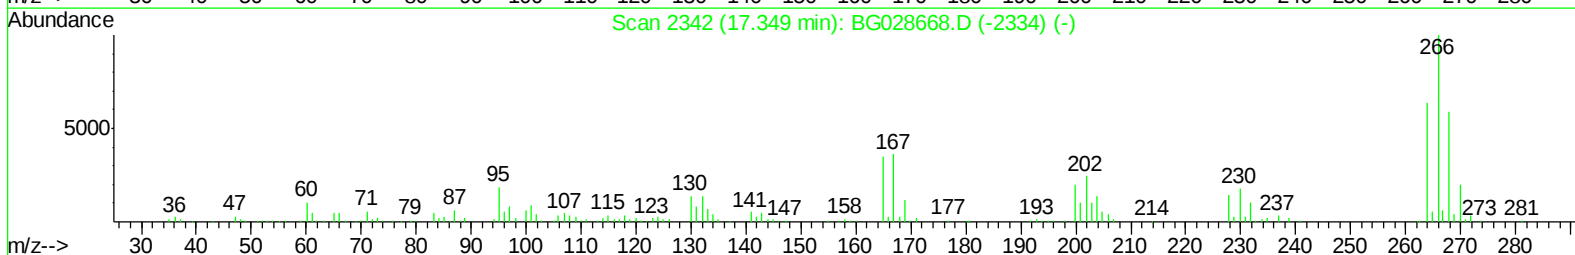
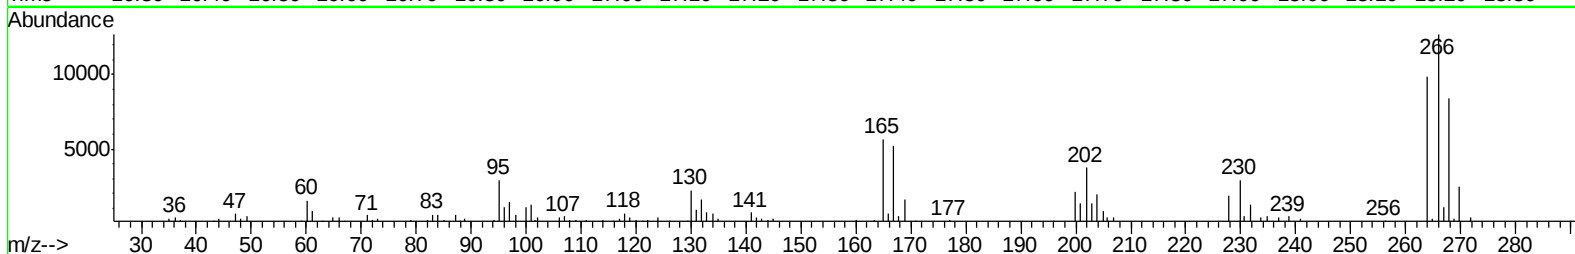


Data Path : Z:\HPCHEM1\BNA G\DATA\BG092217\
Data File : BG028877.D
Acq On : 22 Sep 2017 16:42
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 23 04:20:36 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 16:57:11 2017
Response via : Initial Calibration

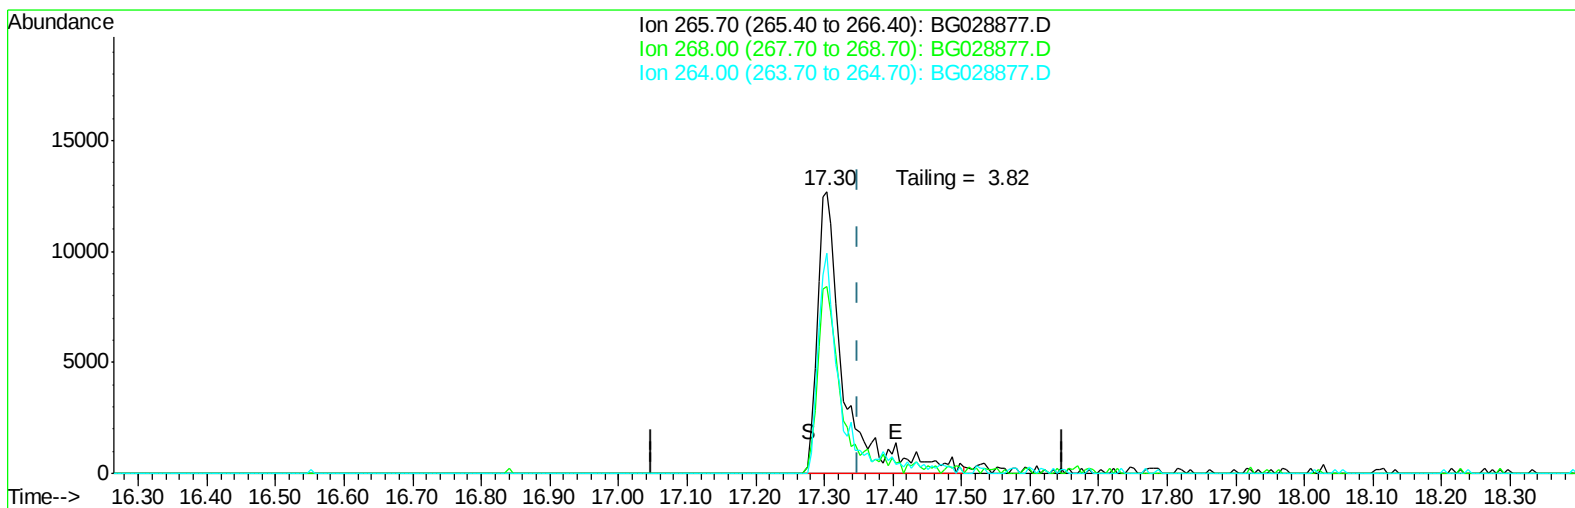

TIC: BG028877.D

(69) Pentachlorophenol (C)




17.304min (-0.045) 0.00ng

response 28465

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	66.24
264.00	62.60	78.02#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG092217\
Data File : BG028877.D
Acq On : 22 Sep 2017 16:42
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 23 04:20:36 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 16:57:11 2017
Response via : Initial Calibration

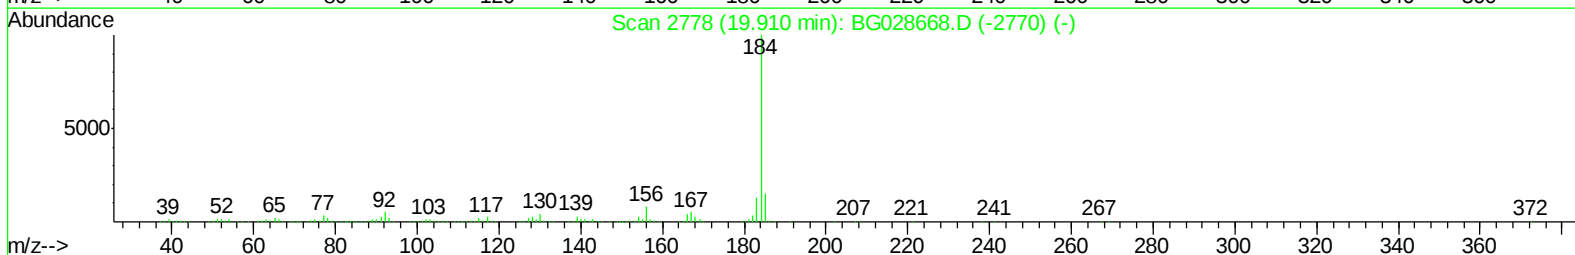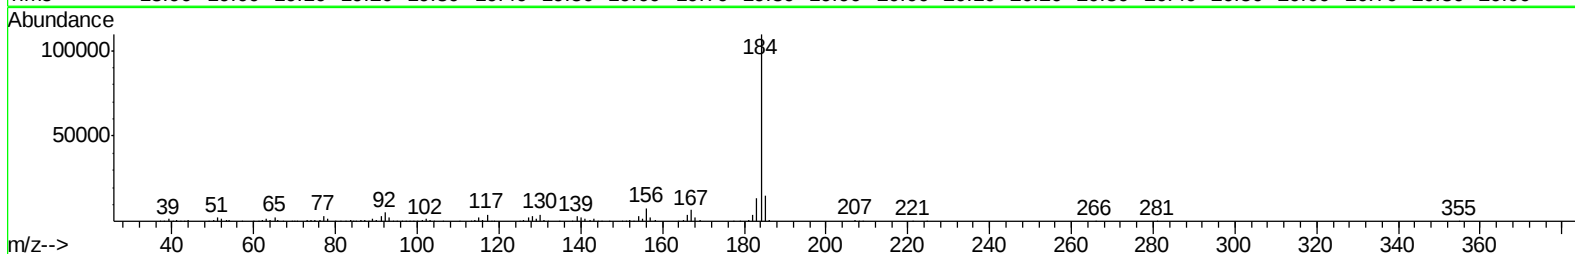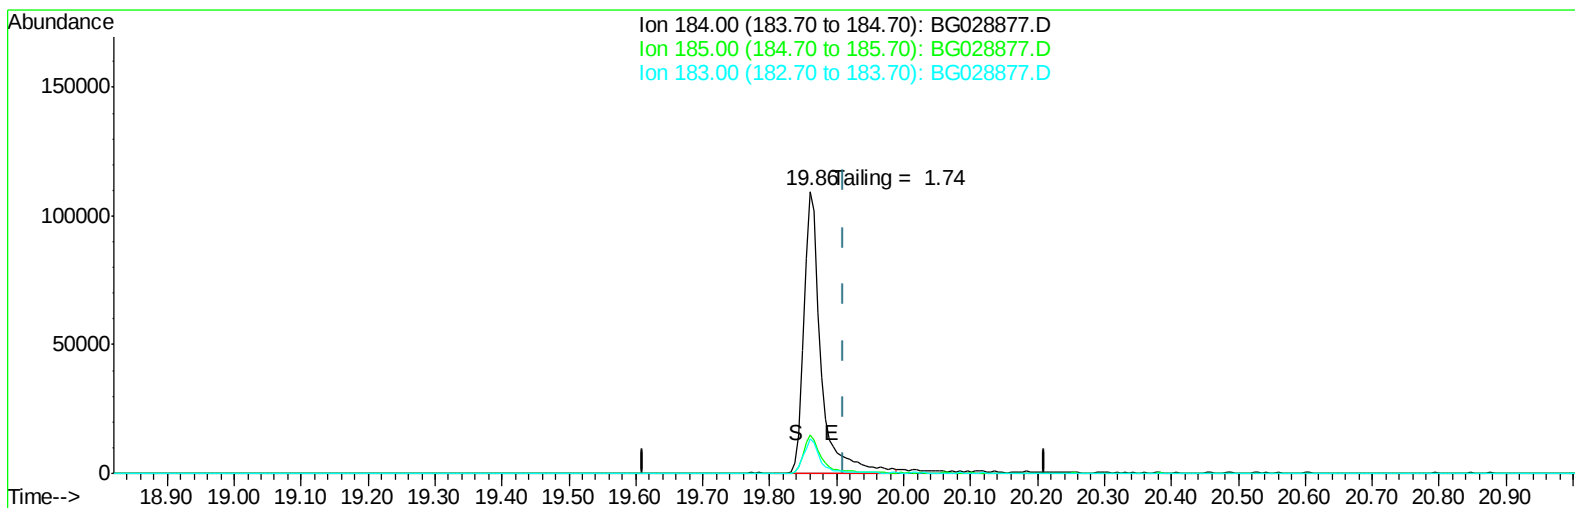

TIC: BG028877.D

(76) Benzidine

19.860min (-0.050) 9236.98ng

response 200971

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	13.65
183.00	13.80	12.21
0.00	0.00	0.00