


Data Path : Z:\HPCHEM1\BNA G\Data\BG092217\
 Data File : BG028877.D
 Acq On : 22 Sep 2017 16:42
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 12 16:57:11 2017

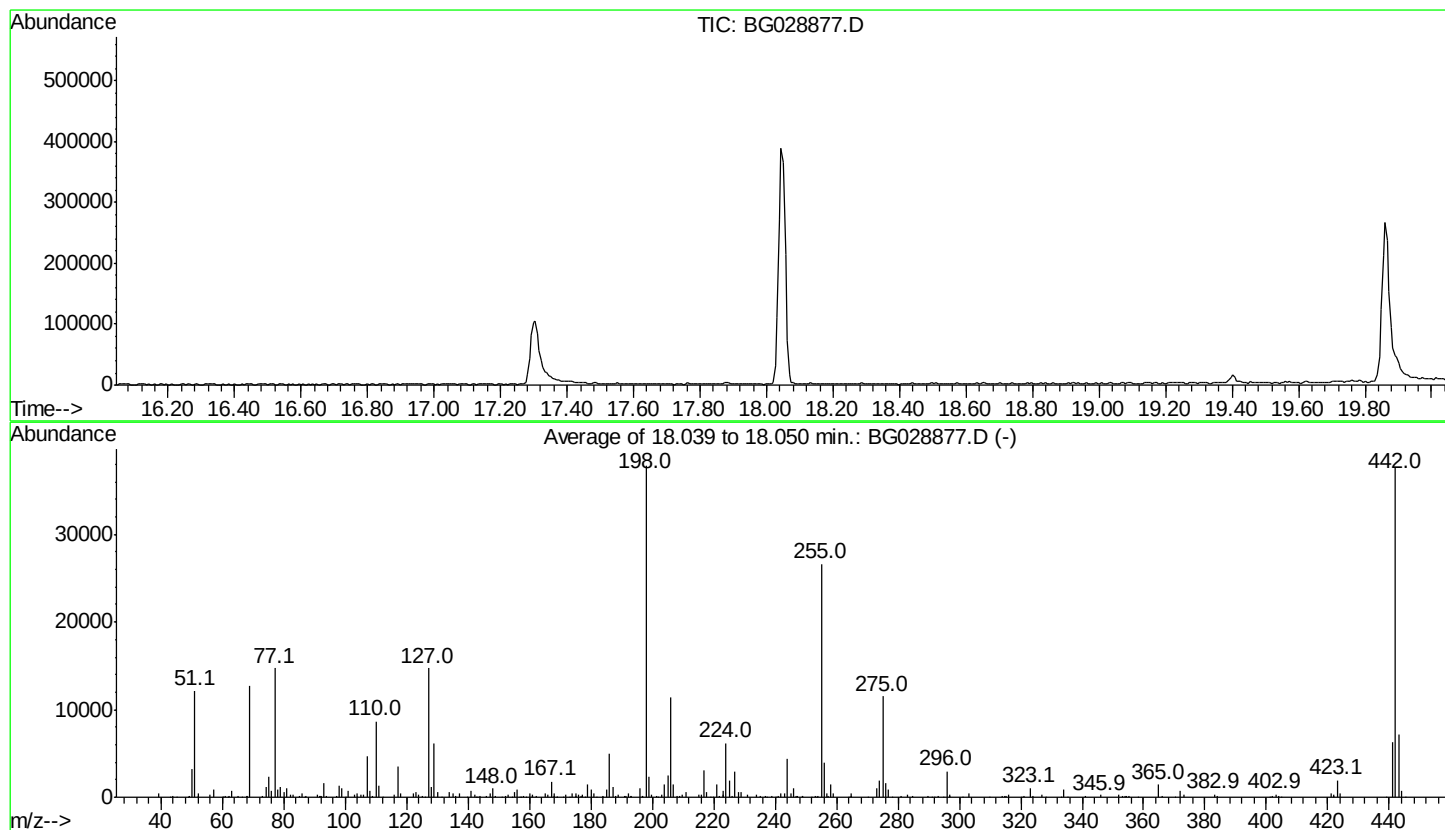

AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	12127	PASS
68	69	0.00	2	0.8	99	PASS
69	198	0.00	100	33.5	12664	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.9	14722	PASS
197	198	0.00	2	0.5	185	PASS
198	198	100	100	100.0	37842	PASS
199	198	5	9	6.3	2377	PASS
275	198	10	60	30.4	11509	PASS
365	198	1	100	3.8	1435	PASS
441	442	0.01	24	16.6	6271	PASS
442	198	50	100	99.6	37704	PASS
443	442	15	24	19.1	7183	PASS