
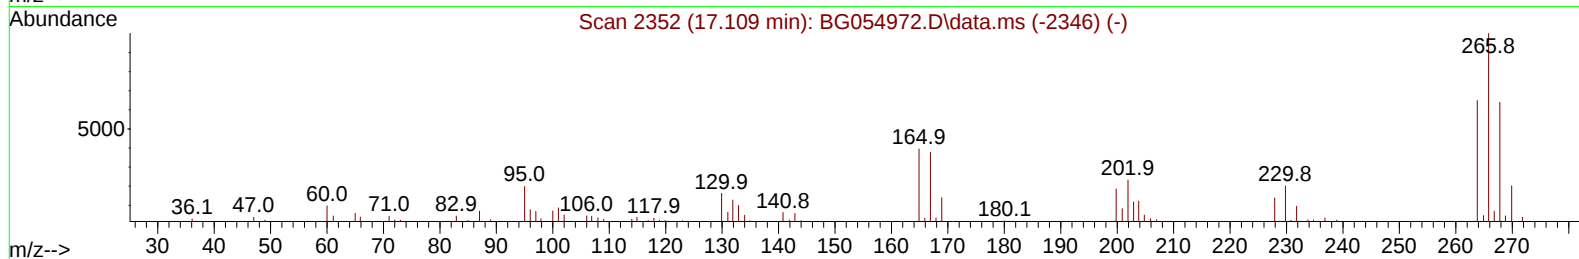
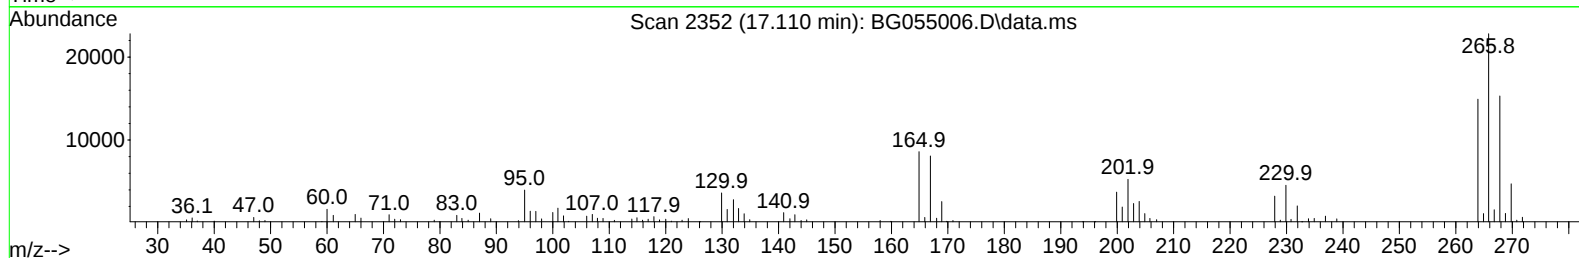


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092222\
Data File : BG055006.D
Acq On : 22 Sep 2022 11:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 23 04:12:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 19 17:41:40 2022
Response via : Initial Calibration

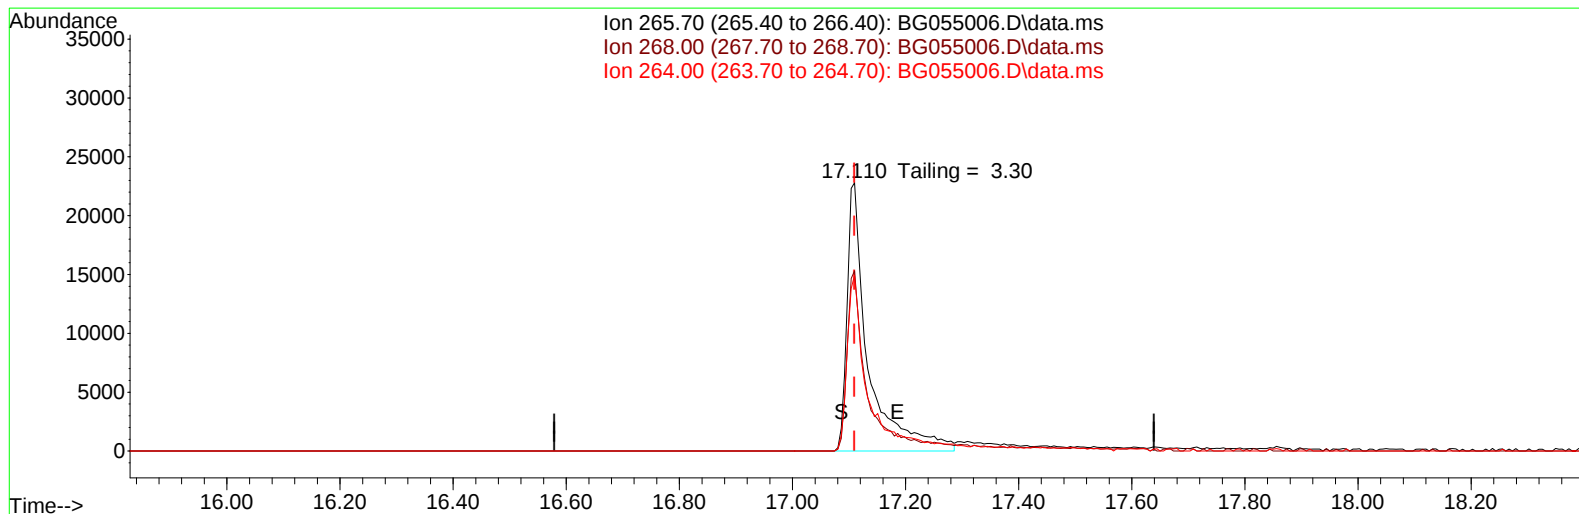

TIC: BG055006.D\data.ms

(70) Pentachlorophenol (C)




17.110min (+ 0.001) 3109.79 ng

response 59443

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	67.12
264.00	61.70	65.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092222\
Data File : BG055006.D
Acq On : 22 Sep 2022 11:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 23 04:12:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 19 17:41:40 2022
Response via : Initial Calibration

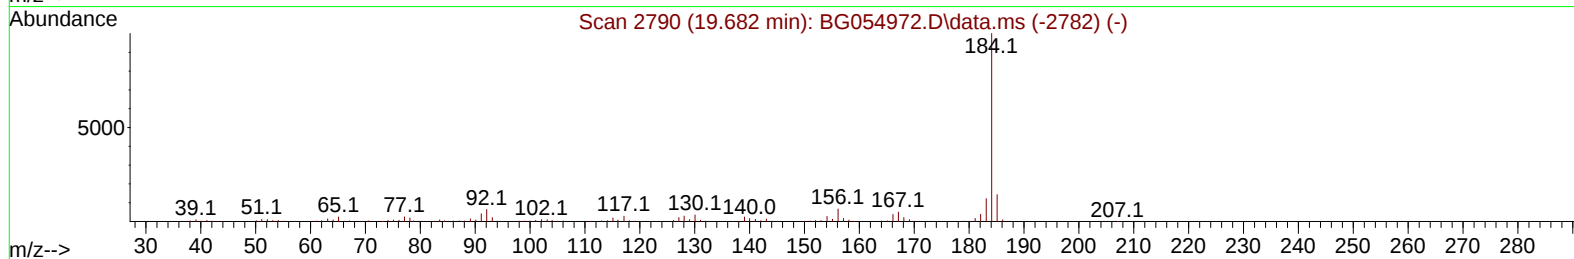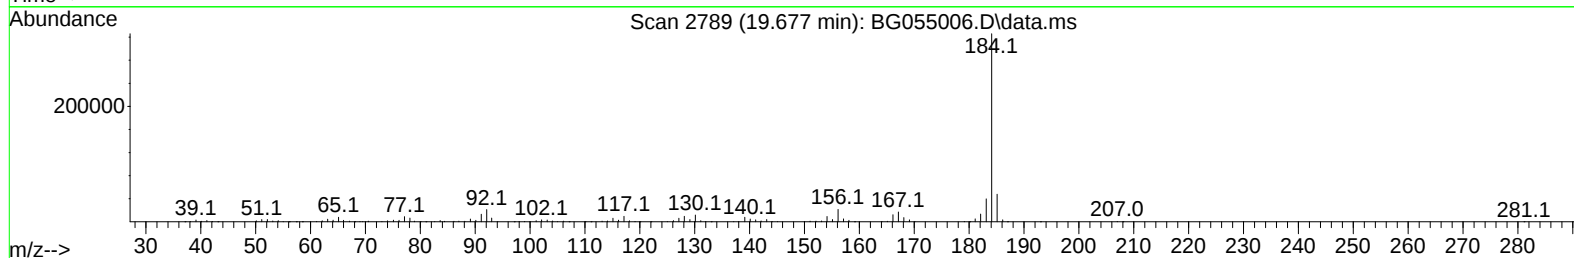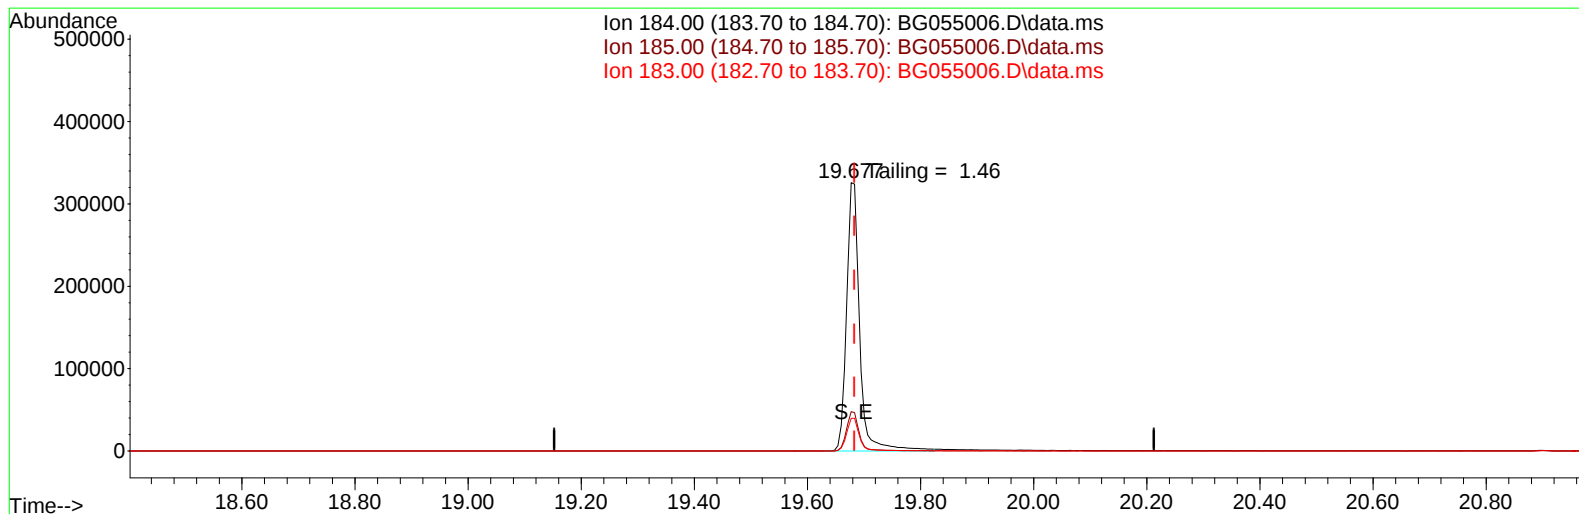

TIC: BG055006.D\data.ms

(77) Benzidine

19.677min (-0.005) 0.00 ng

response 532613

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.68
183.00	12.30	12.18
0.00	0.00	0.00