

Data Path : Z:\HPCHEM1\BNA G\DATA\BG092315\
 Data File : BG018859.D
 Acq On : 23 Sep 2015 20:15
 Operator : UM/NP
 Sample : G3690-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BC2W4

Quant Time: Sep 24 04:13:44 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG091015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 24 04:11:41 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.00	152	70582	20.00	ng/ul	0.00
18) Naphthalene-d8	10.80	136	312285	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.62	164	211566	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.37	188	543937	20.00	ng/ul	0.00
78) Chrysene-d12	21.62	240	596256	20.00	ng/ul	0.00
86) Perylene-d12	24.81	264	600049	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.44	96	5953	4.05	ng/uL	0.00
5) Phenol-d5	7.16	99	132334	22.83	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.32	67	76465	22.77	ng/ul	0.00
9) 2-Chlorophenol-d4	7.53	132	106301	24.22	ng/ul	0.00
13) 4-Methylphenol-d8	8.70	113	109466	23.28	ng/ul	0.00
19) Nitrobenzene-d5	9.15	128	56709	23.97	ng/ul	0.00
22) 2-Nitrophenol-d4	9.88	143	61035	25.65	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.42	165	118804	23.72	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	160448	27.53	ng/ul	0.00
44) Dimethylphthalate-d6	14.03	166	394452	23.17	ng/ul	0.00
47) Acenaphthylene-d8	14.32	160	489745	24.27	ng/ul	0.00
52) 4-Nitrophenol-d4	14.82	143	65784	20.13	ng/ul	0.00
58) Fluorene-d10	15.62	176	355603	23.88	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.74	200	38394	14.91	ng/ul	0.00
71) Anthracene-d10	17.47	188	543832	22.71	ng/ul	0.00
79) Pyrene-d10	19.75	212	602422	21.96	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.59	264	602833	20.64	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.07	163	176081	10.67	ng/ul#	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG092315\
Data File : BG018859.D
Acq On : 23 Sep 2015 20:15
Operator : UM/NP
Sample : G3690-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BC2W4

Quant Time: Sep 24 04:13:44 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG091015.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 24 04:11:41 2015
Response via : Initial Calibration

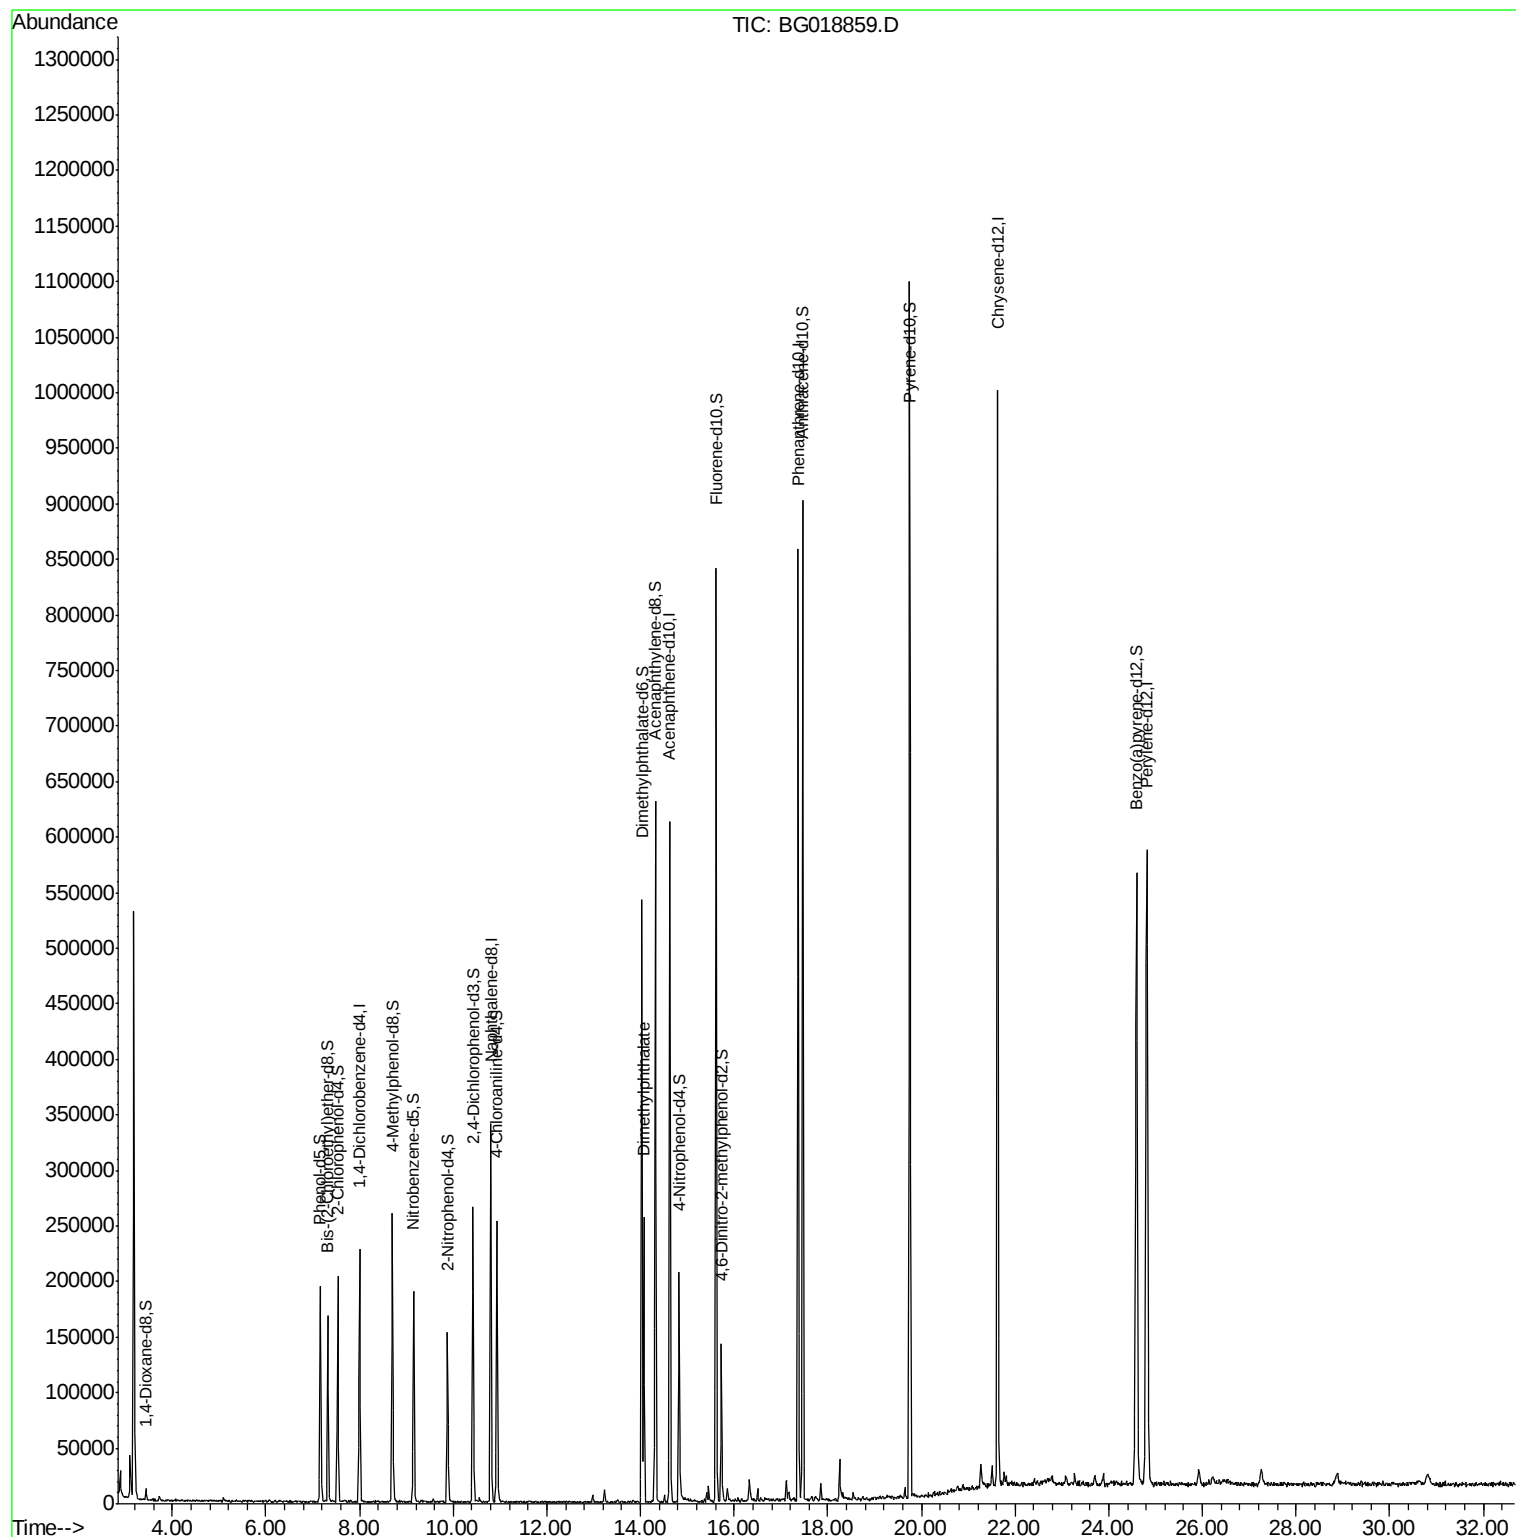

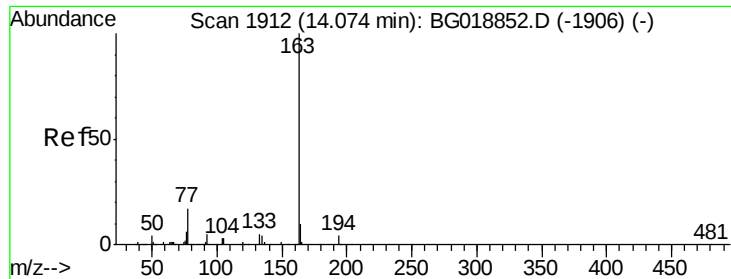

#45
 Dimethylphthalate
 Concen: 10.67 ng/ul
 RT: 14.07 min Scan# 1912
 Delta R.T. -0.00 min
 Lab File: BG018859.D
 Acq: 23 Sep 2015 20:15

Instrument :
 BNA_G
 ClientSampleId :
 BC2W4

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.4	2.9	4.3#
164	9.3	7.7	11.5

