
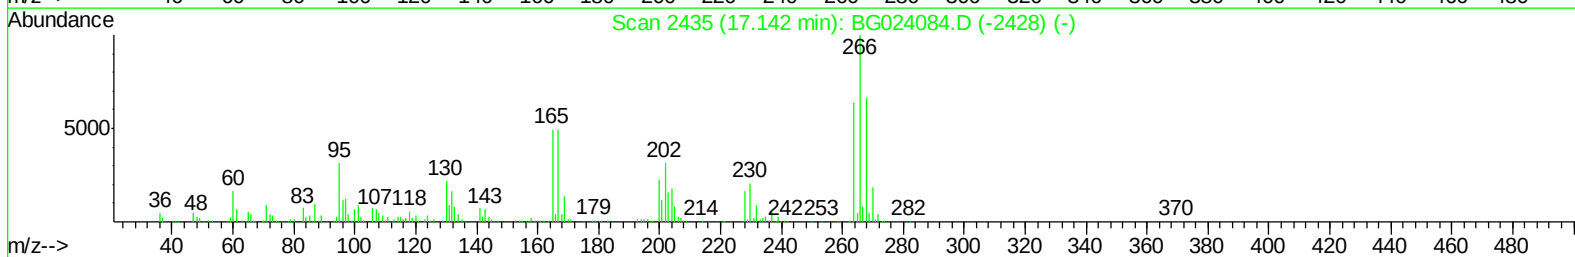
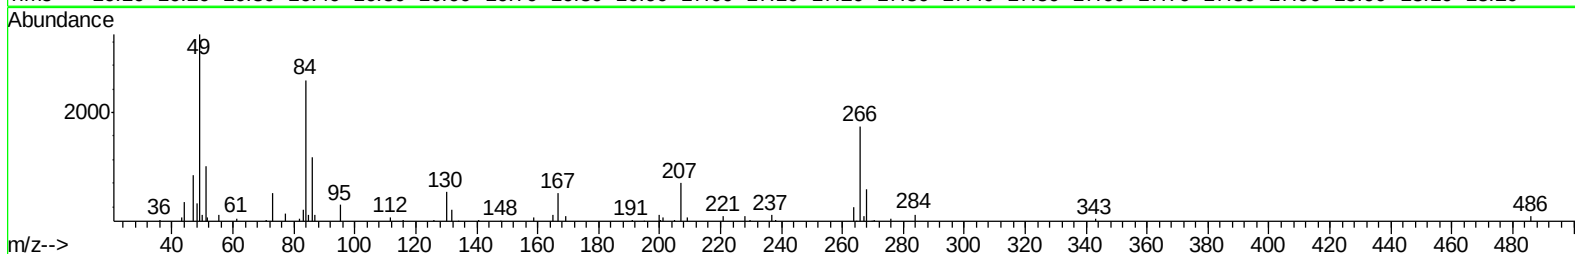


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG092316\
Data File : BG024080.D
Acq On : 23 Sep 2016 10:12
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 01:51:42 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG092316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 23 15:35:28 2016
Response via : Initial Calibration

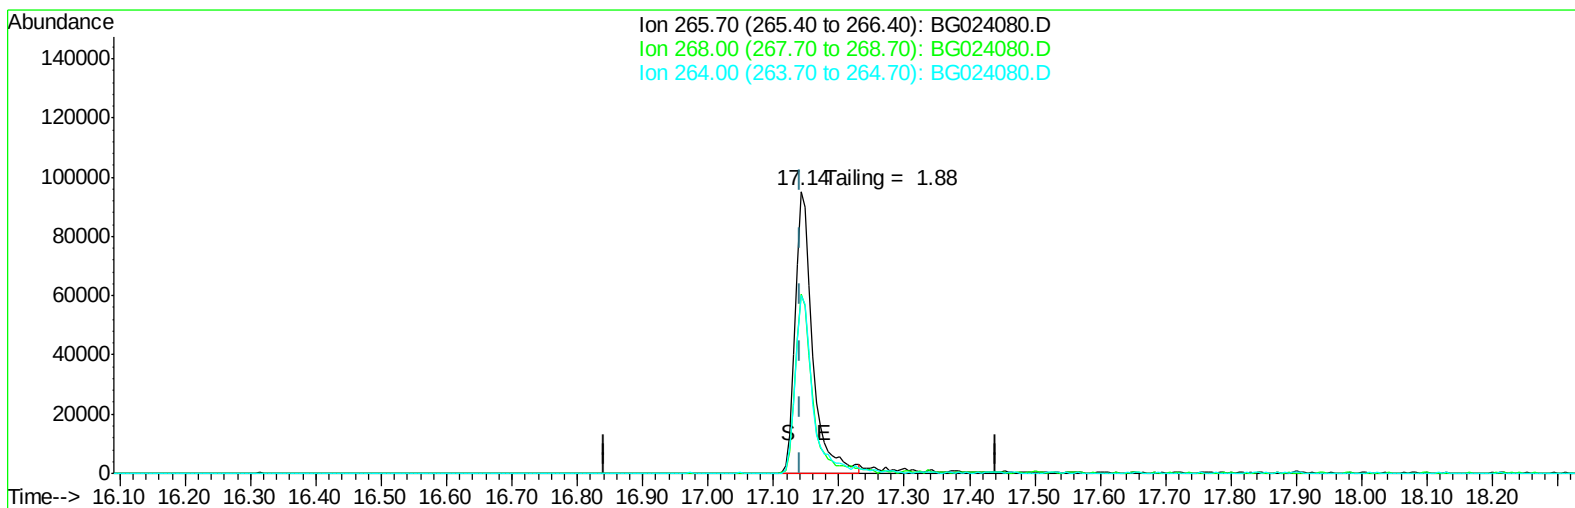

TIC: BG024080.D

(69) Pentachlorophenol (C)




17.301min (+0.159) 3311.27ng

response 1407

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	40.16#
264.00	63.20	8.73#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG092316\
Data File : BG024080.D
Acq On : 23 Sep 2016 10:12
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 01:51:42 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG092316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 23 15:35:28 2016
Response via : Initial Calibration

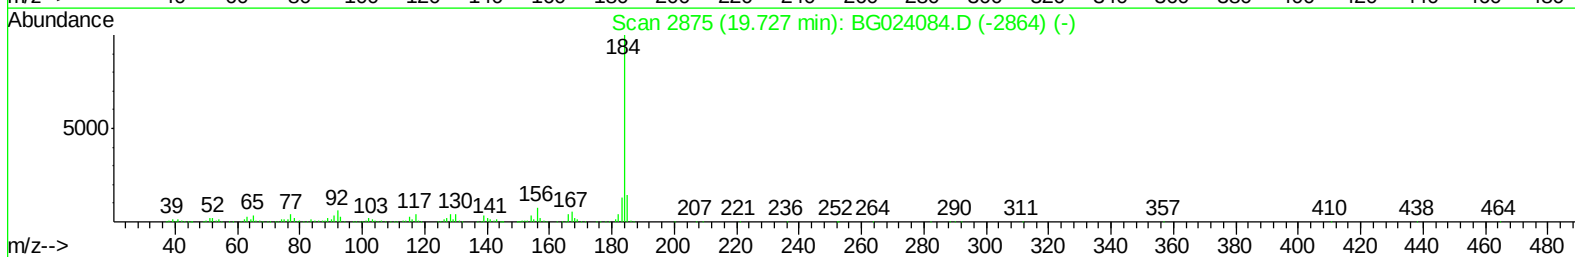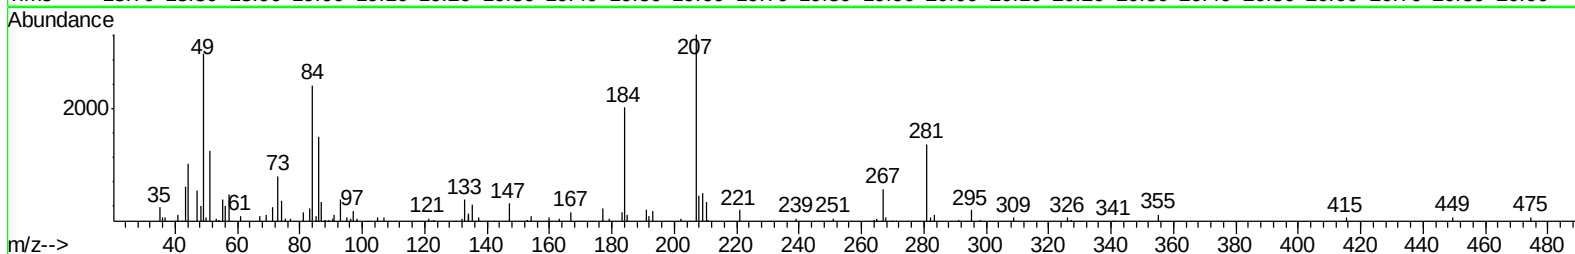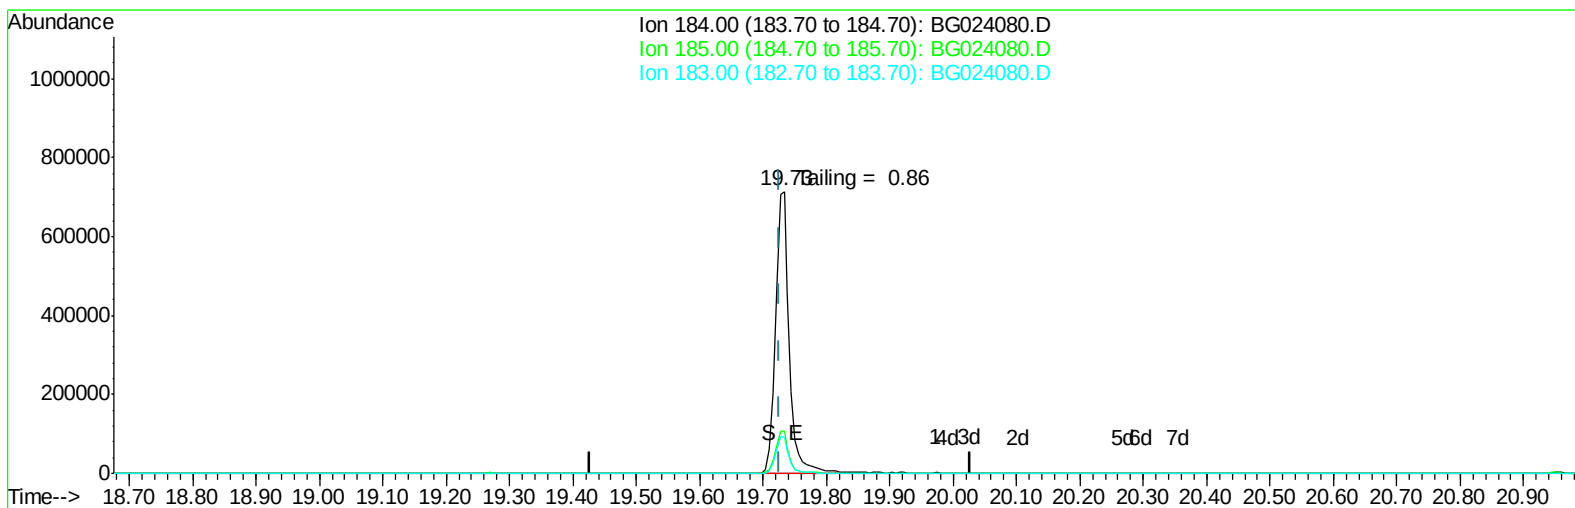

TIC: BG024080.D

(76) Benzidine

19.974min (+0.247) 632.01ng

response 984

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	12.75
183.00	13.40	14.77
0.00	0.00	0.00