
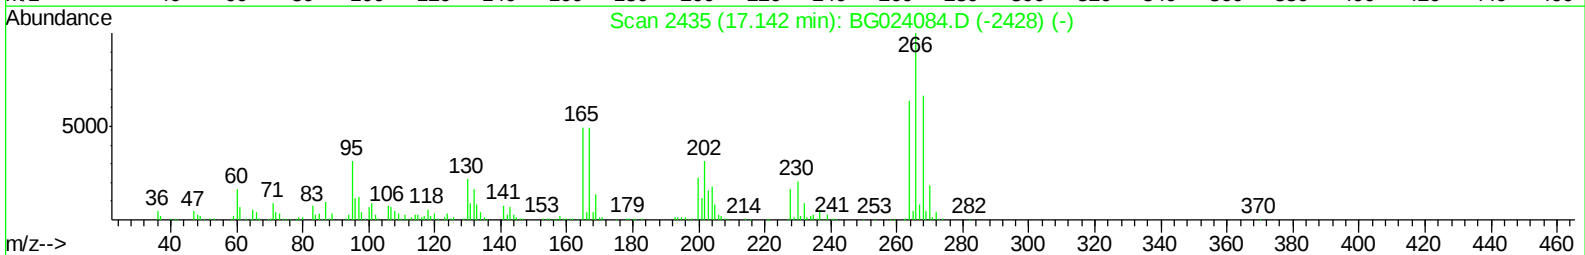
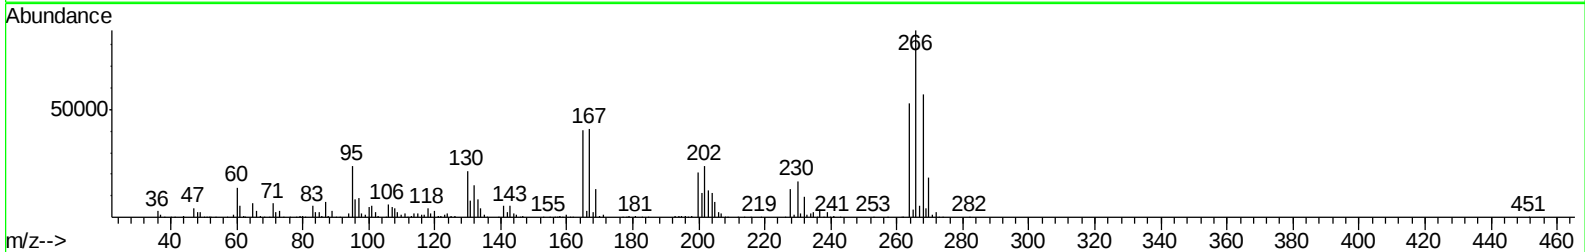


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG092316\
Data File : BG024089.D
Acq On : 23 Sep 2016 16:13
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 01:54:11 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG092316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 23 15:35:28 2016
Response via : Initial Calibration

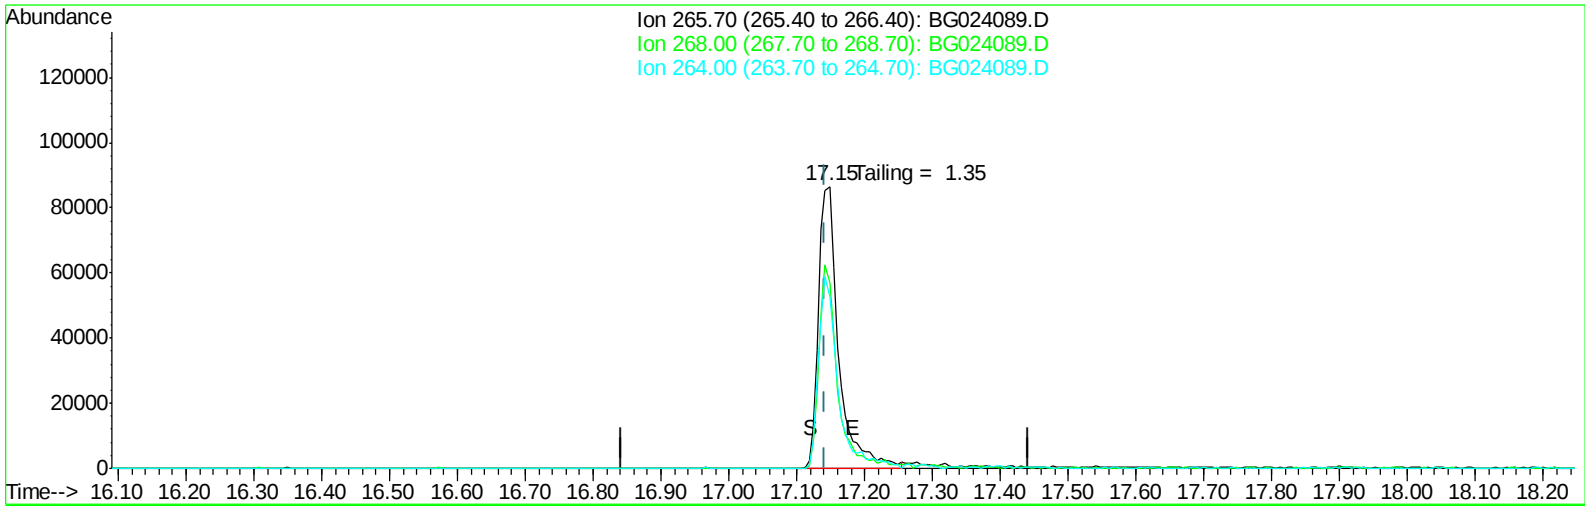

TIC: BG024089.D

(69) Pentachlorophenol (C)




17.148min (+0.006) 411320.53ng

response 174962

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	65.92
264.00	63.20	60.86
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG092316\
Data File : BG024089.D
Acq On : 23 Sep 2016 16:13
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 01:54:11 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG092316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 23 15:35:28 2016
Response via : Initial Calibration

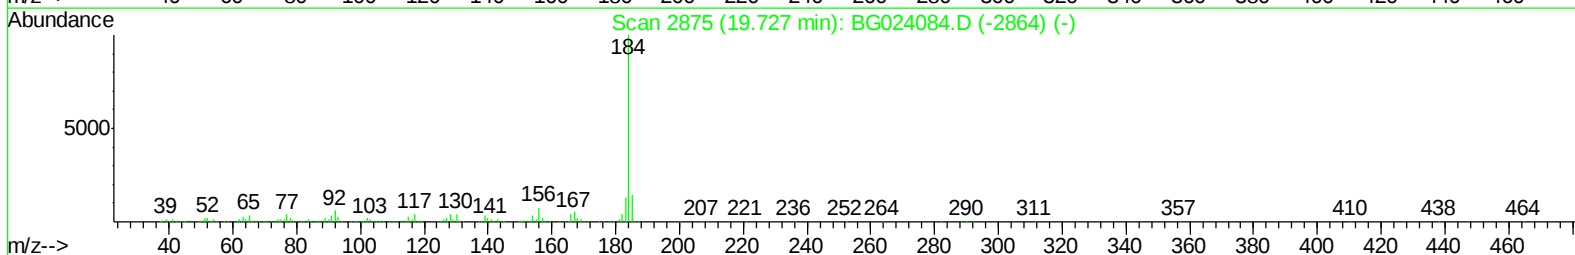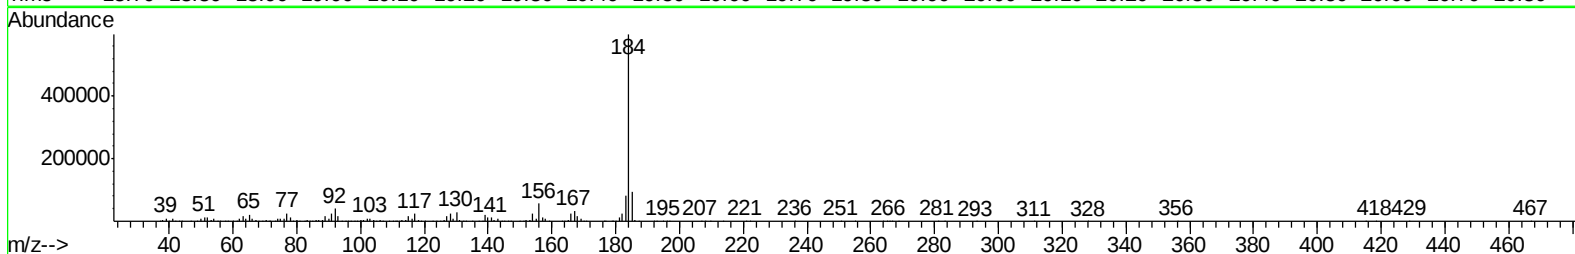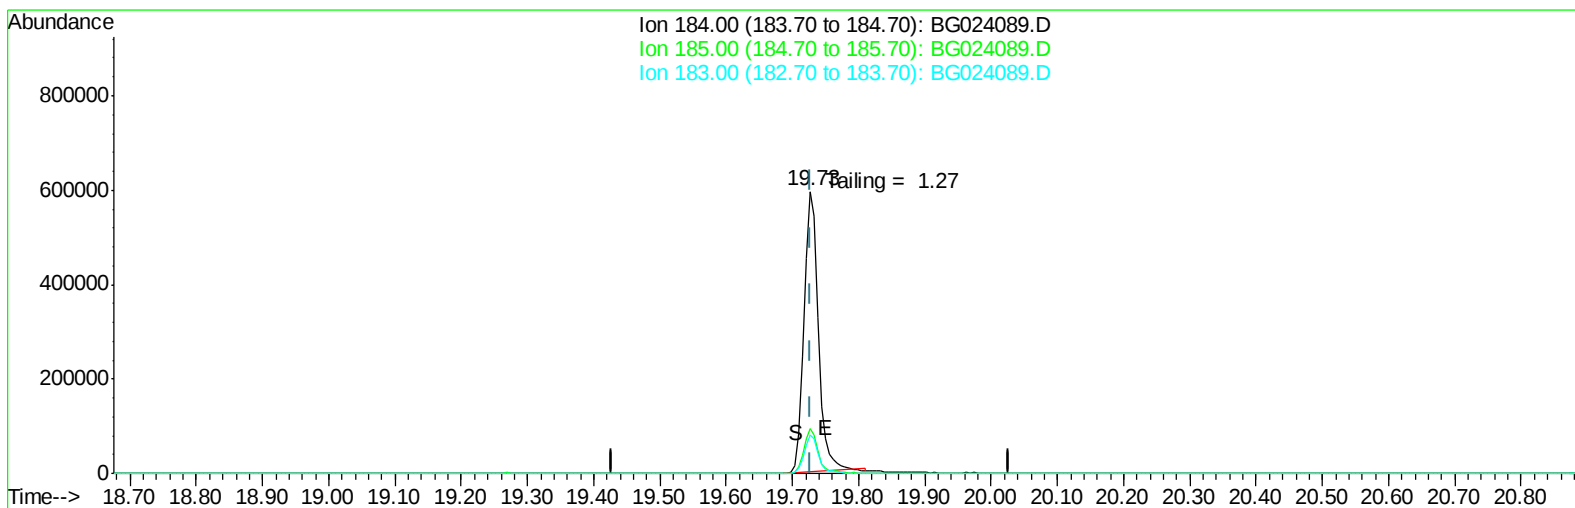

TIC: BG024089.D

(76) Benzidine

19.727min (-0.000) 385821.49ng

response 950191

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	15.88
183.00	13.40	13.56
0.00	0.00	0.00