
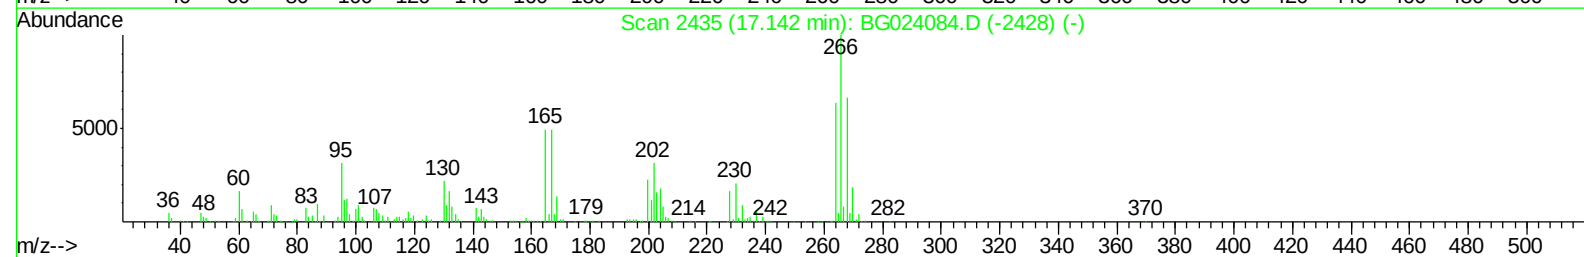
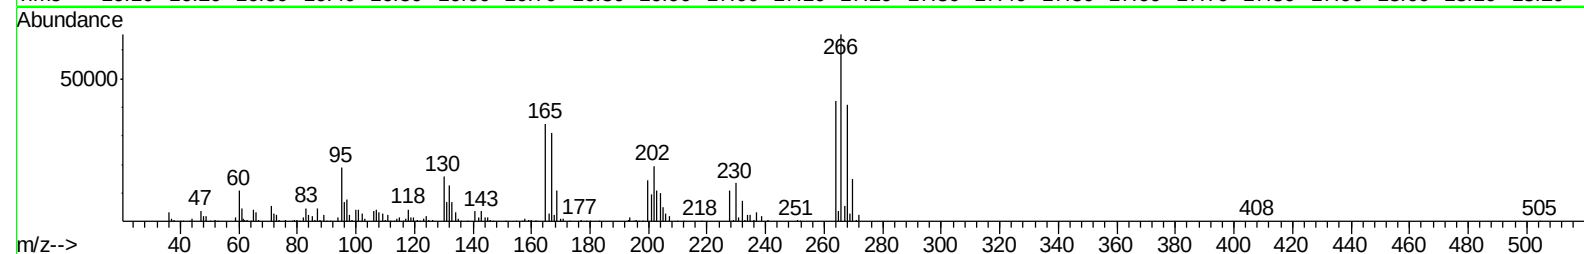


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG092316\
Data File : BG024106.D
Acq On : 24 Sep 2016 3:05
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 01:55:00 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG092316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 23 15:35:28 2016
Response via : Initial Calibration

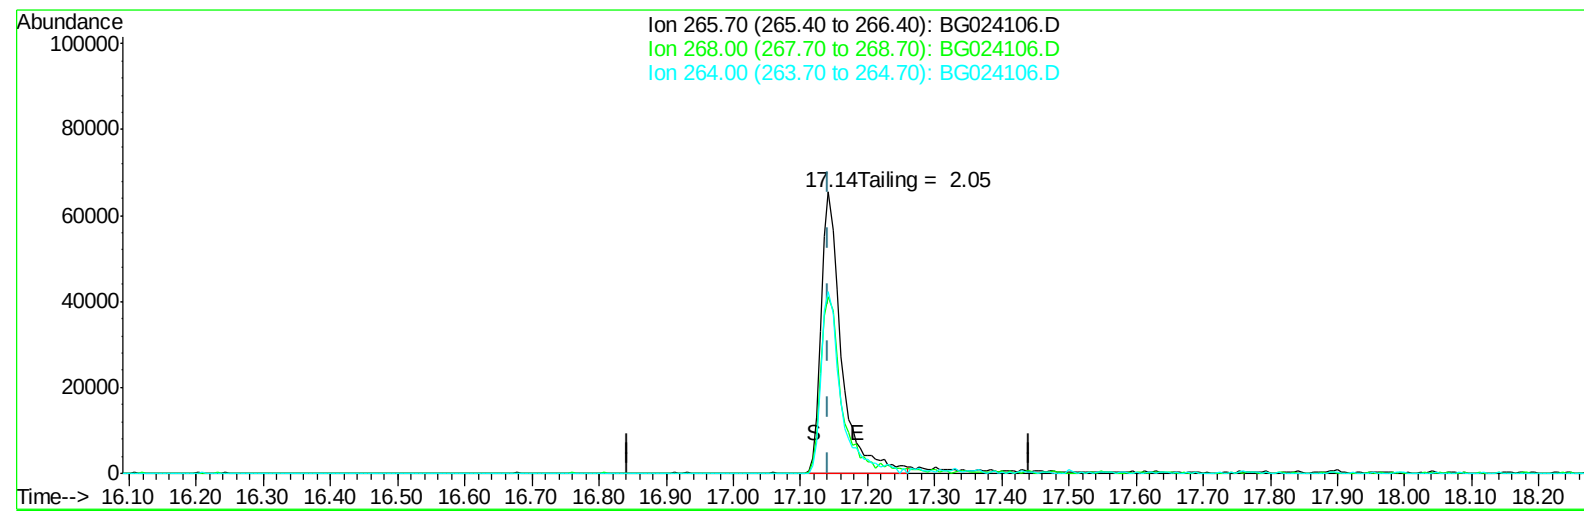

TIC: BG024106.D

(69) Pentachlorophenol (C)




17.142min (-0.000) 93310.85ng

response 136931

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	62.73
264.00	63.20	64.64
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG092316\
 Data File : BG024106.D
 Acq On : 24 Sep 2016 3:05
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 01:55:00 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG092316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 23 15:35:28 2016
 Response via : Initial Calibration

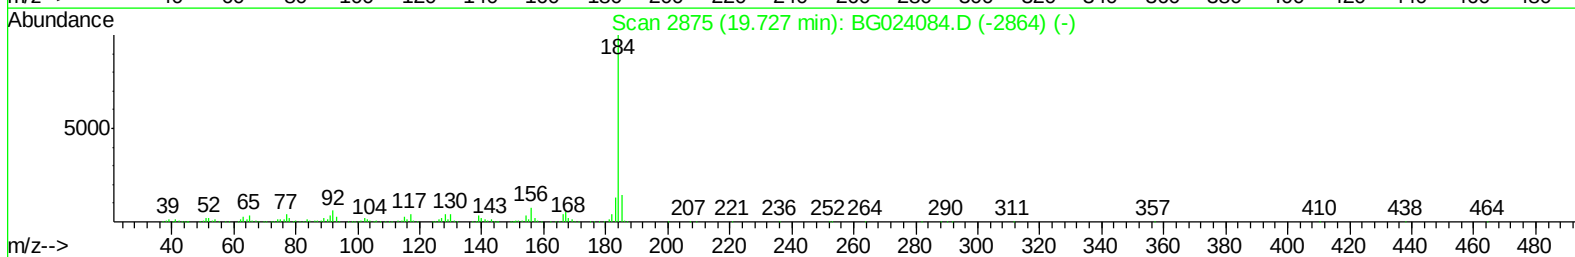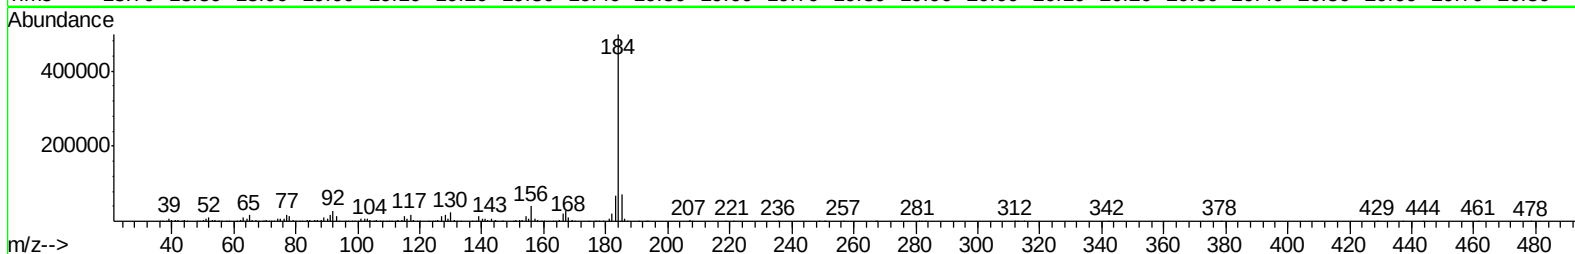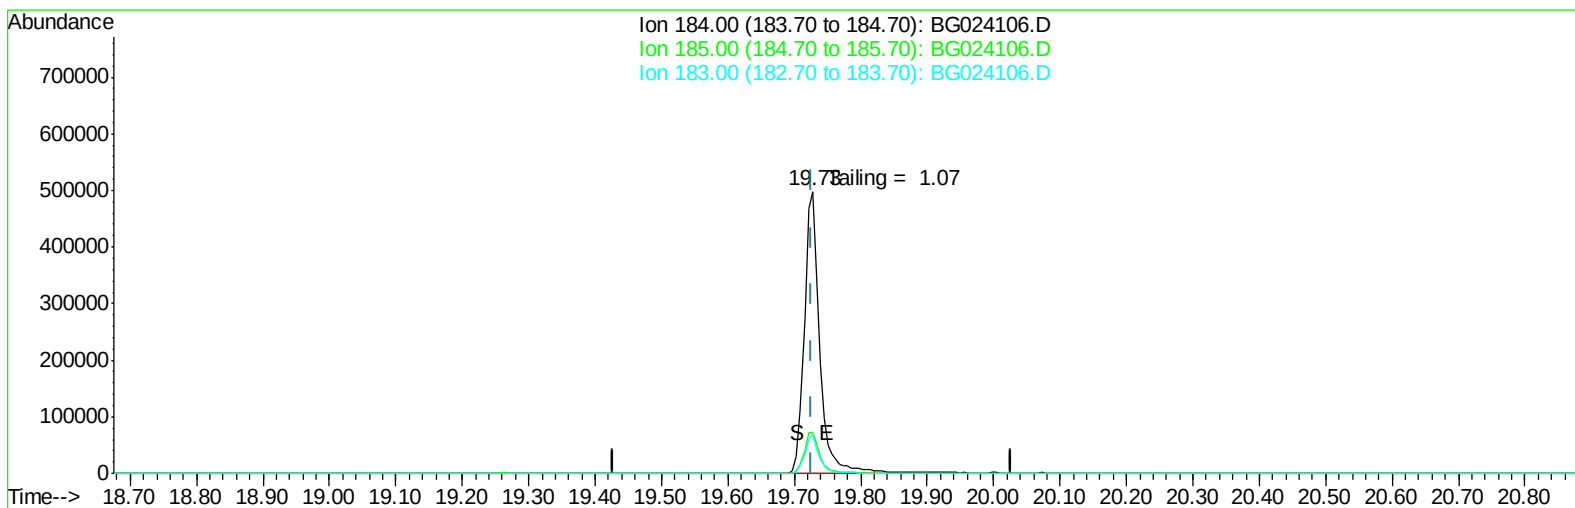

TIC: BG024106.D

(76) Benzidine

19.727min (-0.000) 41667.49ng

response 793812

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	14.40
183.00	13.40	13.44
0.00	0.00	0.00