


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG092316\
 Data File : BG024080.D
 Acq On : 23 Sep 2016 10:12
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG092316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 23 15:35:28 2016

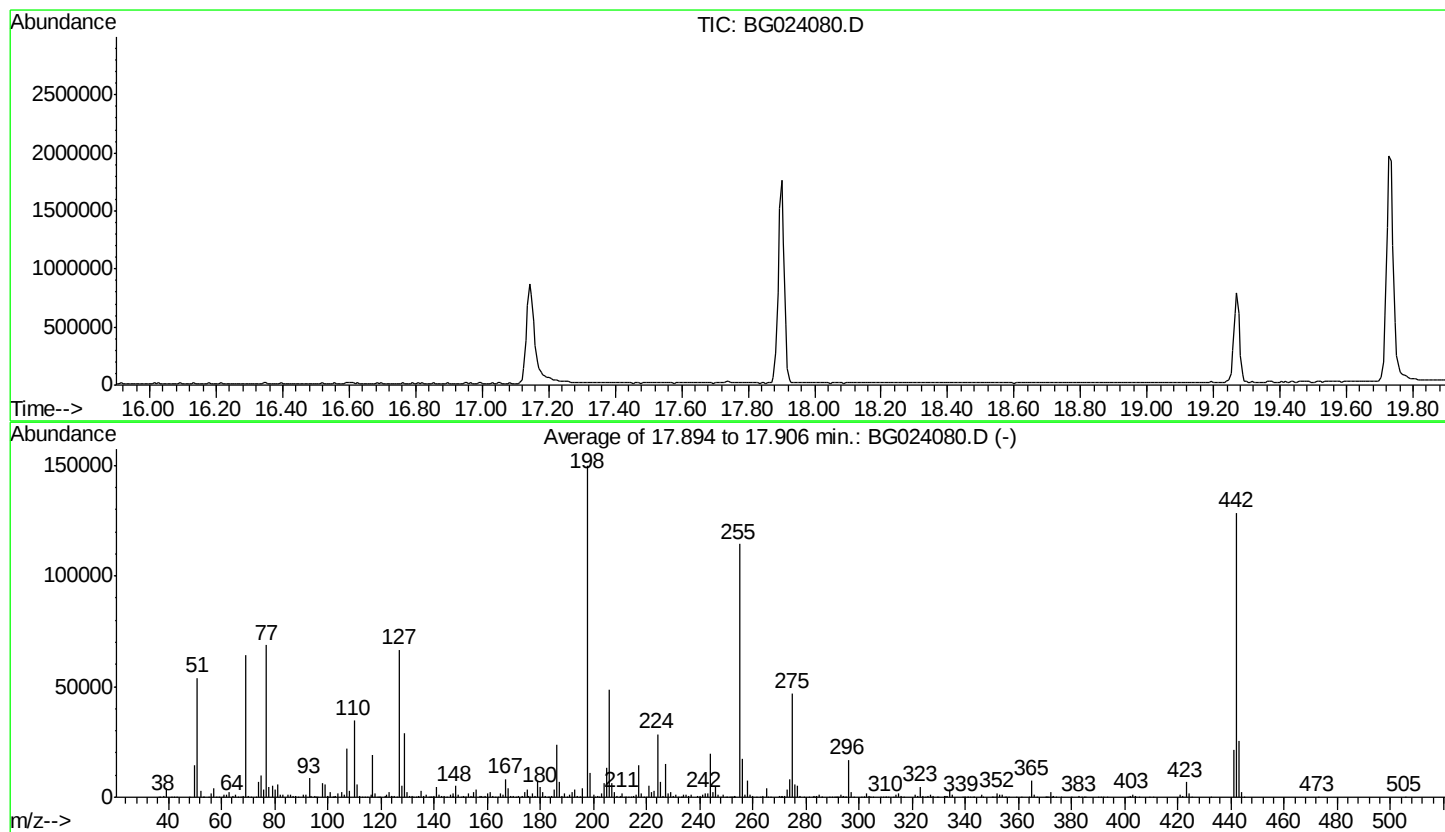

AutoFind: Scans 2563, 2564, 2565; Background Corrected with Scan 2555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	54061	PASS
68	69	0.00	2	1.1	706	PASS
69	198	0.00	100	43.0	64509	PASS
70	69	0.00	2	0.6	369	PASS
127	198	10	80	44.4	66584	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	149848	PASS
199	198	5	9	7.5	11292	PASS
275	198	10	60	31.1	46634	PASS
365	198	1	100	4.9	7398	PASS
441	442	0.01	24	16.7	21504	PASS
442	198	50	100	85.7	128448	PASS
443	442	15	24	19.9	25616	PASS