


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG092316\
Data File : BG024089.D
Acq On : 23 Sep 2016 16:13
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG092316.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Sep 23 15:35:28 2016

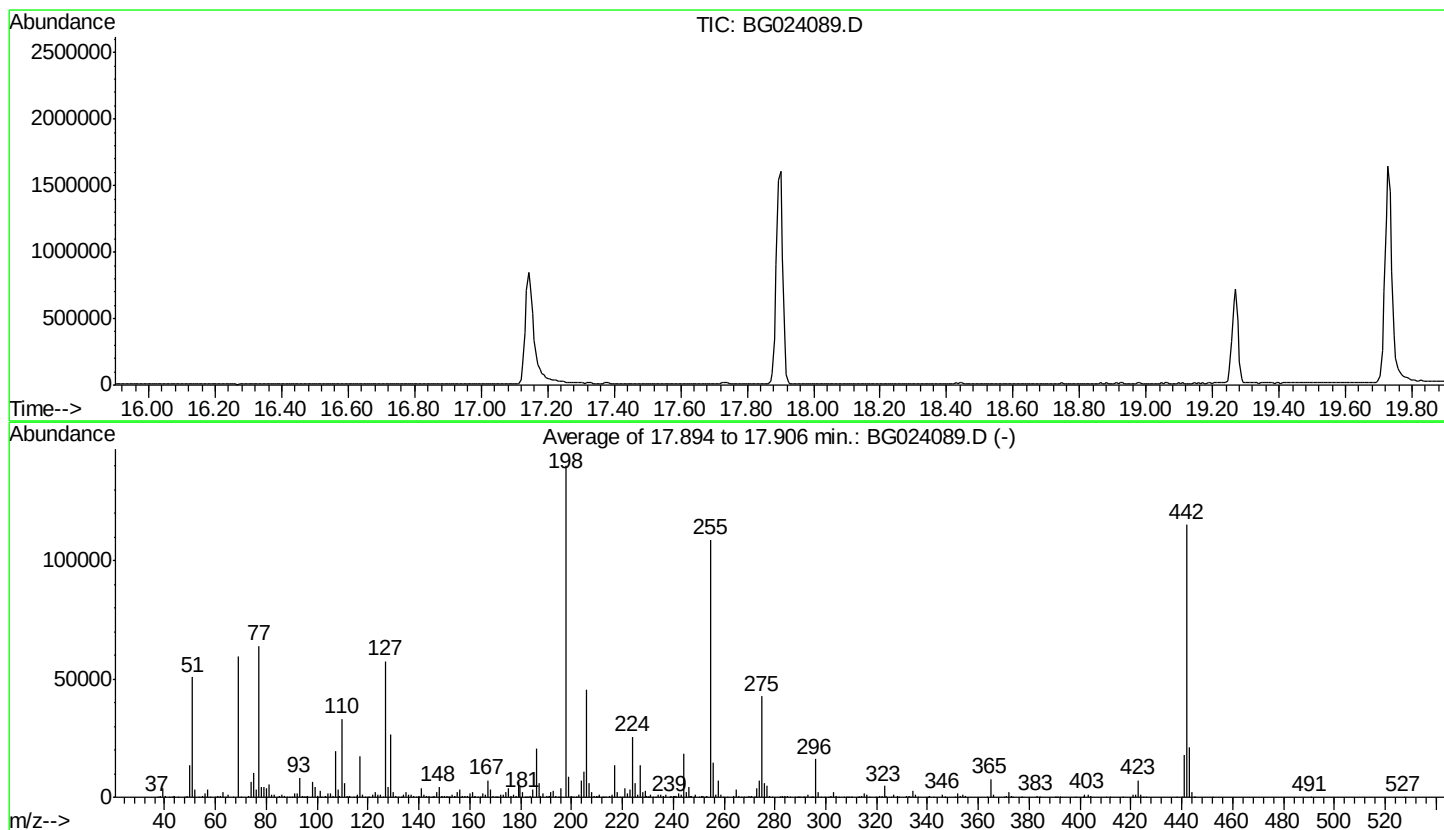

AutoFind: Scans 2563, 2564, 2565; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	50812	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.4	59413	PASS
70	69	0.00	2	0.2	106	PASS
127	198	10	80	41.0	57418	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	140072	PASS
199	198	5	9	6.0	8439	PASS
275	198	10	60	30.4	42522	PASS
365	198	1	100	5.5	7666	PASS
441	442	0.01	24	15.5	17846	PASS
442	198	50	100	82.1	114970	PASS
443	442	15	24	18.2	20933	PASS