


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG092316\
Data File : BG024125.D
Acq On : 24 Sep 2016 15:12
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG092316.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Sep 23 15:35:28 2016

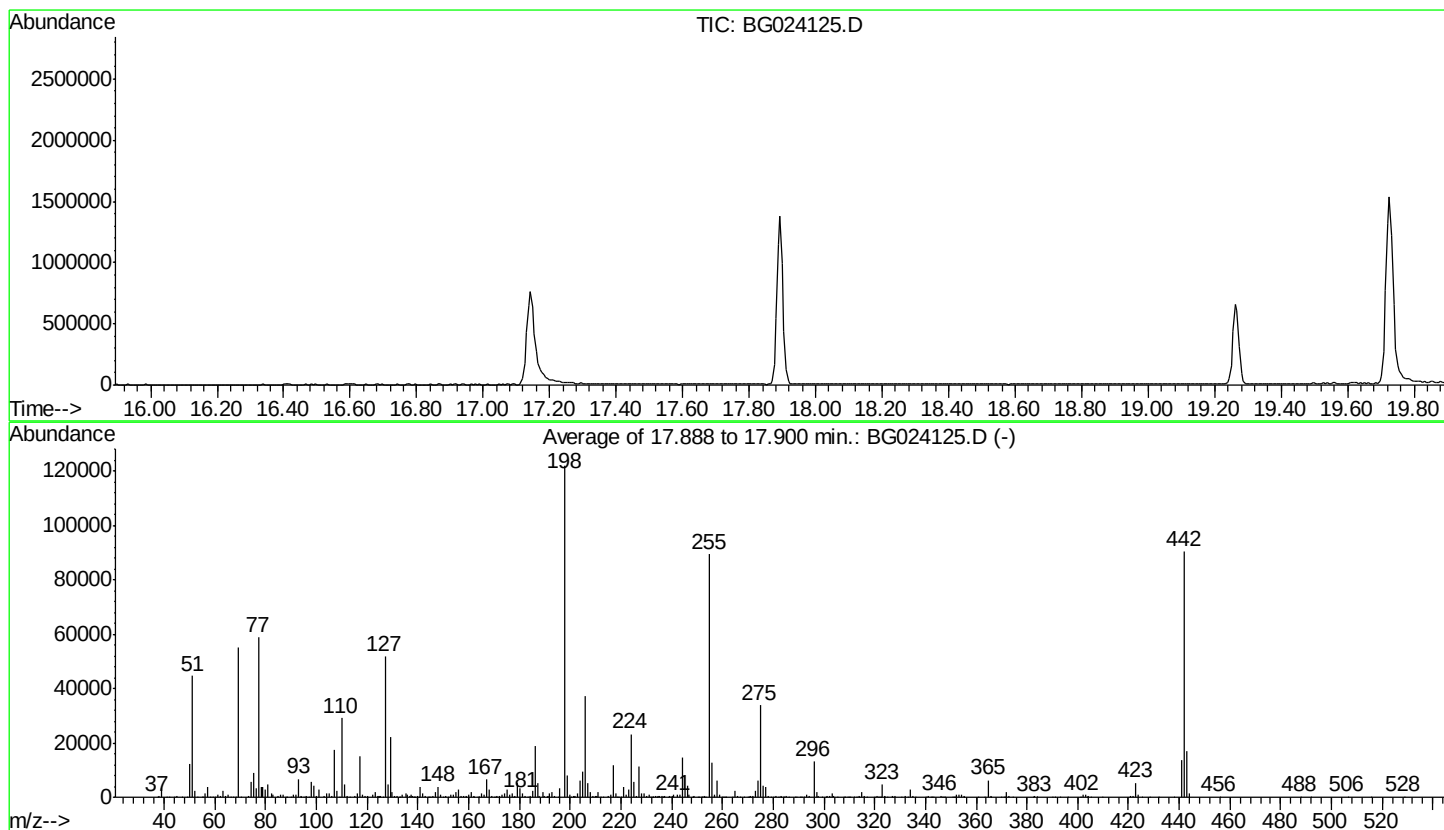

AutoFind: Scans 2562, 2563, 2564; Background Corrected with Scan 2555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	44618	PASS
68	69	0.00	2	0.4	234	PASS
69	198	0.00	100	45.0	54925	PASS
70	69	0.00	2	0.3	155	PASS
127	198	10	80	42.4	51810	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	122090	PASS
199	198	5	9	6.6	8005	PASS
275	198	10	60	27.7	33762	PASS
365	198	1	100	5.0	6138	PASS
441	442	0.01	24	15.2	13754	PASS
442	198	50	100	73.9	90282	PASS
443	442	15	24	19.0	17184	PASS