


Data Path : Z:\HPCHEM1\BNA G\Data\BG092317\
 Data File : BG028890.D
 Acq On : 23 Sep 2017 8:59
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 12 16:57:11 2017

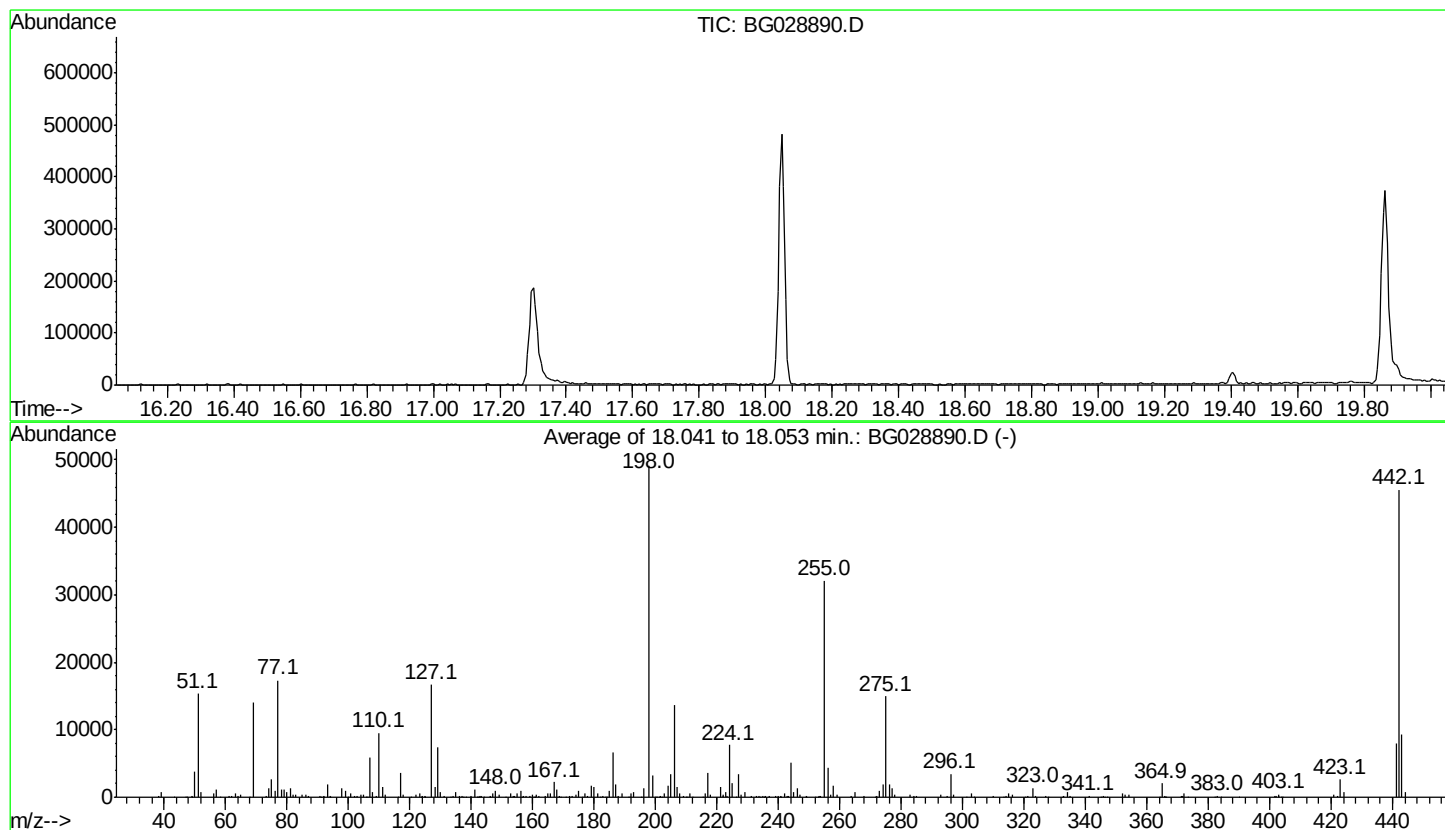

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.2	15343	PASS
68	69	0.00	2	0.4	62	PASS
69	198	0.00	100	28.5	14000	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	33.8	16604	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	49138	PASS
199	198	5	9	6.7	3279	PASS
275	198	10	60	30.4	14926	PASS
365	198	1	100	4.1	2009	PASS
441	442	0.01	24	17.6	8006	PASS
442	198	50	100	92.7	45541	PASS
443	442	15	24	20.3	9232	PASS