
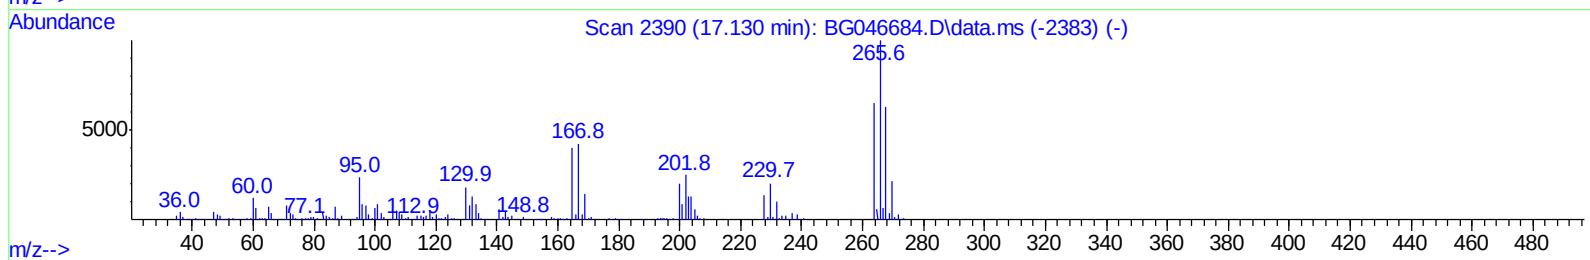
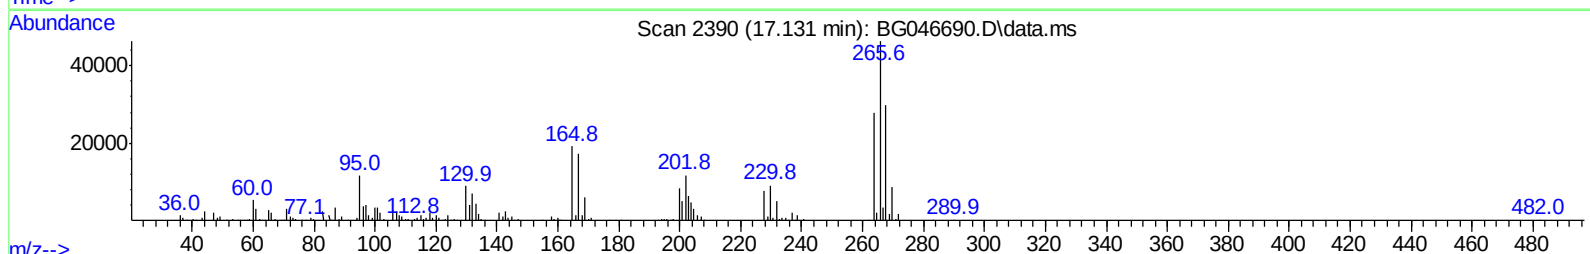


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092320\
Data File : BG046690.D
Acq On : 23 Sep 2020 12:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 24 05:33:36 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 22 21:47:28 2020
Response via : Initial Calibration

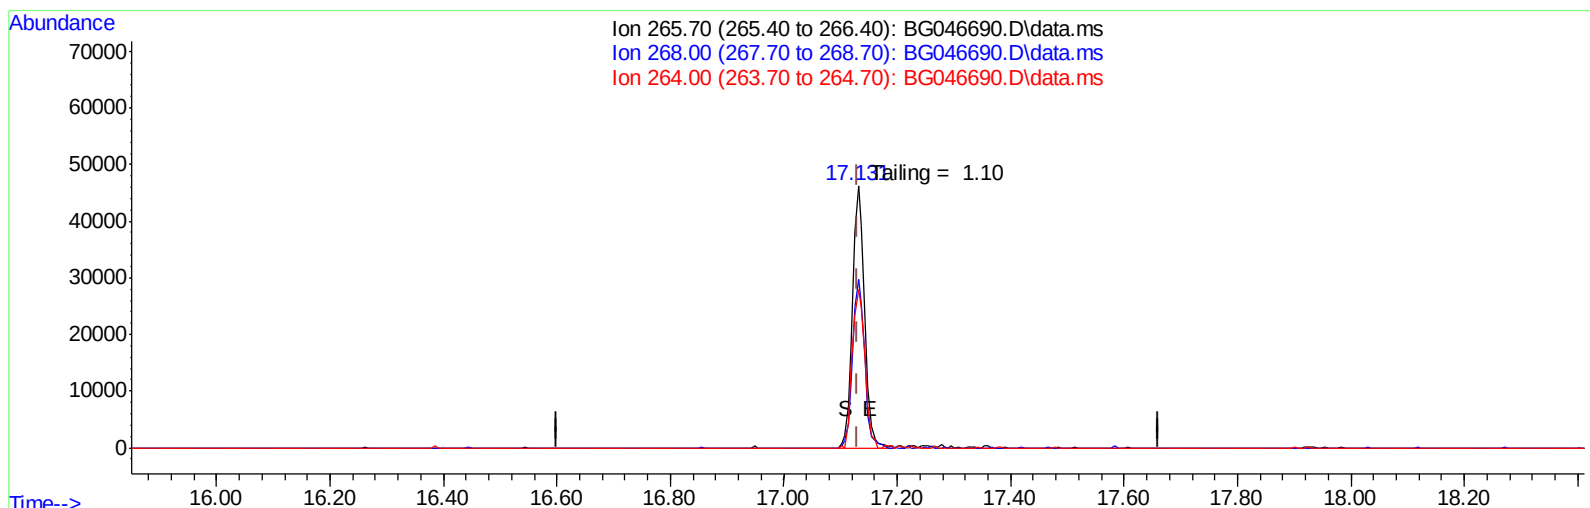

TIC: BG046690.D\data.ms

(70) Pentachlorophenol (C)




17.131min (+ 0.001) 157066.48 ng

response 67794

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.31
264.00	61.60	64.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092320\
Data File : BG046690.D
Acq On : 23 Sep 2020 12:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 24 05:33:36 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 22 21:47:28 2020
Response via : Initial Calibration

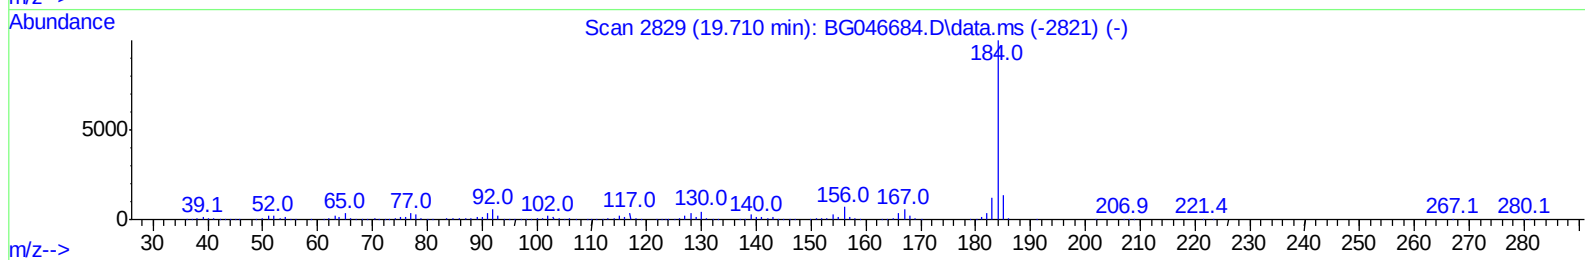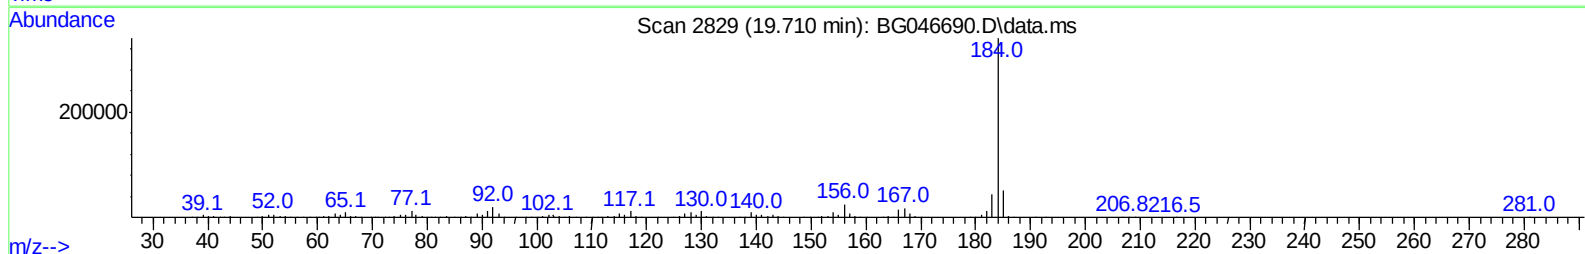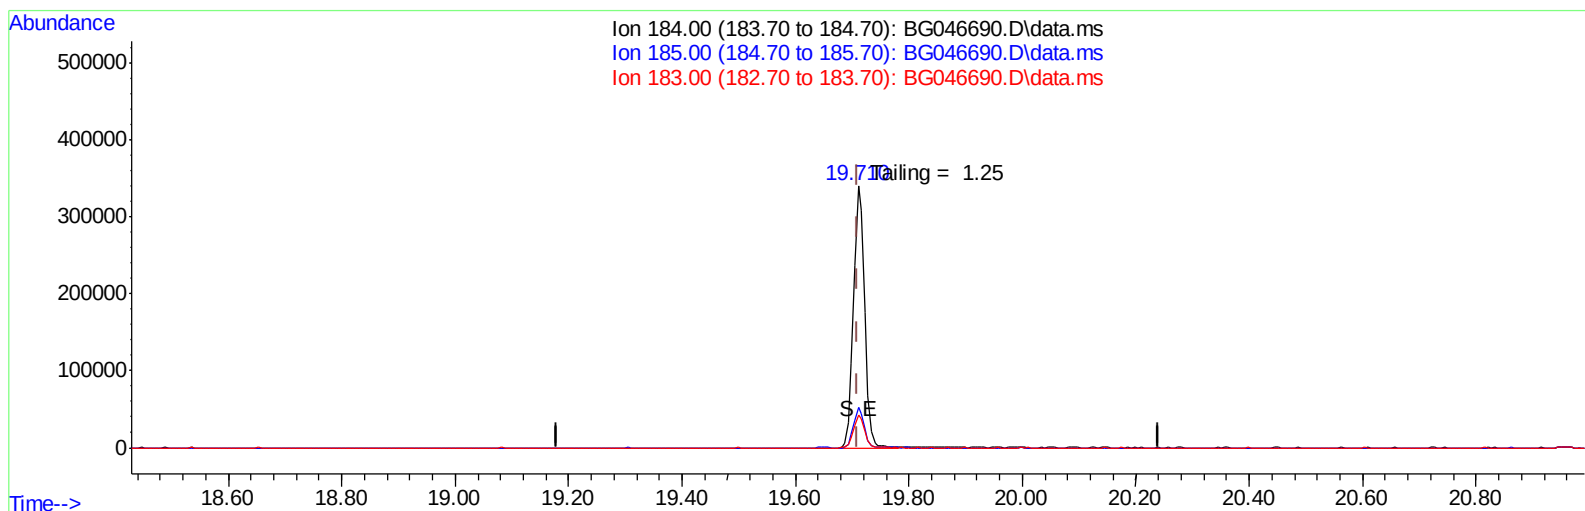

TIC: BG046690.D\data.ms

(77) Benzidine

19.710min (+ 0.001) 15281.96 ng

response 463064

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.32
183.00	13.20	12.62
0.00	0.00	0.00