
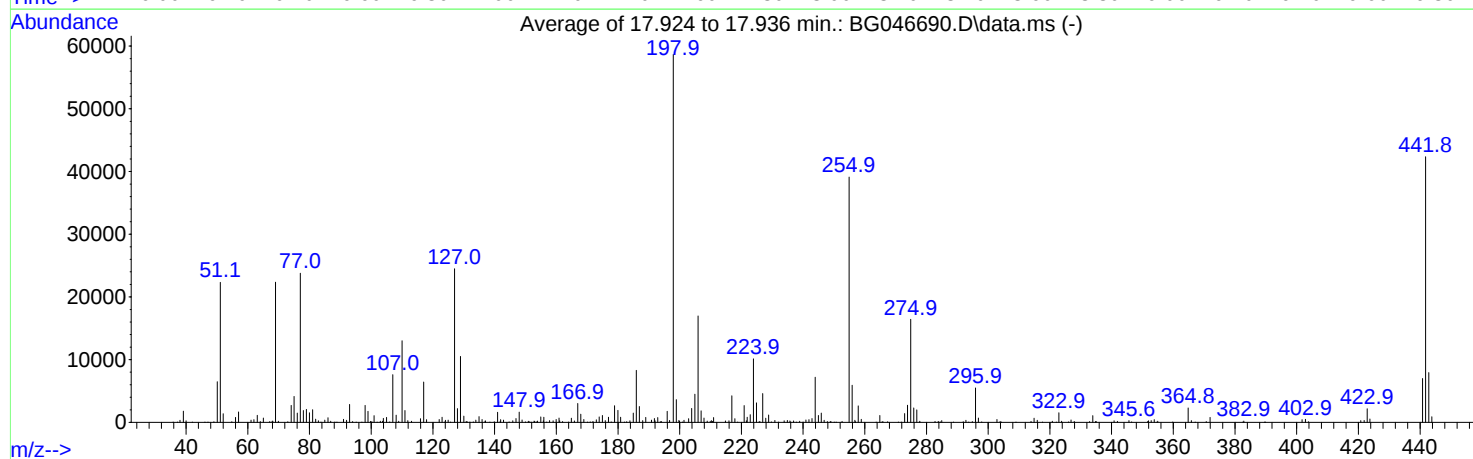


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092320\
 Data File : BG046690.D
 Acq On : 23 Sep 2020 12:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 22 21:47:28 2020

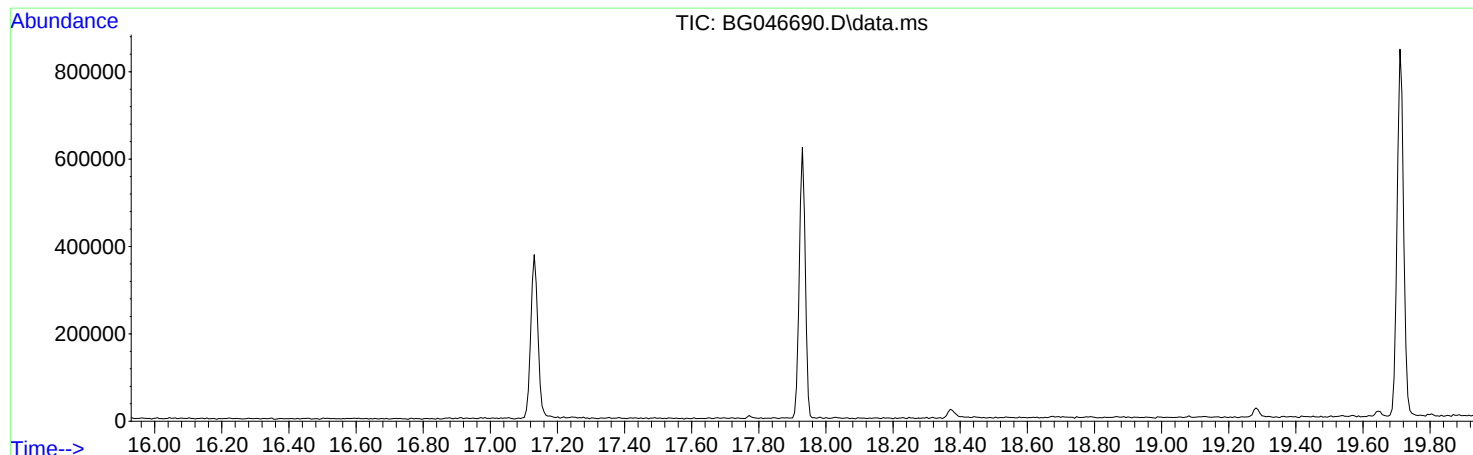

AutoFind: Scans 2525, 2526, 2527; Background Corrected with Scan 2518

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.1	22333	PASS
68	69	0.00	2	0.9	208	PASS
69	198	0.00	100	38.1	22352	PASS
70	69	0.00	2	0.9	192	PASS
127	198	10	80	41.7	24485	PASS
197	198	0.00	2	0.5	302	PASS
198	198	100	100	100.0	58656	PASS
199	198	5	9	6.2	3612	PASS
275	198	10	60	28.0	16426	PASS
365	198	1	100	3.9	2293	PASS
441	198	0.01	100	11.9	6992	PASS
442	198	50	100	72.2	42360	PASS
443	442	15	24	18.7	7924	PASS