
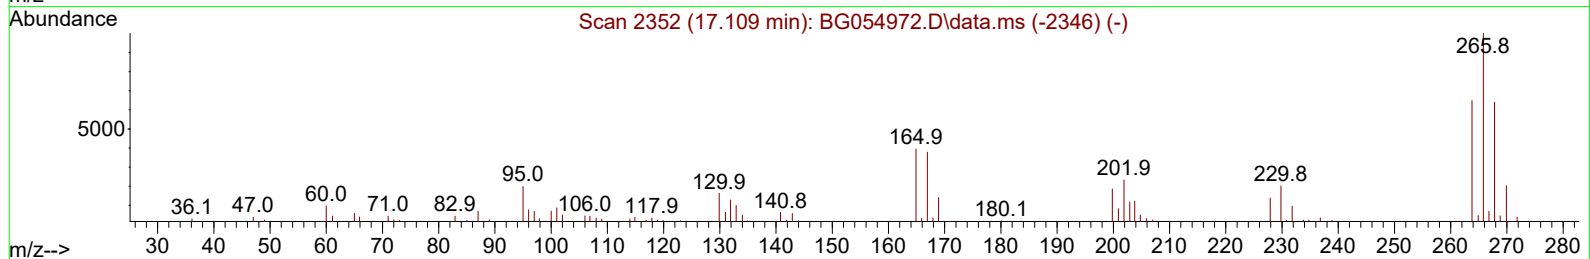
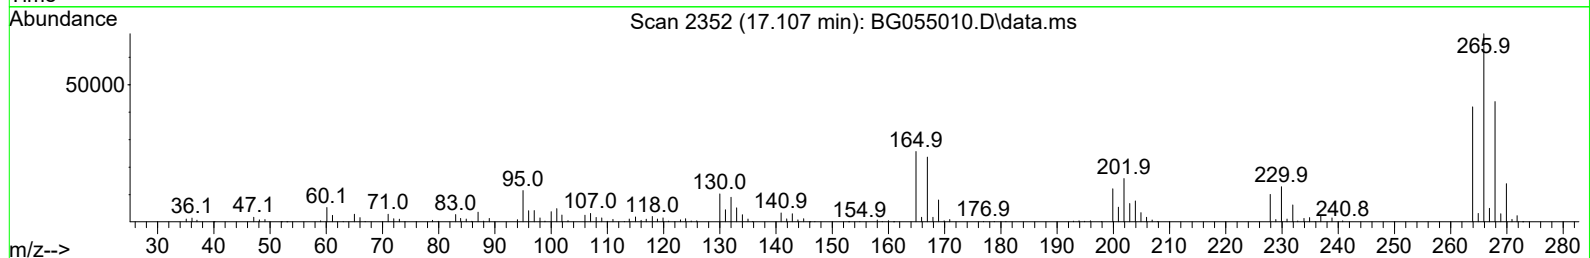


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092322\
Data File : BG055010.D
Acq On : 23 Sep 2022 12:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 24 04:55:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 19 17:41:40 2022
Response via : Initial Calibration

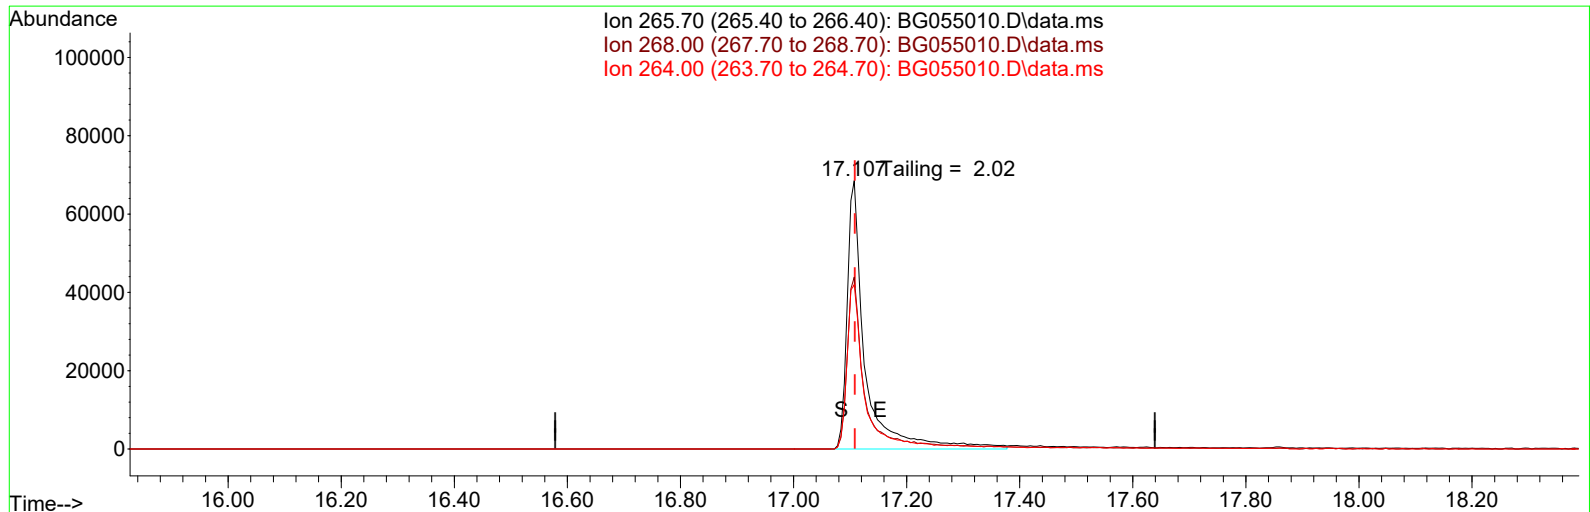

TIC: BG055010.D\data.ms

(70) Pentachlorophenol (C)




17.107min (-0.002) 8893.26 ng

response 152154

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	64.02
264.00	61.70	61.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092322\
Data File : BG055010.D
Acq On : 23 Sep 2022 12:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 24 04:55:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 19 17:41:40 2022
Response via : Initial Calibration

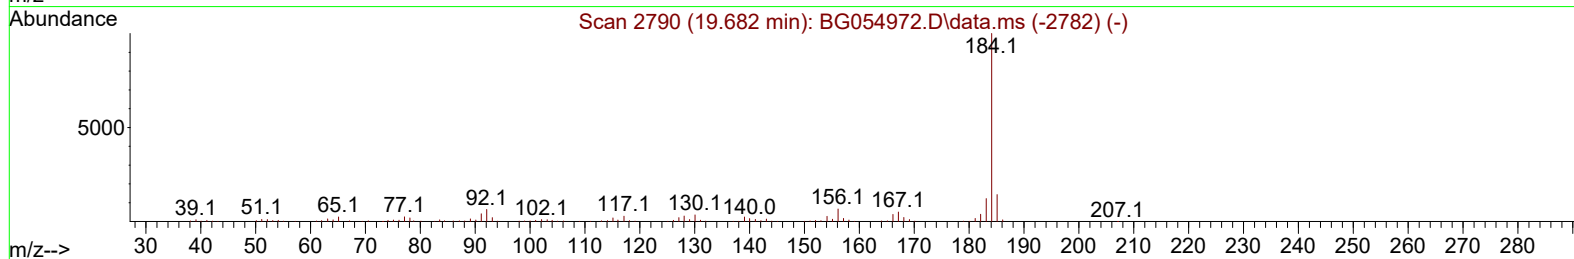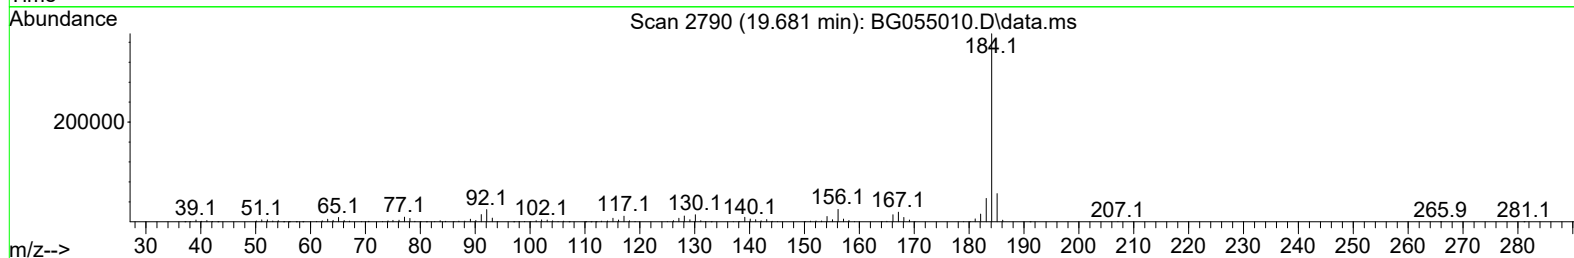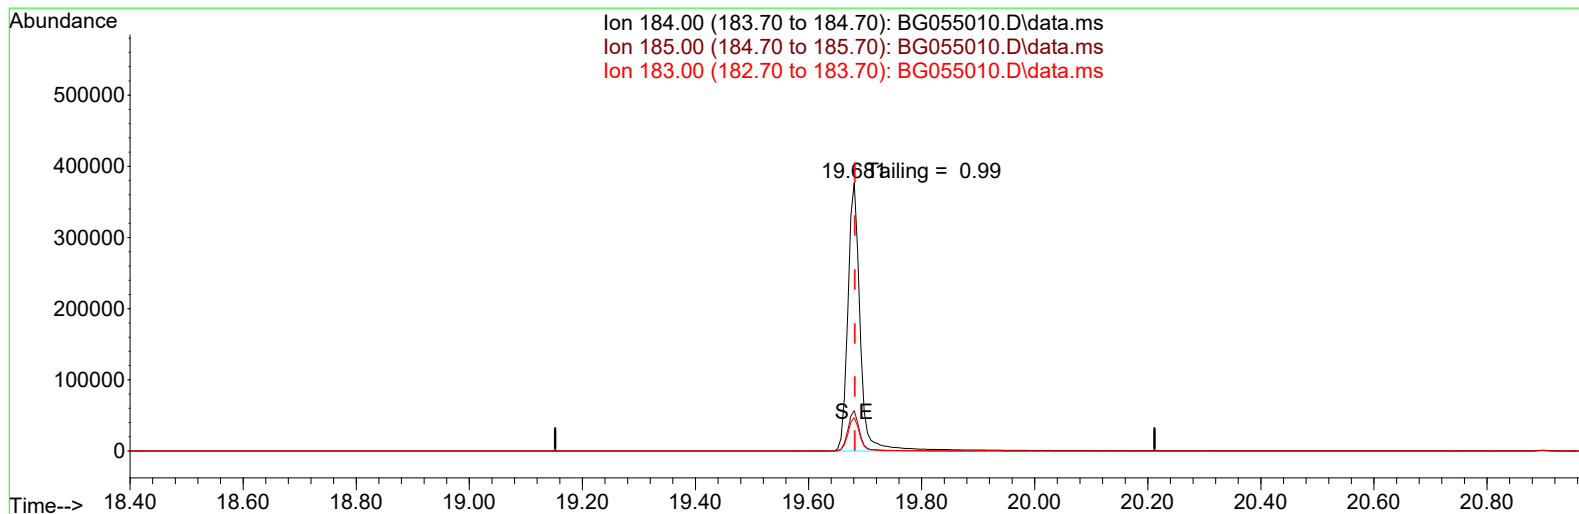

TIC: BG055010.D\data.ms

(77) Benzidine

19.681min (-0.002) 42454.32 ng

response 572203

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	15.05
183.00	12.30	12.43
0.00	0.00	0.00