

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092322\
 Data File : BG055015.D
 Acq On : 23 Sep 2022 16:44
 Operator : CG/JU
 Sample : N4751-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PE-5

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG055015.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.112	304	310	320	rBV	43460	69050	3.53%	0.773%
2	5.600	386	393	406	rBV	379251	621220	31.80%	6.950%
3	7.221	661	669	682	rBV	370776	647213	33.13%	7.241%
4	8.056	804	811	819	rBV	112299	190806	9.77%	2.135%
5	9.237	1004	1012	1025	rBV	216270	399239	20.44%	4.467%
6	10.882	1285	1292	1305	rBV	147252	270853	13.86%	3.030%
7	13.320	1700	1707	1718	rBV	703061	1111943	56.92%	12.440%
8	14.701	1935	1942	1951	rBV	262084	414754	21.23%	4.640%
9	16.193	2189	2196	2218	rBV	428008	753708	38.58%	8.432%
10	17.450	2403	2410	2415	rBV	366092	554177	28.37%	6.200%
11	17.492	2415	2417	2423	rVB	19806	24395	1.25%	0.273%
12	18.085	2514	2518	2523	rBV	23585	27169	1.39%	0.304%
13	19.166	2697	2702	2710	rBV	21397	45257	2.32%	0.506%
14	19.254	2713	2717	2721	rVB	46026	51372	2.63%	0.575%
15	19.383	2734	2739	2744	rVB	32677	39211	2.01%	0.439%
16	19.501	2751	2759	2766	rBV2	48465	99156	5.08%	1.109%
17	19.865	2817	2821	2826	rVB	42423	58673	3.00%	0.656%
18	20.047	2846	2852	2860	rBV	1474618	1953576	100.00%	21.856%
19	20.347	2896	2903	2910	rVB4	8117	23800	1.22%	0.266%
20	21.334	3067	3071	3079	rBV5	22266	45482	2.33%	0.509%
21	21.728	3130	3138	3144	rBV	378450	683365	34.98%	7.645%
22	23.984	3513	3522	3523	rBV2	14368	29442	1.51%	0.329%
23	24.730	3643	3649	3656	rVB2	9419	22007	1.13%	0.246%
24	25.030	3687	3700	3713	rBV2	210540	690209	35.33%	7.722%
25	26.146	3883	3890	3900	rBV3	14445	42148	2.16%	0.472%
26	27.539	4119	4127	4138	rVB5	12491	40591	2.08%	0.454%
27	29.219	4406	4413	4424	rVB8	8616	29424	1.51%	0.329%




Sum of corrected areas: 8938240

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092322\
Data File : BG055015.D
Acq On : 23 Sep 2022 16:44
Operator : CG/JU
Sample : N4751-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PE-5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

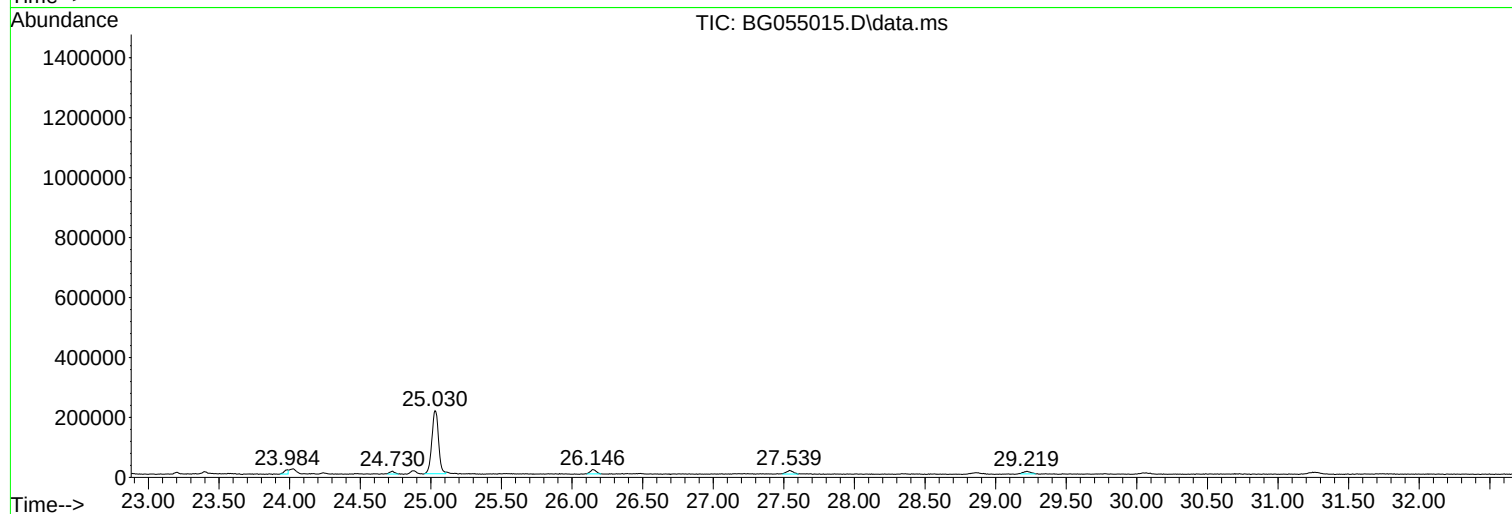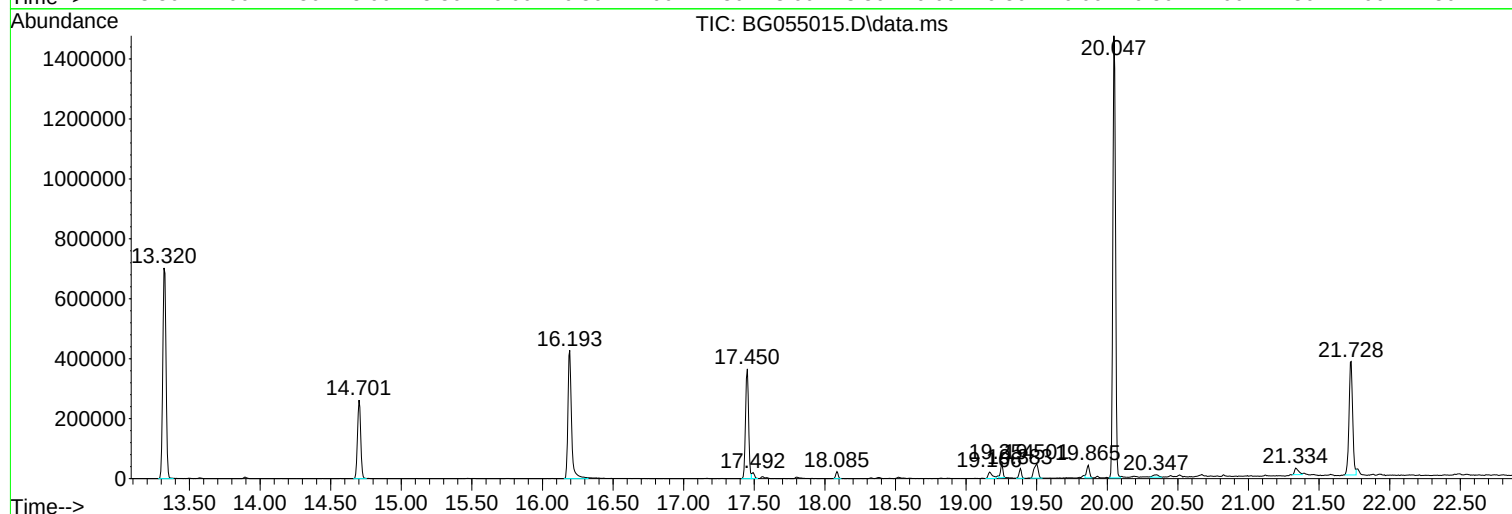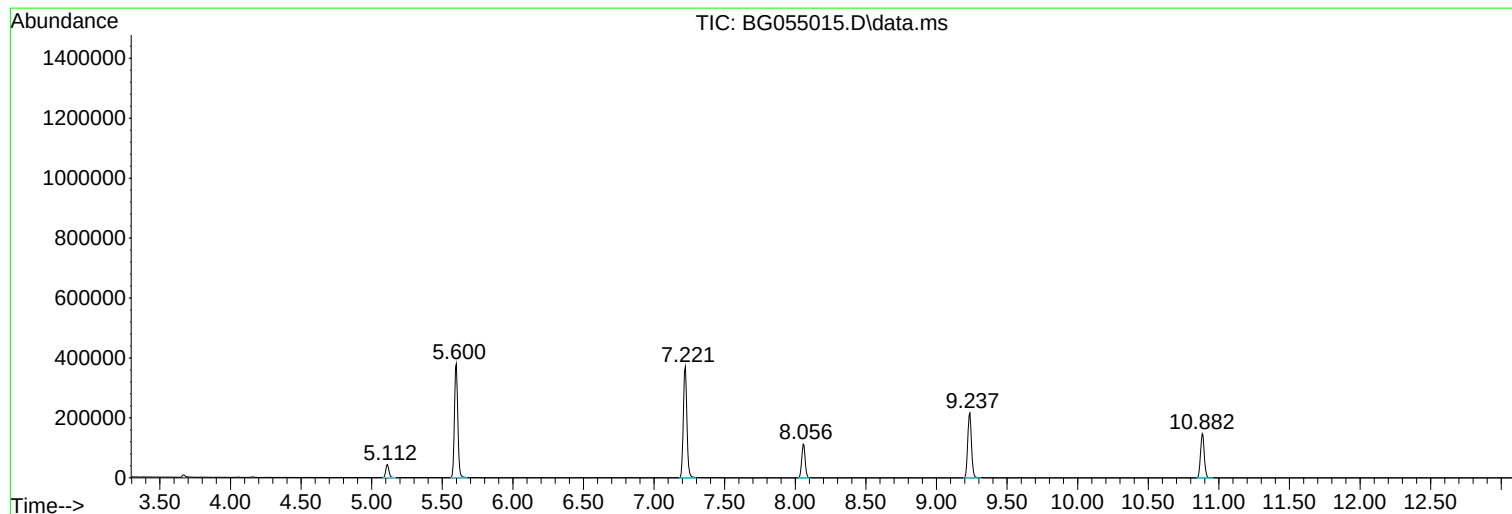

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092322\
Data File : BG055015.D
Acq On : 23 Sep 2022 16:44
Operator : CG/JU
Sample : N4751-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PE-5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.112	7.24 ng	69050	1,4-Dichlorobenzene-d4	8.056

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	53
2			(+)-4-Amino-4,5-dihydro-2(3H)-f...	101	C4H7NO2	016504-58-8	43
3			Guanidine	59	CH5N3	000113-00-8	38
4			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	12
5			1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10

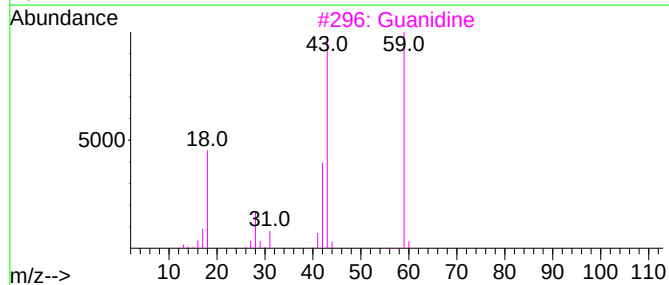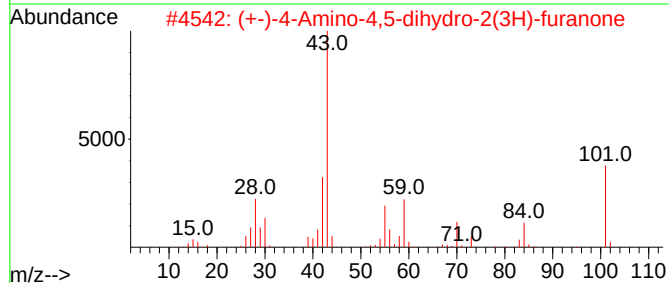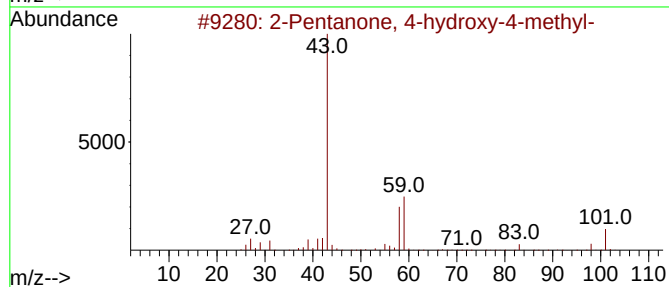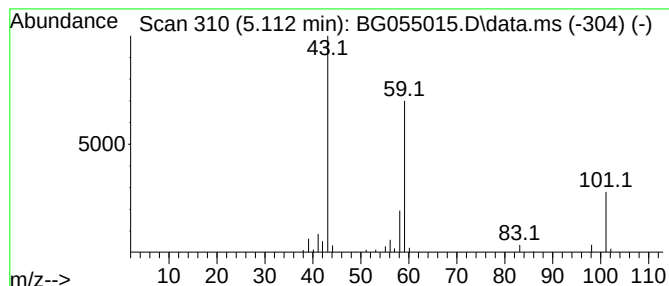

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092322\
Data File : BG055015.D
Acq On : 23 Sep 2022 16:44
Operator : CG/JU
Sample : N4751-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PE-5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.112	7.2	ng	69050	1	8.056	190806	20.0