

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092322\
 Data File : BG055016.D
 Acq On : 23 Sep 2022 17:26
 Operator : CG/JU
 Sample : N4751-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PE-1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG055016.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.109	305	310	318	rBV	55746	84894	3.62%	0.818%
2	5.597	386	393	407	rBV	476403	762211	32.50%	7.348%
3	7.219	662	669	683	rBV	463503	800431	34.13%	7.717%
4	8.059	805	812	819	rBV	123498	204605	8.73%	1.973%
5	9.234	1004	1012	1027	rBV	277917	496848	21.19%	4.790%
6	10.885	1285	1293	1302	rBV	160586	292806	12.49%	2.823%
7	13.323	1701	1708	1718	rBV	896305	1380975	58.89%	13.313%
8	14.704	1935	1943	1951	rBV	282920	449224	19.16%	4.331%
9	16.190	2190	2196	2220	rBV	549277	935628	39.90%	9.020%
10	17.448	2404	2410	2415	rBV	387454	578528	24.67%	5.577%
11	17.489	2415	2417	2425	rVB	22405	29624	1.26%	0.286%
12	18.088	2514	2519	2524	rVB	25875	31500	1.34%	0.304%
13	19.252	2710	2717	2721	rBV4	33526	42452	1.81%	0.409%
14	19.387	2733	2740	2746	rBV3	19638	25750	1.10%	0.248%
15	19.498	2752	2759	2767	rVB	56322	79877	3.41%	0.770%
16	19.863	2807	2821	2829	rVB	50447	93301	3.98%	0.899%
17	20.051	2847	2853	2862	rBV	1831706	2344945	100.00%	22.607%
18	21.337	3068	3072	3079	rBV3	24033	47006	2.00%	0.453%
19	21.725	3130	3138	3144	rBV2	413852	725538	30.94%	6.995%
20	21.772	3144	3146	3153	rVB	28349	35893	1.53%	0.346%
21	23.981	3514	3522	3523	rBV2	18553	33230	1.42%	0.320%
22	24.727	3642	3649	3657	rVB3	10990	29663	1.26%	0.286%
23	24.880	3666	3675	3685	rVB3	17112	47655	2.03%	0.459%
24	25.033	3688	3701	3715	rBV3	230724	715632	30.52%	6.899%
25	26.149	3885	3891	3900	rVB4	12923	35738	1.52%	0.345%
26	27.548	4124	4129	4139	rVB7	11372	36104	1.54%	0.348%
27	29.222	4406	4414	4427	rVB8	8948	32796	1.40%	0.316%




Sum of corrected areas: 10372854

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092322\
Data File : BG055016.D
Acq On : 23 Sep 2022 17:26
Operator : CG/JU
Sample : N4751-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PE-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

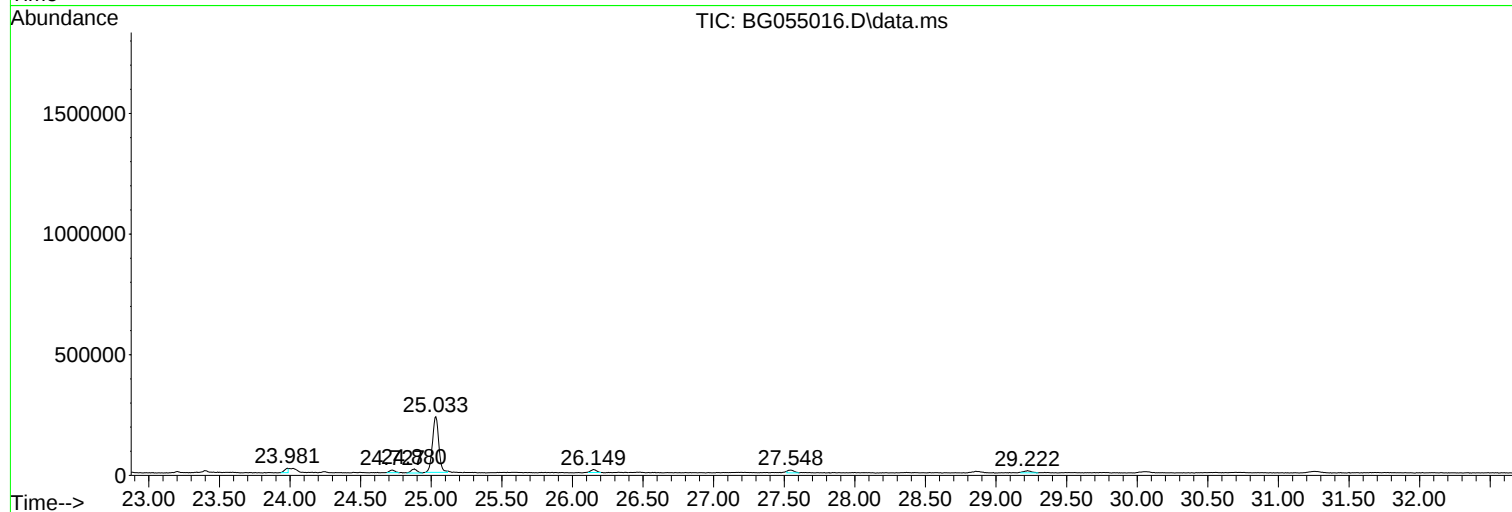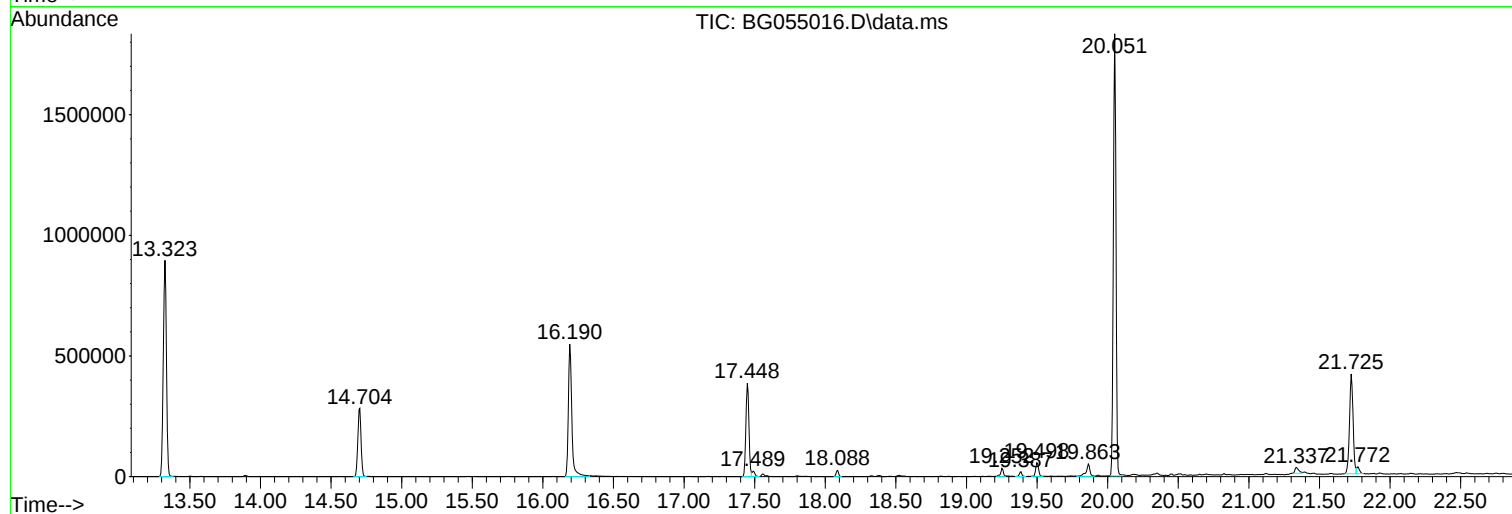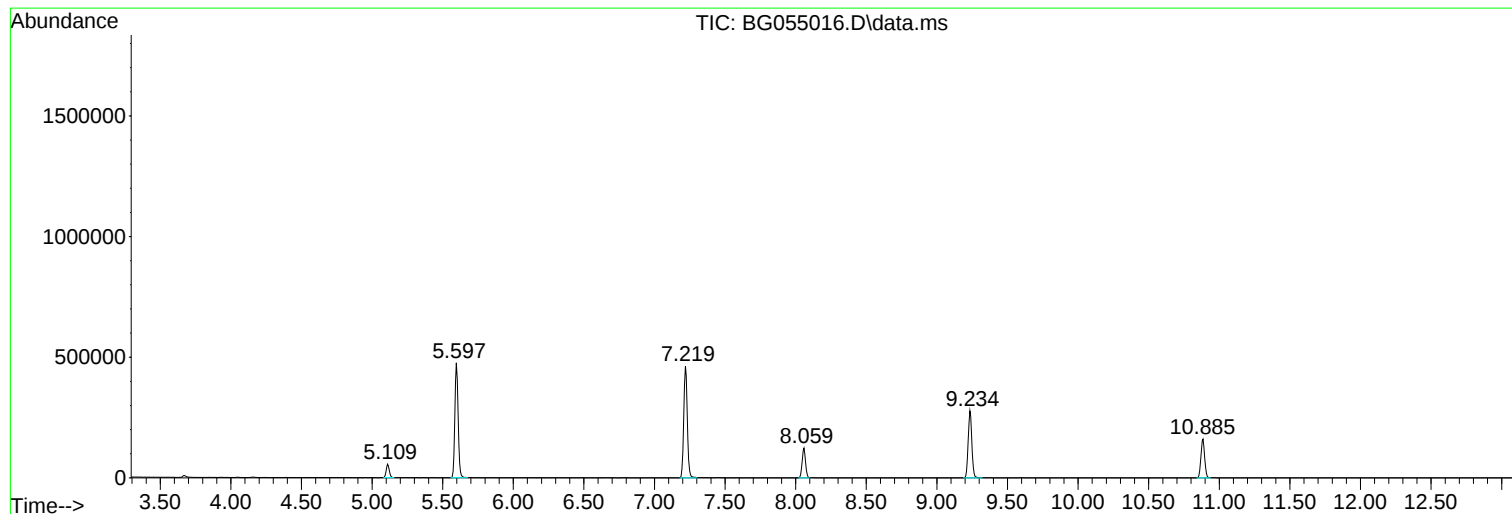

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092322\
Data File : BG055016.D
Acq On : 23 Sep 2022 17:26
Operator : CG/JU
Sample : N4751-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PE-1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.109	8.30 ng	84894	1,4-Dichlorobenzene-d4	8.059

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56		
2	Guanidine	59	CH5N3	000113-00-8	43		
3	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	17		
4	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
5	Acetone	58	C3H6O	000067-64-1	10		

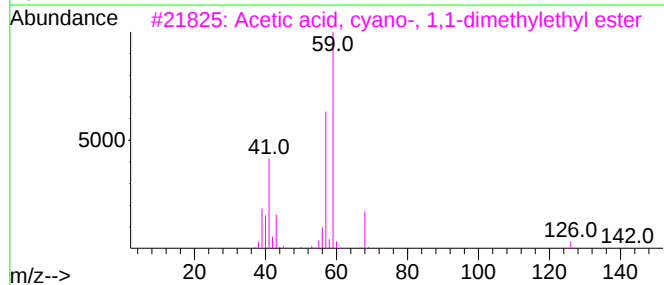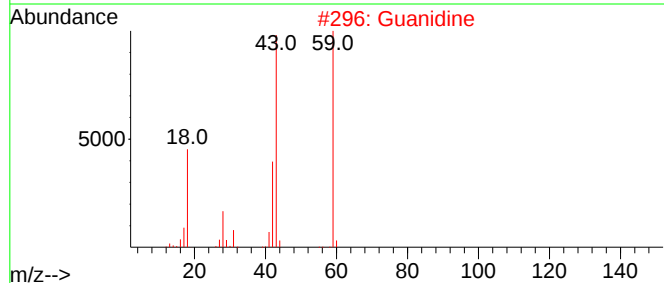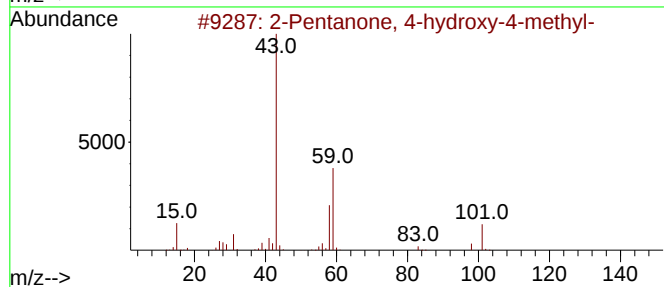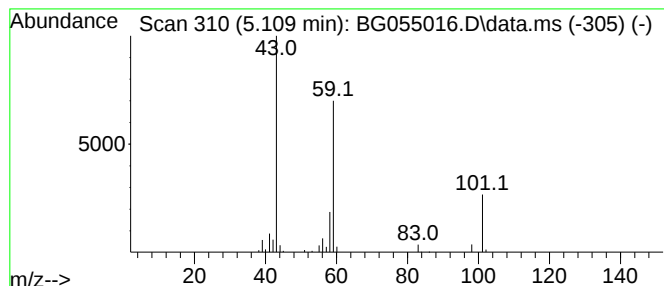

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092322\
Data File : BG055016.D
Acq On : 23 Sep 2022 17:26
Operator : CG/JU
Sample : N4751-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PE-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.109	8.3	ng	84894	1	8.059	204605	20.0