


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG092322\  
 Data File : BG055010.D  
 Acq On : 23 Sep 2022 12:17  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG091922.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Sep 19 17:41:40 2022

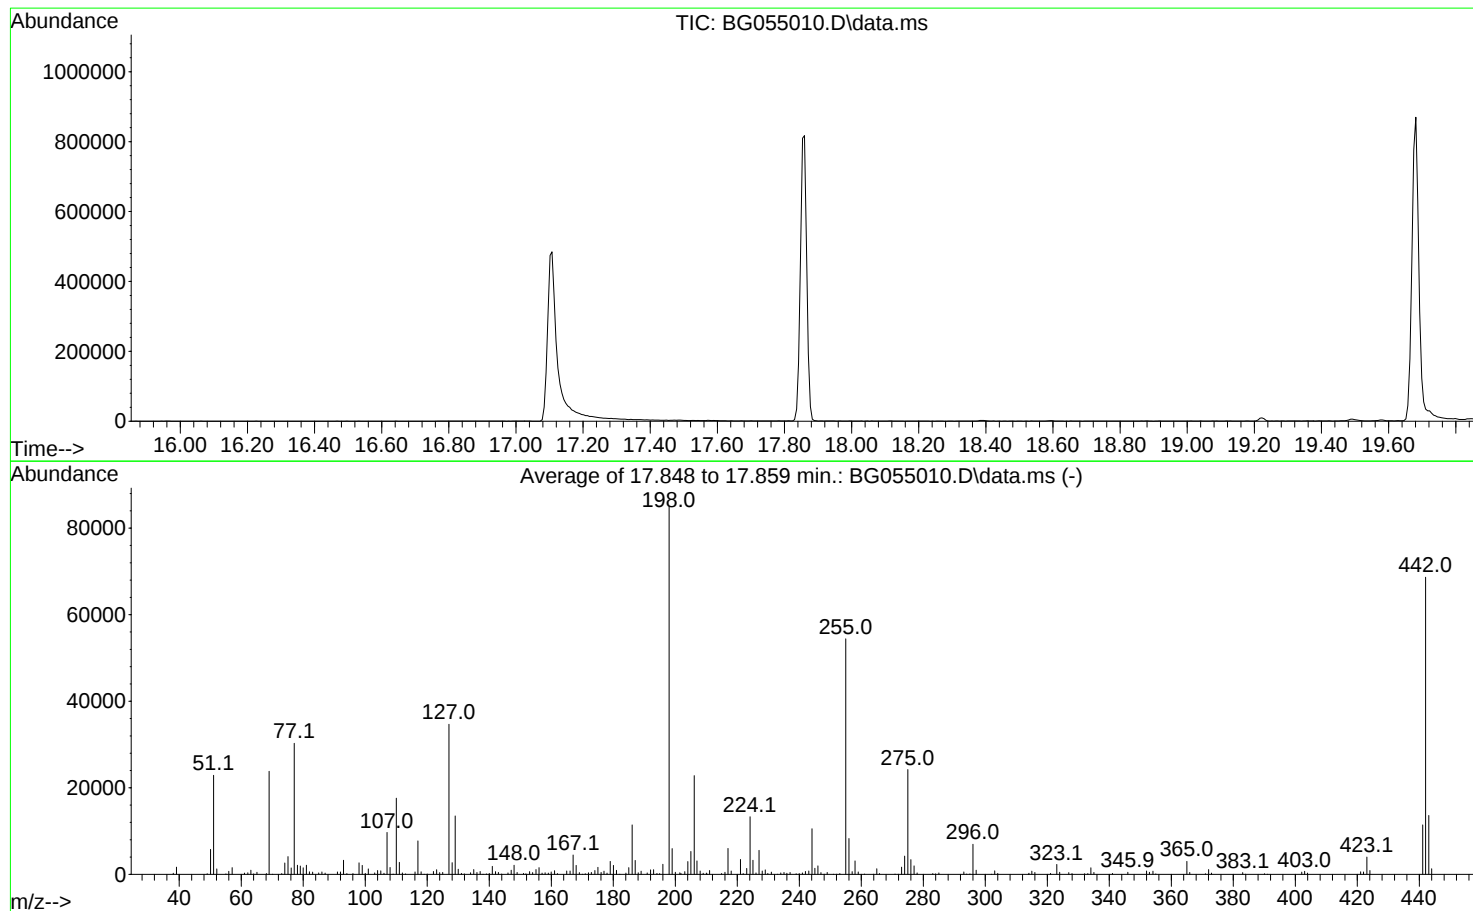

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 26.9         | 22893      | PASS                |
| 68             | 69              | 0.00            | 2               | 0.7          | 178        | PASS                |
| 69             | 198             | 0.00            | 100             | 28.0         | 23805      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.2          | 56         | PASS                |
| 127            | 198             | 10              | 80              | 40.8         | 34677      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 85003      | PASS                |
| 199            | 198             | 5               | 9               | 7.0          | 5959       | PASS                |
| 275            | 198             | 10              | 60              | 28.5         | 24227      | PASS                |
| 365            | 198             | 1               | 100             | 3.5          | 2998       | PASS                |
| 441            | 198             | 0.01            | 100             | 13.4         | 11421      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 68677      | PASS                |
| 443            | 442             | 15              | 24              | 19.8         | 13597      | PASS                |

# DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 9/23/2022     | BNA_G            | <u>BG055010.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 302469           | 20.903             |
| DDD           | 12524            | 20.462             |
| DDE           | 713              | 19.951             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 13237         | 315706           | 4.19               |
|               |                  |                    |

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG092322\  
Data File : BG055010.D  
Acq On : 23 Sep 2022 12:17  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Sep 24 04:55:31 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG091922.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Sep 19 17:41:40 2022  
Response via : Initial Calibration

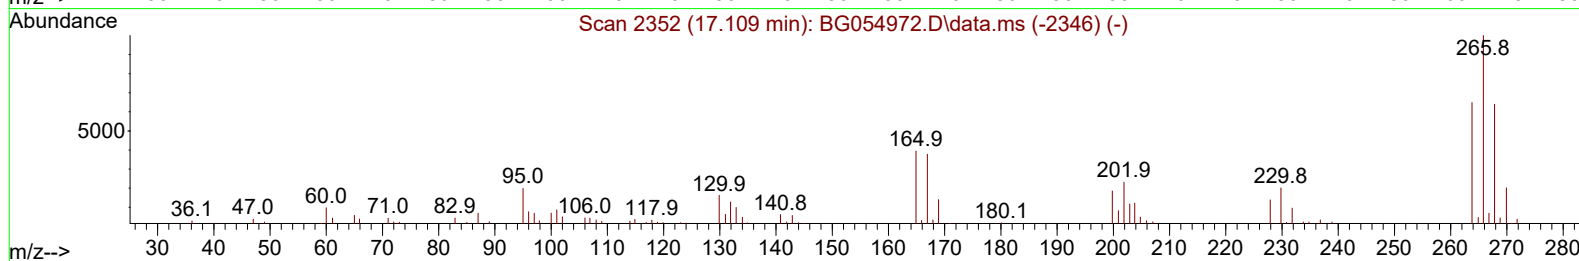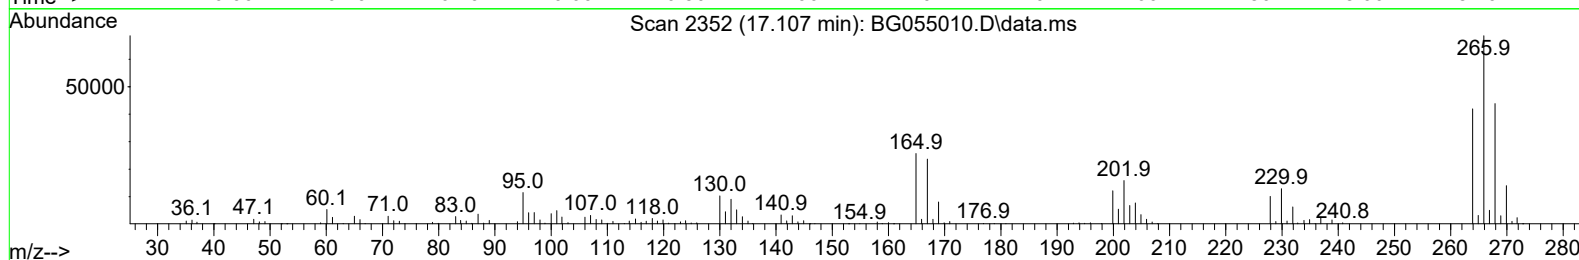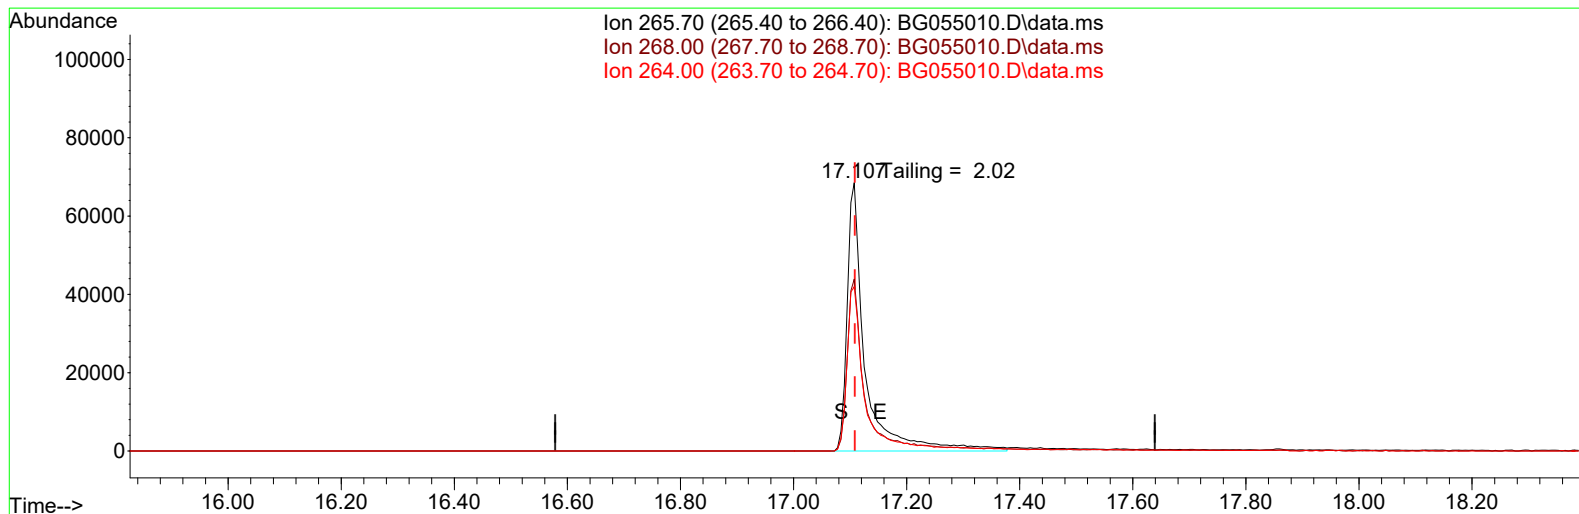

TIC: BG055010.D\data.ms

**(70) Pentachlorophenol (C)**

17.107min (-0.002) 8893.26 ng




response 152154

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.00  | 64.02  |
| 264.00 | 61.70  | 61.21  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG092322\  
Data File : BG055010.D  
Acq On : 23 Sep 2022 12:17  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Sep 24 04:55:31 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG091922.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Sep 19 17:41:40 2022  
Response via : Initial Calibration

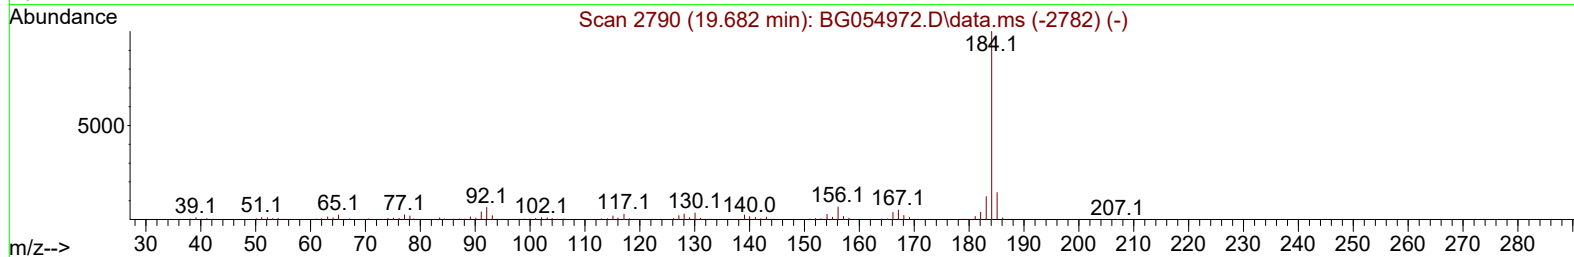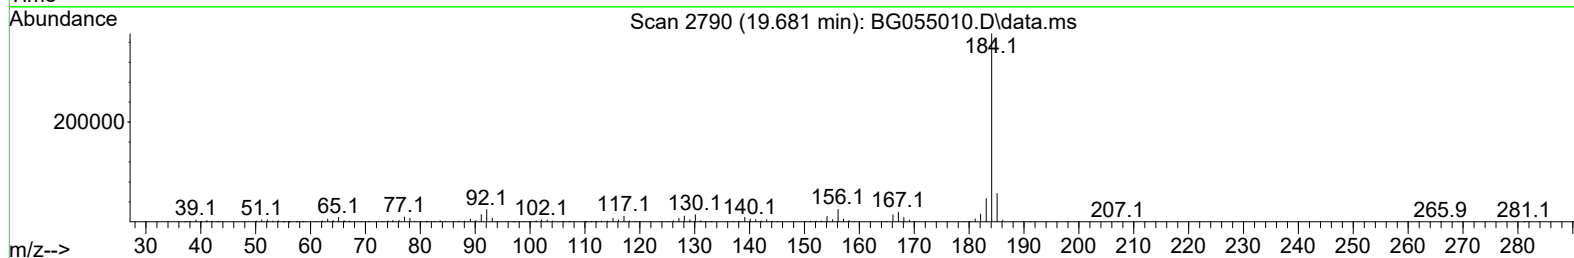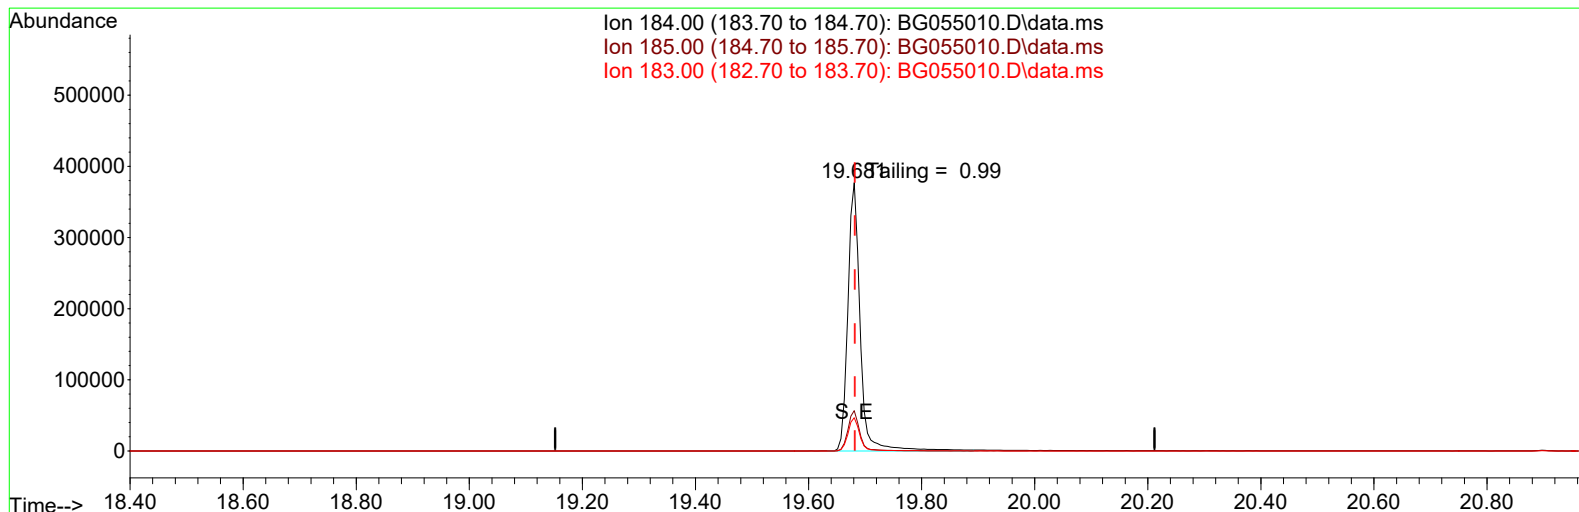

TIC: BG055010.D\data.ms

(77) Benzidine

19.681min (-0.002) 42454.32 ng

response 572203

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.20  | 15.05  |
| 183.00 | 12.30  | 12.43  |
| 0.00   | 0.00   | 0.00   |