
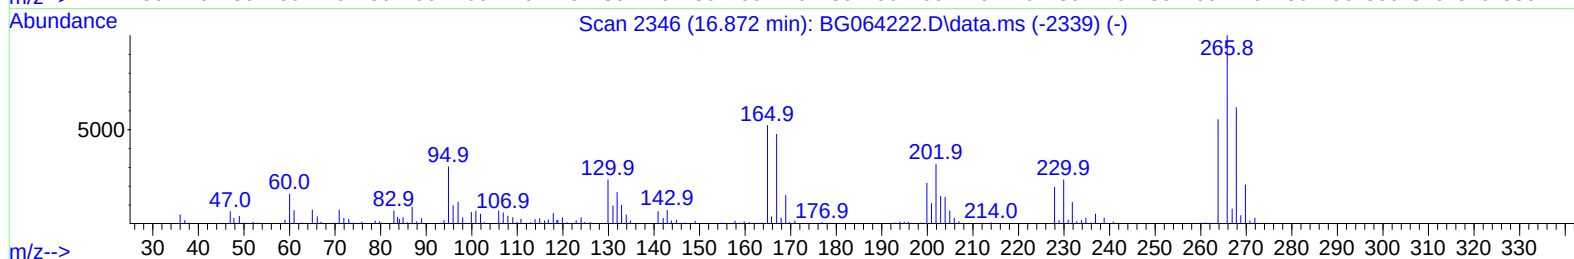
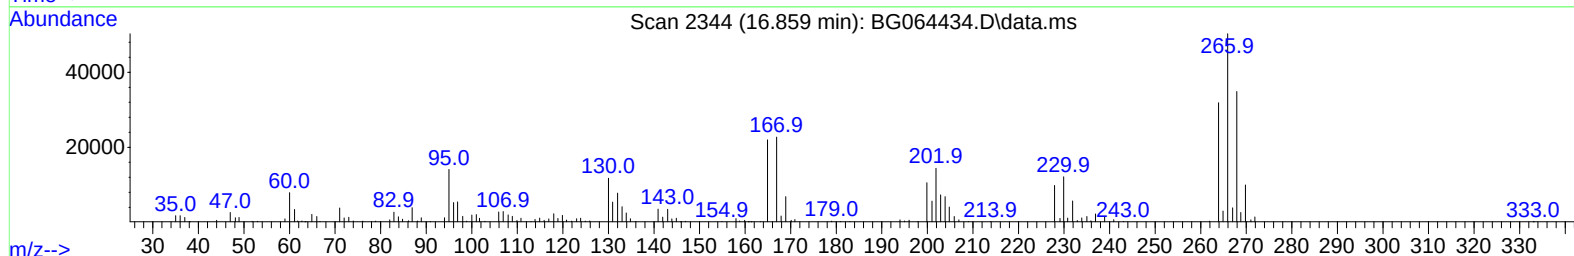


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092325\
Data File : BG064434.D
Acq On : 23 Sep 2025 10:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 23 11:53:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

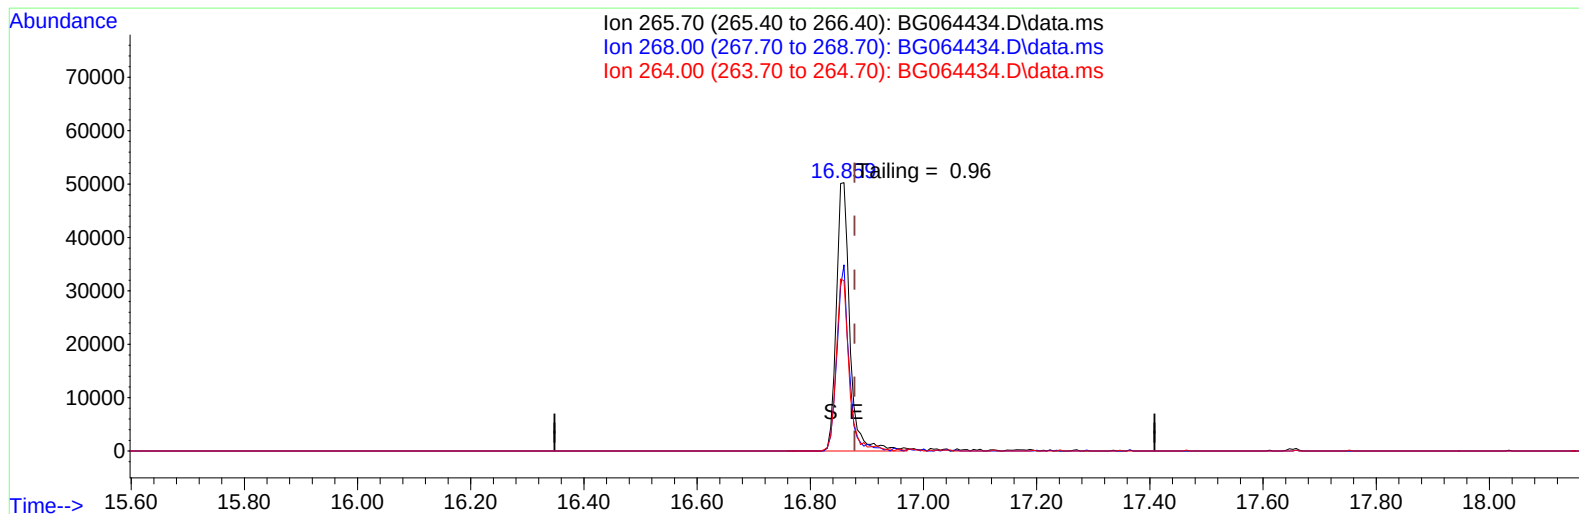

TIC: BG064434.D\data.ms

(70) Pentachlorophenol (C)




16.859min (-0.019) 27097.60 ng m

response 83137

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	69.33
264.00	55.40	63.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092325\
Data File : BG064434.D
Acq On : 23 Sep 2025 10:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 23 11:53:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

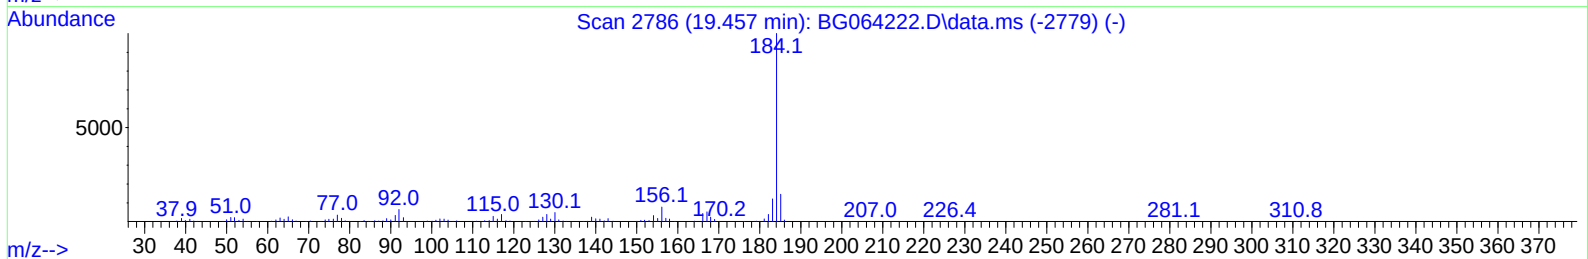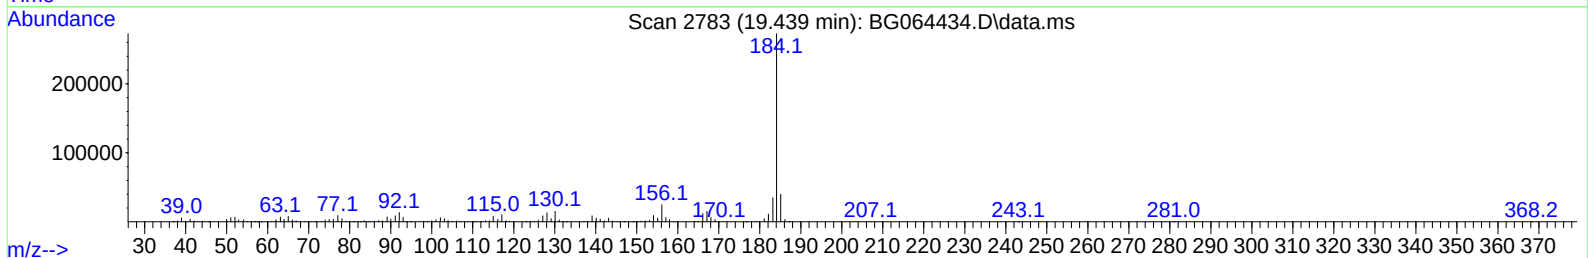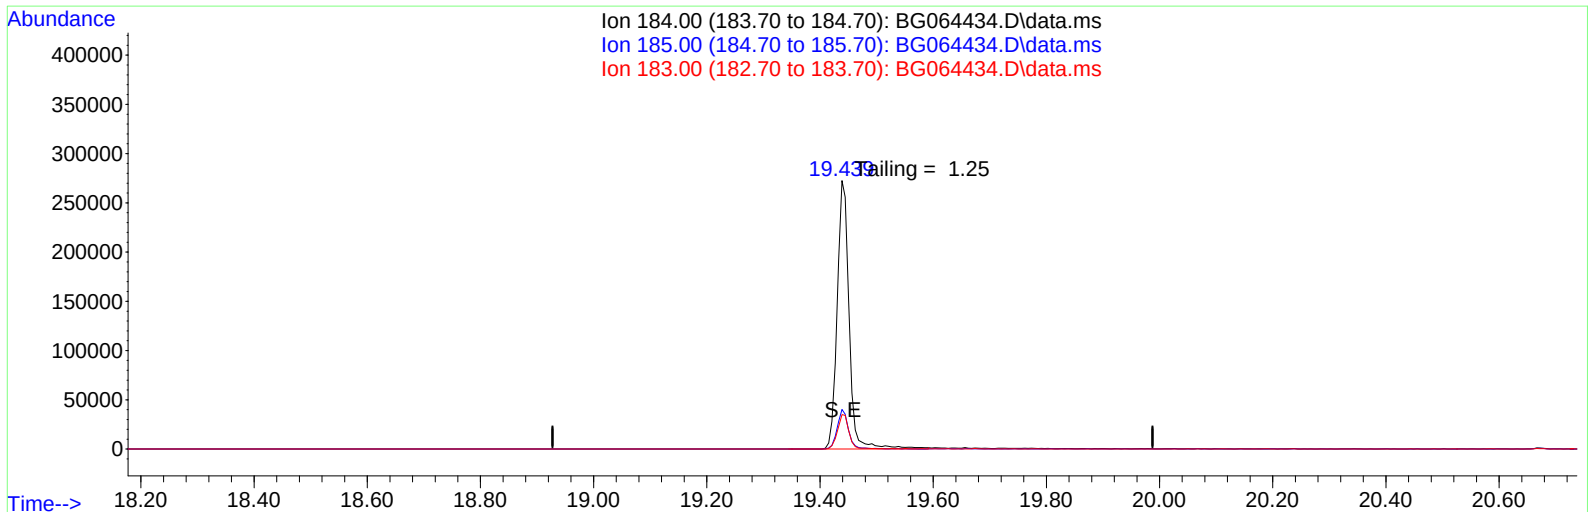

TIC: BG064434.D\data.ms

(77) Benzidine

19.439min (-0.019) 302619.30 ng m

response 394695

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.72
183.00	12.10	12.83
0.00	0.00	0.00