


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092325\
Data File : BG064434.D
Acq On : 23 Sep 2025 10:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 28 17:41:58 2025

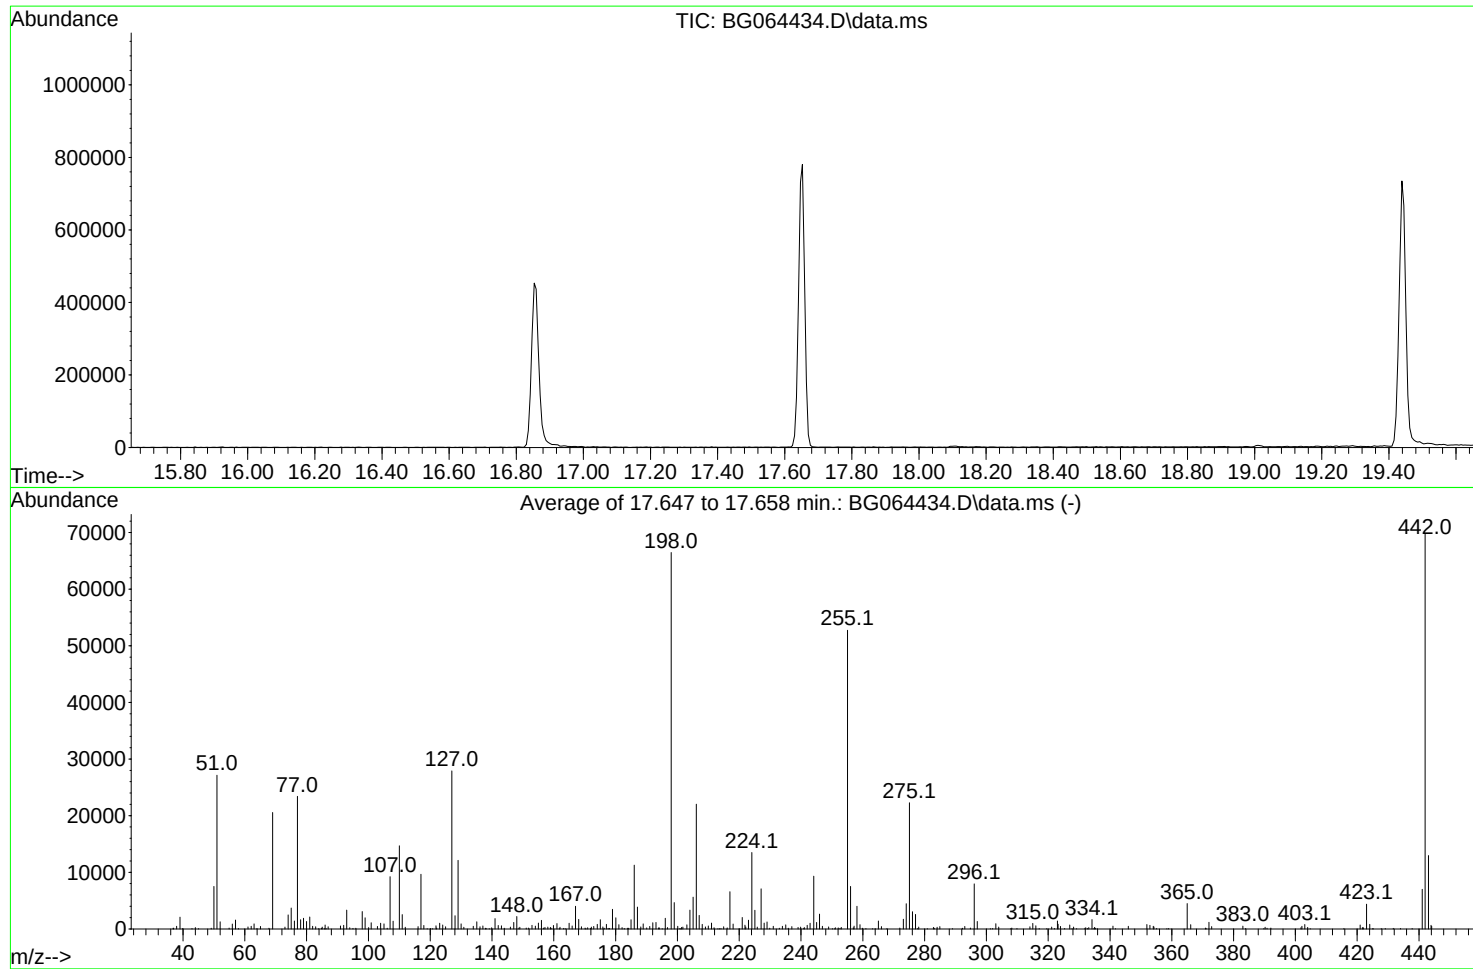




AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	0.6	122	PASS
69	69	100	100	100.0	20561	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.4	252	PASS
198	198	100	100	100.0	66480	PASS
199	198	5	9	7.0	4636	PASS
365	198	1	100	6.7	4485	PASS
441	443	0.01	150	54.0	6994	PASS
442	442	100	100	100.0	69725	PASS
443	442	15	24	18.6	12944	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092325\
Data File : BG064434.D
Acq On : 23 Sep 2025 10:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 23 11:53:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

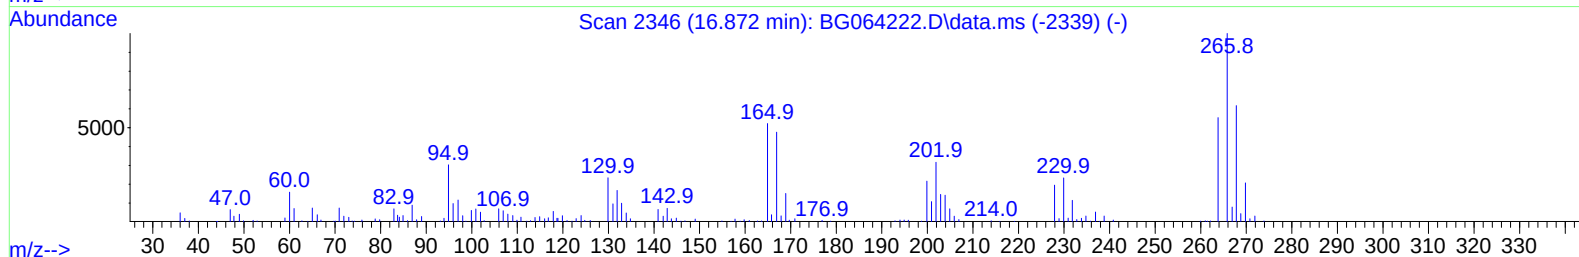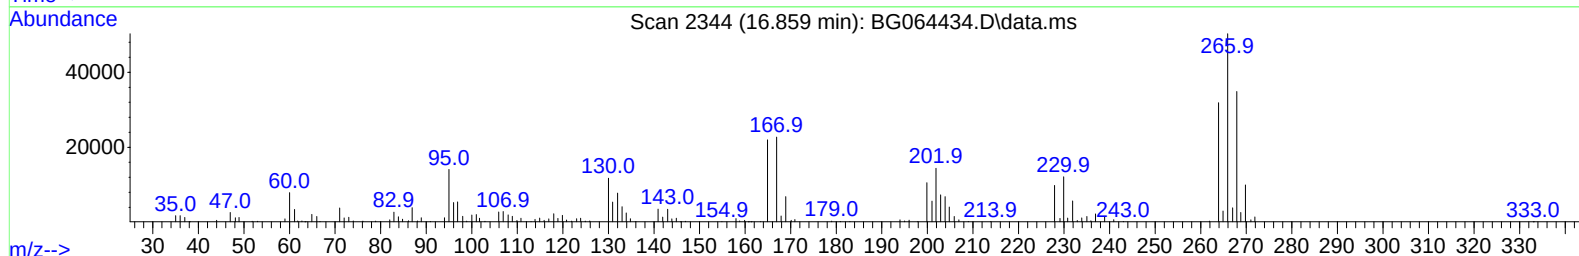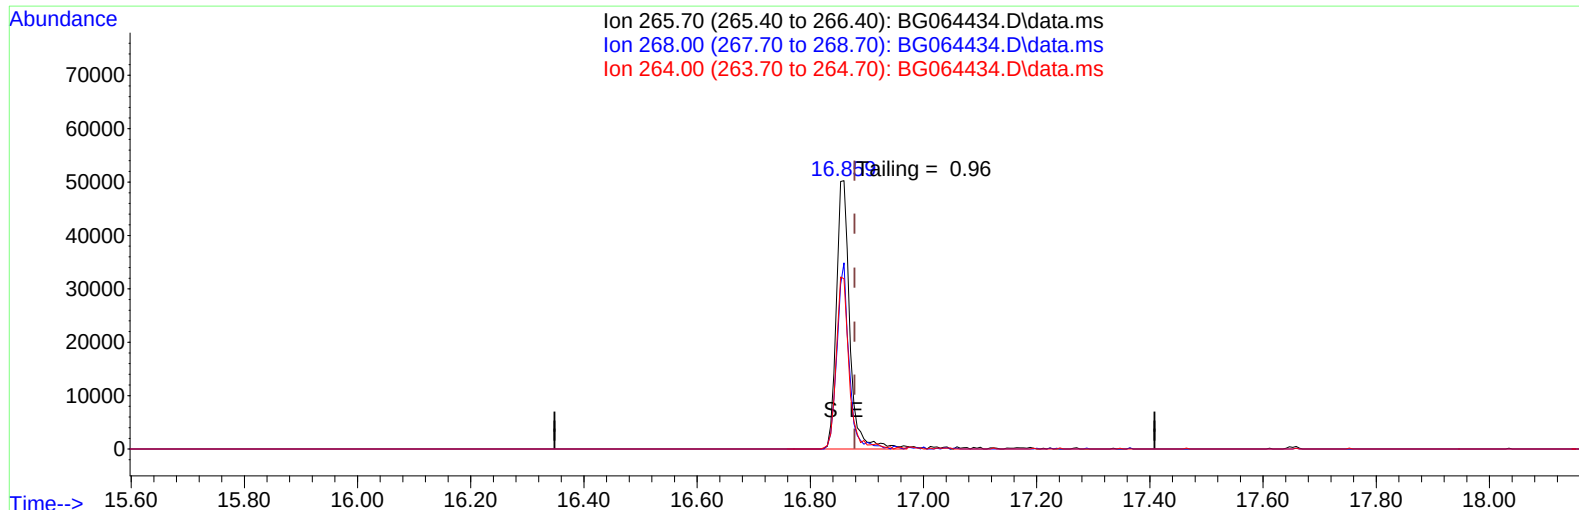

TIC: BG064434.D\data.ms

(70) Pentachlorophenol (C)

16.859min (-0.019) 27097.60 ng m




response 83137

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	69.33
264.00	55.40	63.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092325\
Data File : BG064434.D
Acq On : 23 Sep 2025 10:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 23 11:53:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

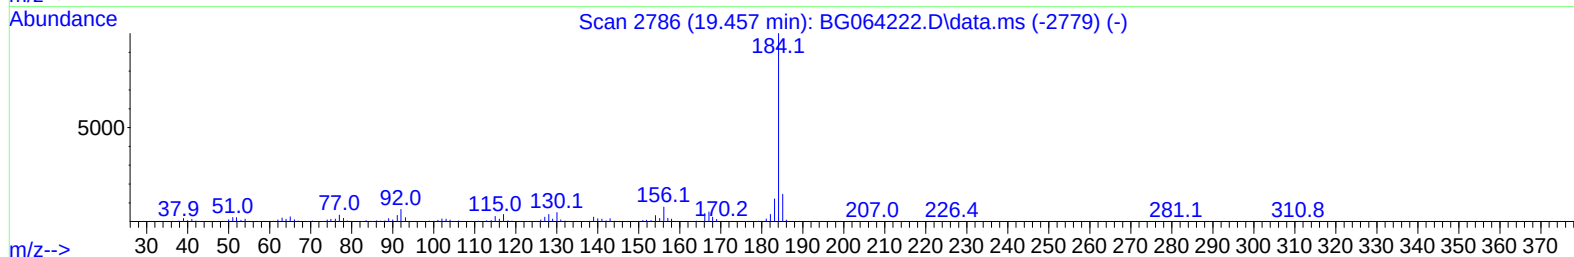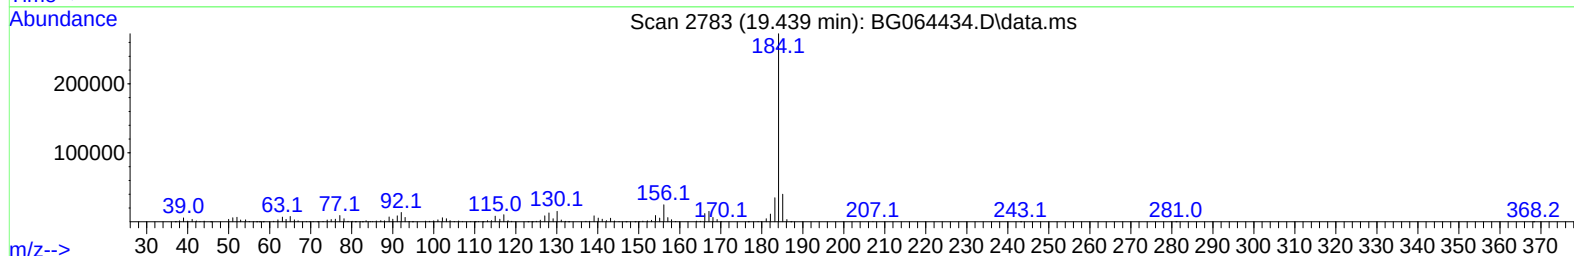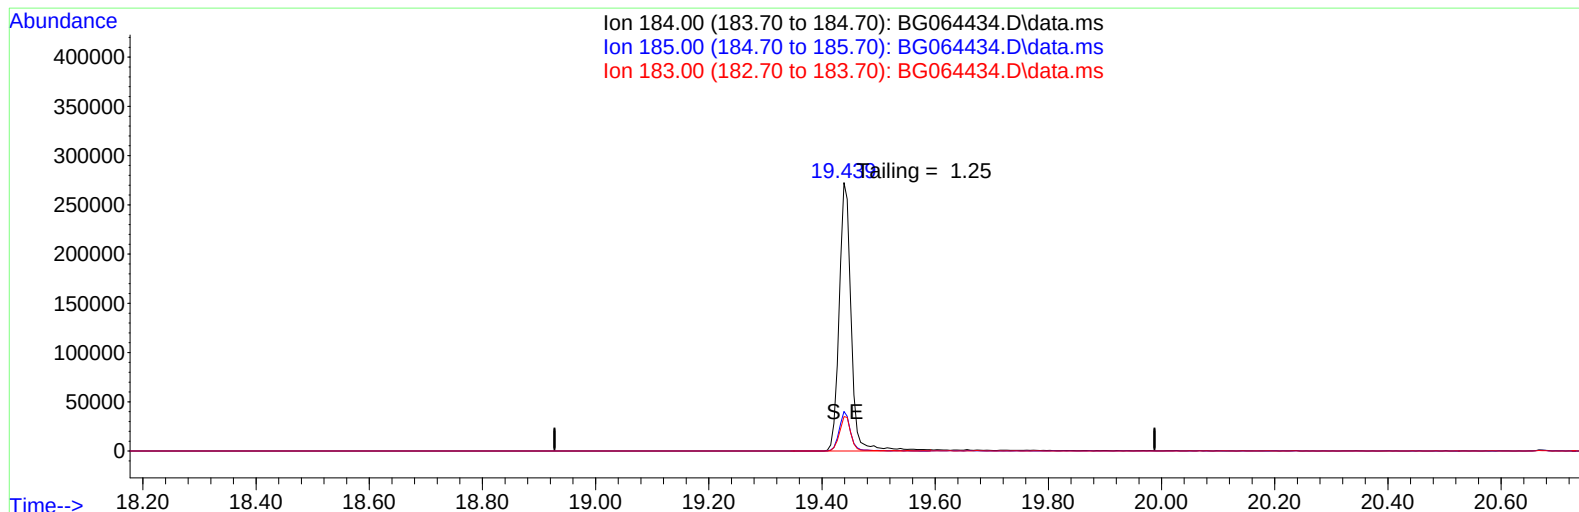

TIC: BG064434.D\data.ms

(77) Benzidine

19.439min (-0.019) 302619.30 ng m

response 394695

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.72
183.00	12.10	12.83
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/23/2025	BNA_G	<u>BG064434.D</u>
Compound Name	Response	Retention Time
DDT	235294	20.67
DDD	11458	20.232
DDE	202	19.733
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11660	246954	4.72

Instrument :
BNA_G
ClientSampleId :
DFTPP