

Data Path : Z:\HPCHEM1\BNA G\DATA\BG092415\
 Data File : BG018877.D
 Acq On : 24 Sep 2015 20:44
 Operator : TP
 Sample : G3780-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0GG2

Quant Time: Sep 25 04:03:56 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG091015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 25 04:02:29 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.00	152	46810	20.00	ng/ul	0.00
18) Naphthalene-d8	10.80	136	203088	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.62	164	134200	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.37	188	356115	20.00	ng/ul	0.00
78) Chrysene-d12	21.62	240	408424	20.00	ng/ul	0.00
86) Perylene-d12	24.81	264	418216	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.44	96	1583	1.63	ng/uL	0.00
5) Phenol-d5	7.16	99	28628	7.45	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.32	67	69082	31.01	ng/ul	0.00
9) 2-Chlorophenol-d4	7.53	132	77203	26.52	ng/ul	0.00
13) 4-Methylphenol-d8	8.70	113	52072	16.70	ng/ul	0.00
19) Nitrobenzene-d5	9.15	128	50526	32.84	ng/ul	0.00
22) 2-Nitrophenol-d4	9.88	143	55770	36.05	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.42	165	95490	29.31	ng/ul	0.00
29) 4-Chloroaniline-d4	10.93	131	8006	2.11	ng/ul	0.00
44) Dimethylphthalate-d6	14.03	166	387151	35.85	ng/ul	0.00
47) Acenaphthylene-d8	14.32	160	429242	33.54	ng/ul	0.00
52) 4-Nitrophenol-d4	14.83	143	12899	6.22	ng/ul	0.00
58) Fluorene-d10	15.62	176	323089	34.21	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.73	200	50301	29.84	ng/ul	0.00
71) Anthracene-d10	17.46	188	560351	35.74	ng/ul	0.00
79) Pyrene-d10	19.75	212	656972	34.96	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.59	264	707559	34.76	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	14.07	163	17591	1.68 ng/ul#	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG092415\
Data File : BG018877.D
Acq On : 24 Sep 2015 20:44
Operator : TP
Sample : G3780-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0GG2

Quant Time: Sep 25 04:03:56 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG091015.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 25 04:02:29 2015
Response via : Initial Calibration

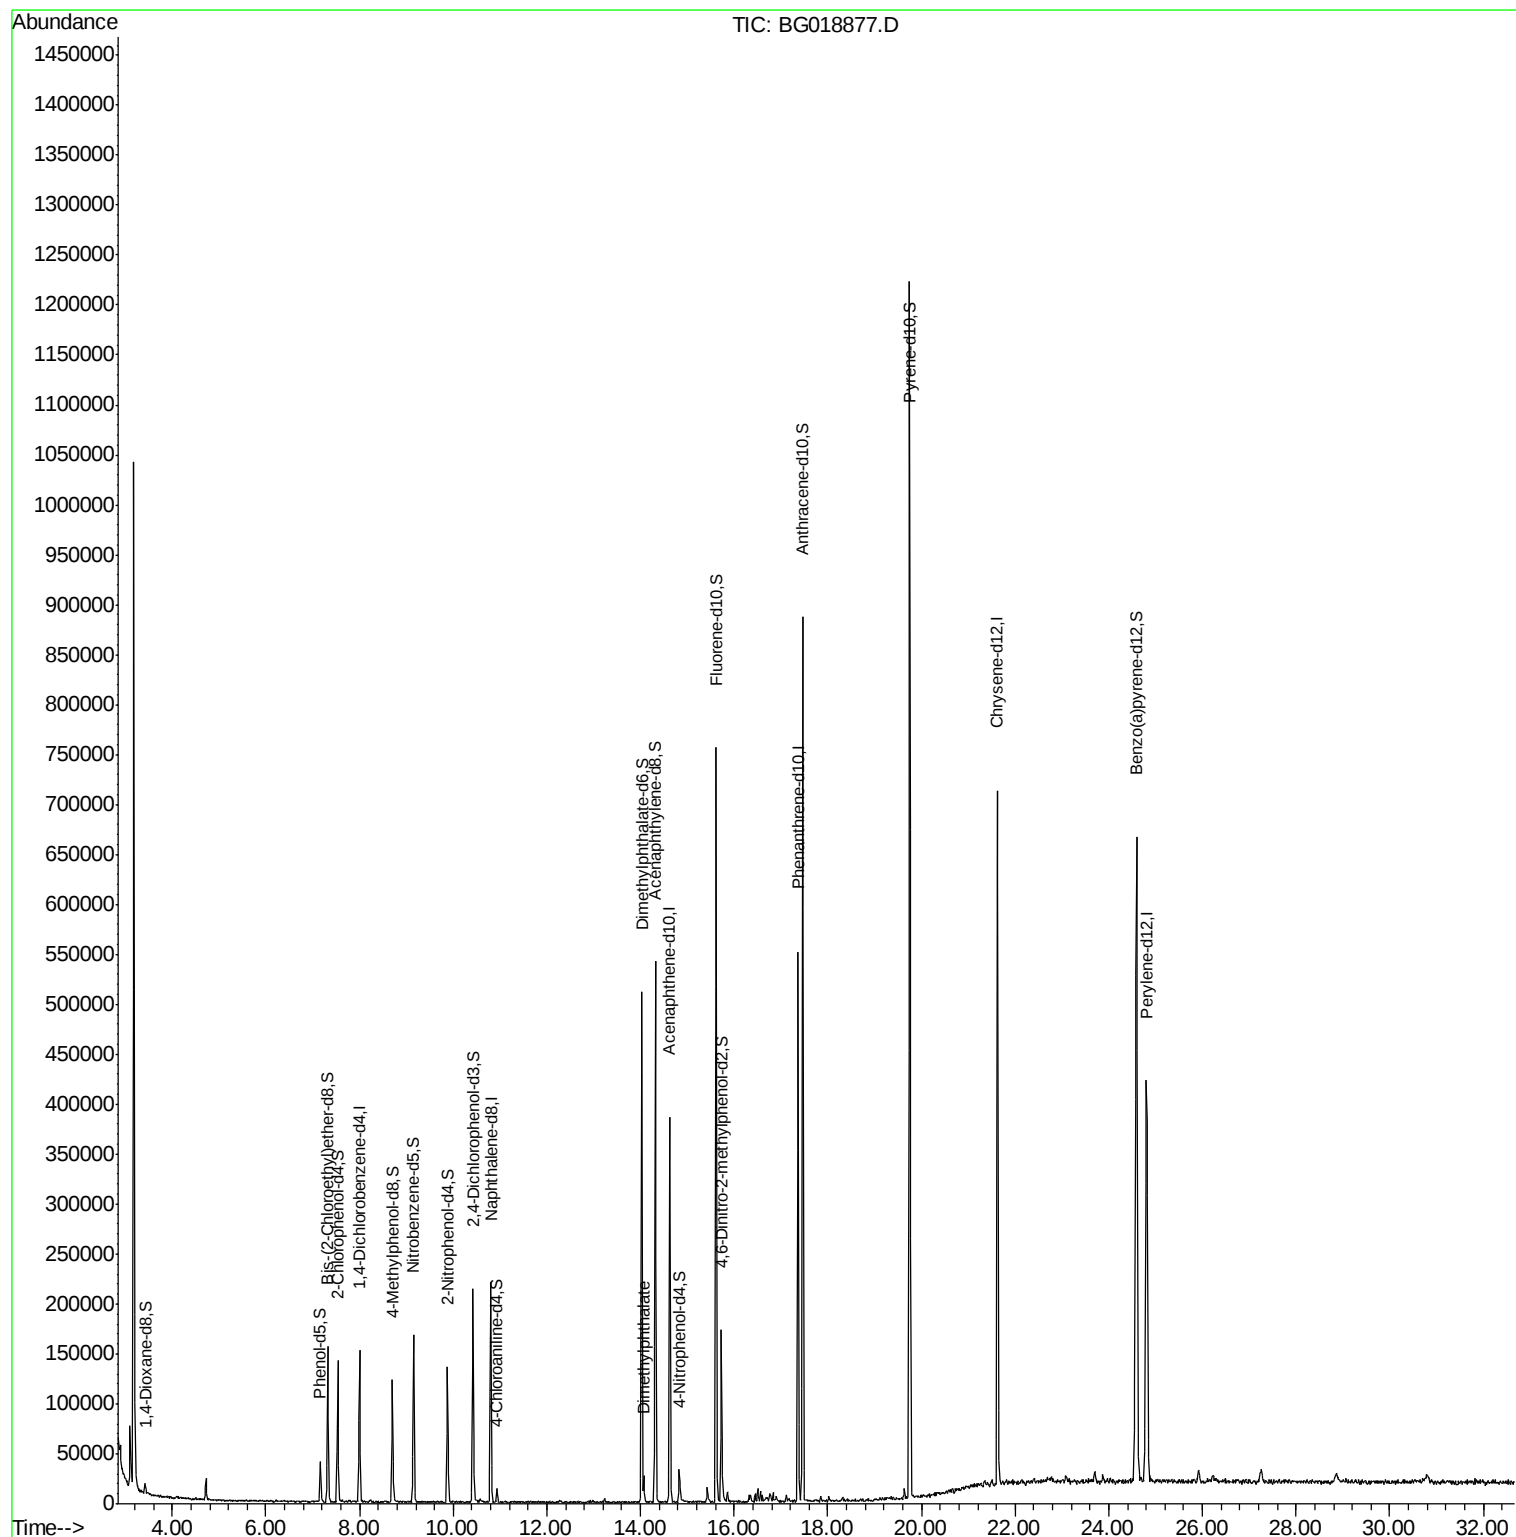

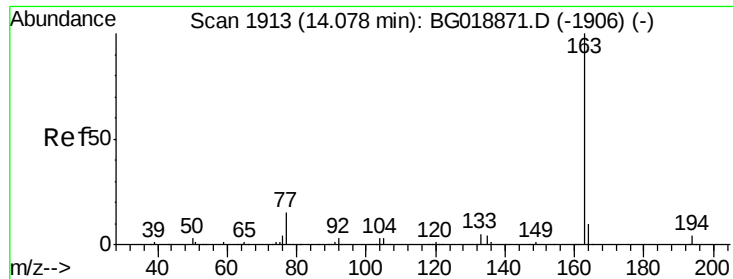

#45

Dimethylphthalate

Concen: 1.68 ng/ul

RT: 14.07 min Scan# 1912

Delta R.T. -0.01 min

Lab File: BG018877.D

Acq: 24 Sep 2015 20:44

Instrument :

BNA_G

ClientSampleId :

C0GG2


Tot Ion:163 Resp: 17591

Ion Ratio Lower Upper

163 100

194 4.9 2.9 4.3#

164 6.9 7.7 11.5#

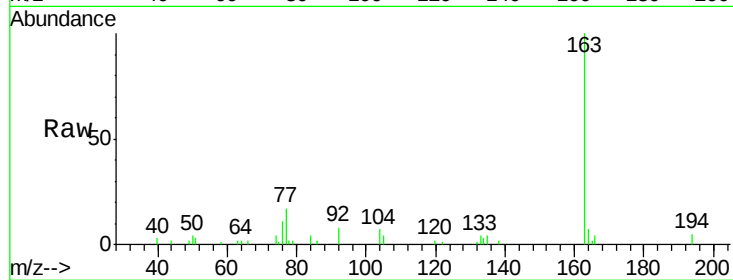

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

