

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG092415\
 Data File : BG018881.D
 Acq On : 24 Sep 2015 23:17
 Operator : TP
 Sample : G3780-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0GN0

Manual Integrations
 APPROVED

MMDadoda
 9/25/2015 2:17:09 PM

Quant Time: Sep 25 08:42:47 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG091015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 25 04:02:29 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.00	152	44348	20.00	ng/ul	0.00
18) Naphthalene-d8	10.80	136	190400	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.62	164	127093	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.36	188	336322	20.00	ng/ul	0.00
78) Chrysene-d12	21.62	240	384650	20.00	ng/ul	0.00
86) Perylene-d12	24.81	264	390030	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.44	96	1284	1.39	ng/uL	0.00
5) Phenol-d5	7.16	99	24494	6.73	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.32	67	65442	31.01	ng/ul	0.00
9) 2-Chlorophenol-d4	7.53	132	71641	25.97	ng/ul	0.00
13) 4-Methylphenol-d8	8.70	113	46341	15.68	ng/ul	0.00
19) Nitrobenzene-d5	9.15	128	48245	33.45	ng/ul	0.00
22) 2-Nitrophenol-d4	9.88	143	51275	35.35	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.42	165	88536	28.99	ng/ul	0.00
29) 4-Chloroaniline-d4	10.93	131	7091	2.00	ng/ul	0.00
44) Dimethylphthalate-d6	14.03	166	370171	36.19	ng/ul	0.00
47) Acenaphthylene-d8	14.32	160	413783	34.14	ng/ul	0.00
52) 4-Nitrophenol-d4	14.83	143	11573m	5.90	ng/ul	0.00
58) Fluorene-d10	15.61	176	319294	35.70	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.73	200	49993	31.40	ng/ul	0.00
71) Anthracene-d10	17.46	188	549793	37.13	ng/ul	0.00
79) Pyrene-d10	19.75	212	651135	36.79	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.59	264	683227	35.99	ng/ul	0.00

Target Compounds					Qvalue
45) Dimethylphthalate	14.07	163	20448	2.06 ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG092415\
Data File : BG018881.D
Acq On : 24 Sep 2015 23:17
Operator : TP
Sample : G3780-14
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
C0GN0

Manual Integrations
APPROVED

MMDadoda
9/25/2015 2:17:09 PM

Quant Time: Sep 25 08:42:47 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG091015.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 25 04:02:29 2015
Response via : Initial Calibration

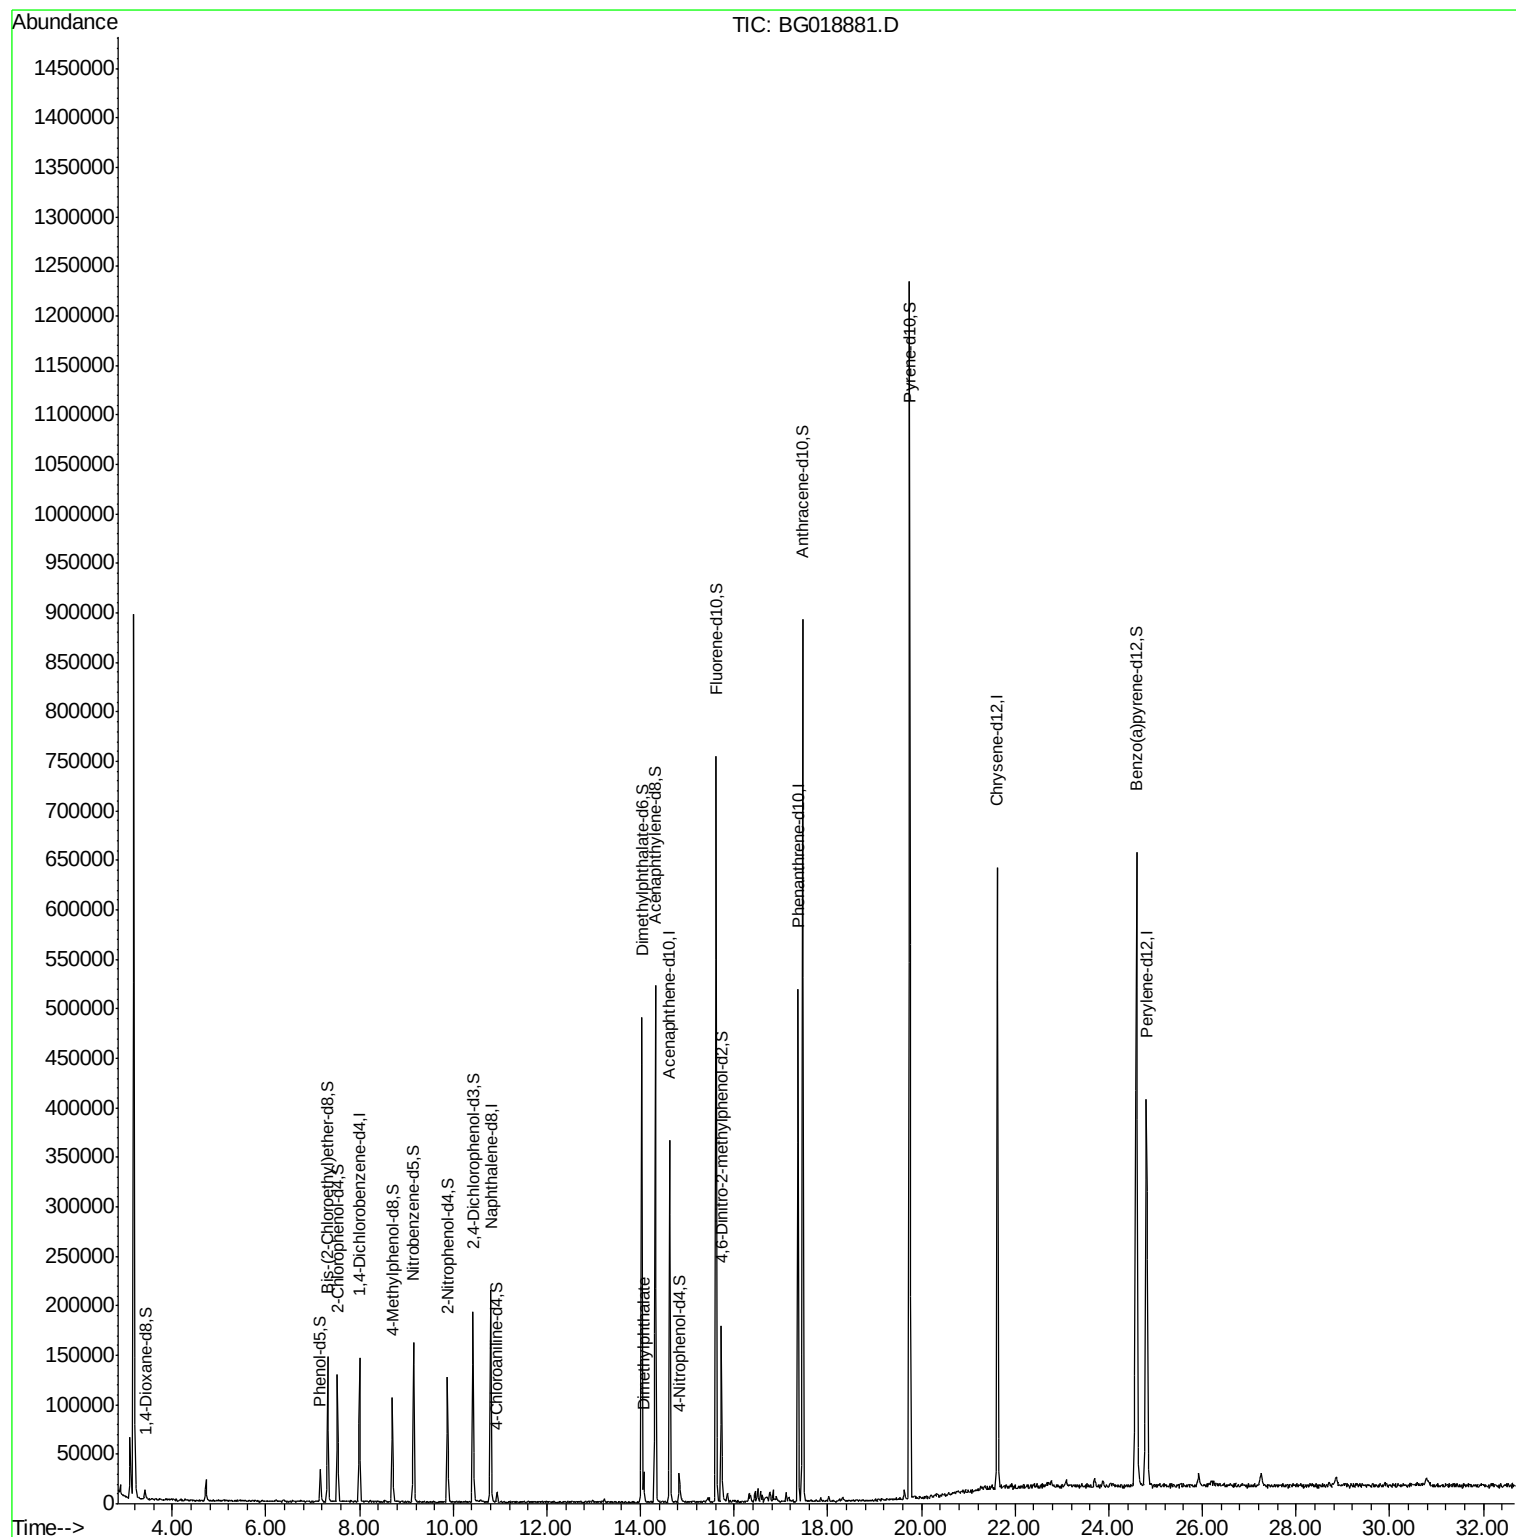

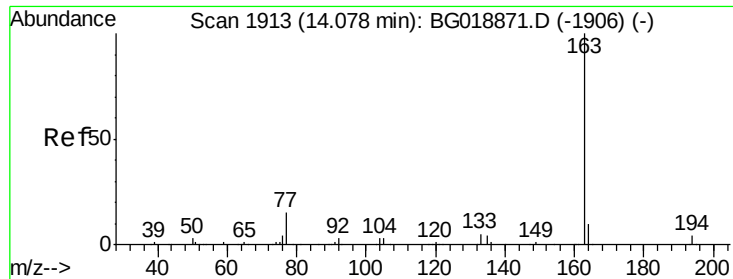

#45
 Dimethylphthalate
 Concen: 2.06 ng/ul
 RT: 14.07 min Scan# 1912
 Delta R.T. -0.01 min
 Lab File: BG018881.D
 Acq: 24 Sep 2015 23:17

Instrument :
 BNA_G
 ClientSampleId :
 C0GN0

Tgt Ion	Ratio	Resp Lower	Resp Upper
163	100		
194	4.0	2.9	4.3
164	10.7	7.7	11.5

Manual Integrations
 APPROVED

MMDadoda
 9/25/2015 2:17:09 PM

