

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG092415\
 Data File : BG018890.D
 Acq On : 25 Sep 2015 4:58
 Operator : TP
 Sample : G3802-07
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E43H8

Quant Time: Sep 25 07:31:59 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG091015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 25 04:50:00 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.00	152	58261	20.00	ng/ul	0.00
18) Naphthalene-d8	10.80	136	248859	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.62	164	161426	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.37	188	398350	20.00	ng/ul	0.00
78) Chrysene-d12	21.62	240	407244	20.00	ng/ul	0.00
86) Perylene-d12	24.81	264	412908	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.44	96	4409	3.64	ng/uL	0.00
5) Phenol-d5	7.16	99	100575	21.02	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.32	67	59981	21.63	ng/ul	0.00
9) 2-Chlorophenol-d4	7.53	132	83590	23.07	ng/ul	0.00
13) 4-Methylphenol-d8	8.70	113	87034	22.42	ng/ul	0.00
19) Nitrobenzene-d5	9.15	128	42159	22.36	ng/ul	0.00
22) 2-Nitrophenol-d4	9.88	143	48844	25.76	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.42	165	92388	23.14	ng/ul	0.00
29) 4-Chloroaniline-d4	10.93	131	116353	25.05	ng/ul	0.00
44) Dimethylphthalate-d6	14.02	166	304288	23.42	ng/ul	0.00
47) Acenaphthylene-d8	14.32	160	361134	23.46	ng/ul	0.00
52) 4-Nitrophenol-d4	14.82	143	47635	19.11	ng/ul	0.00
58) Fluorene-d10	15.62	176	250183	22.02	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.73	200	33552	17.79	ng/ul	0.00
71) Anthracene-d10	17.47	188	380455	21.69	ng/ul	0.00
79) Pyrene-d10	19.75	212	383984	20.49	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.59	264	386891	19.25	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.07	163	172242	13.68	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG092415\
Data File : BG018890.D
Acq On : 25 Sep 2015 4:58
Operator : TP
Sample : G3802-07
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E43H8

Quant Time: Sep 25 07:31:59 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG091015.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 25 04:50:00 2015
Response via : Initial Calibration

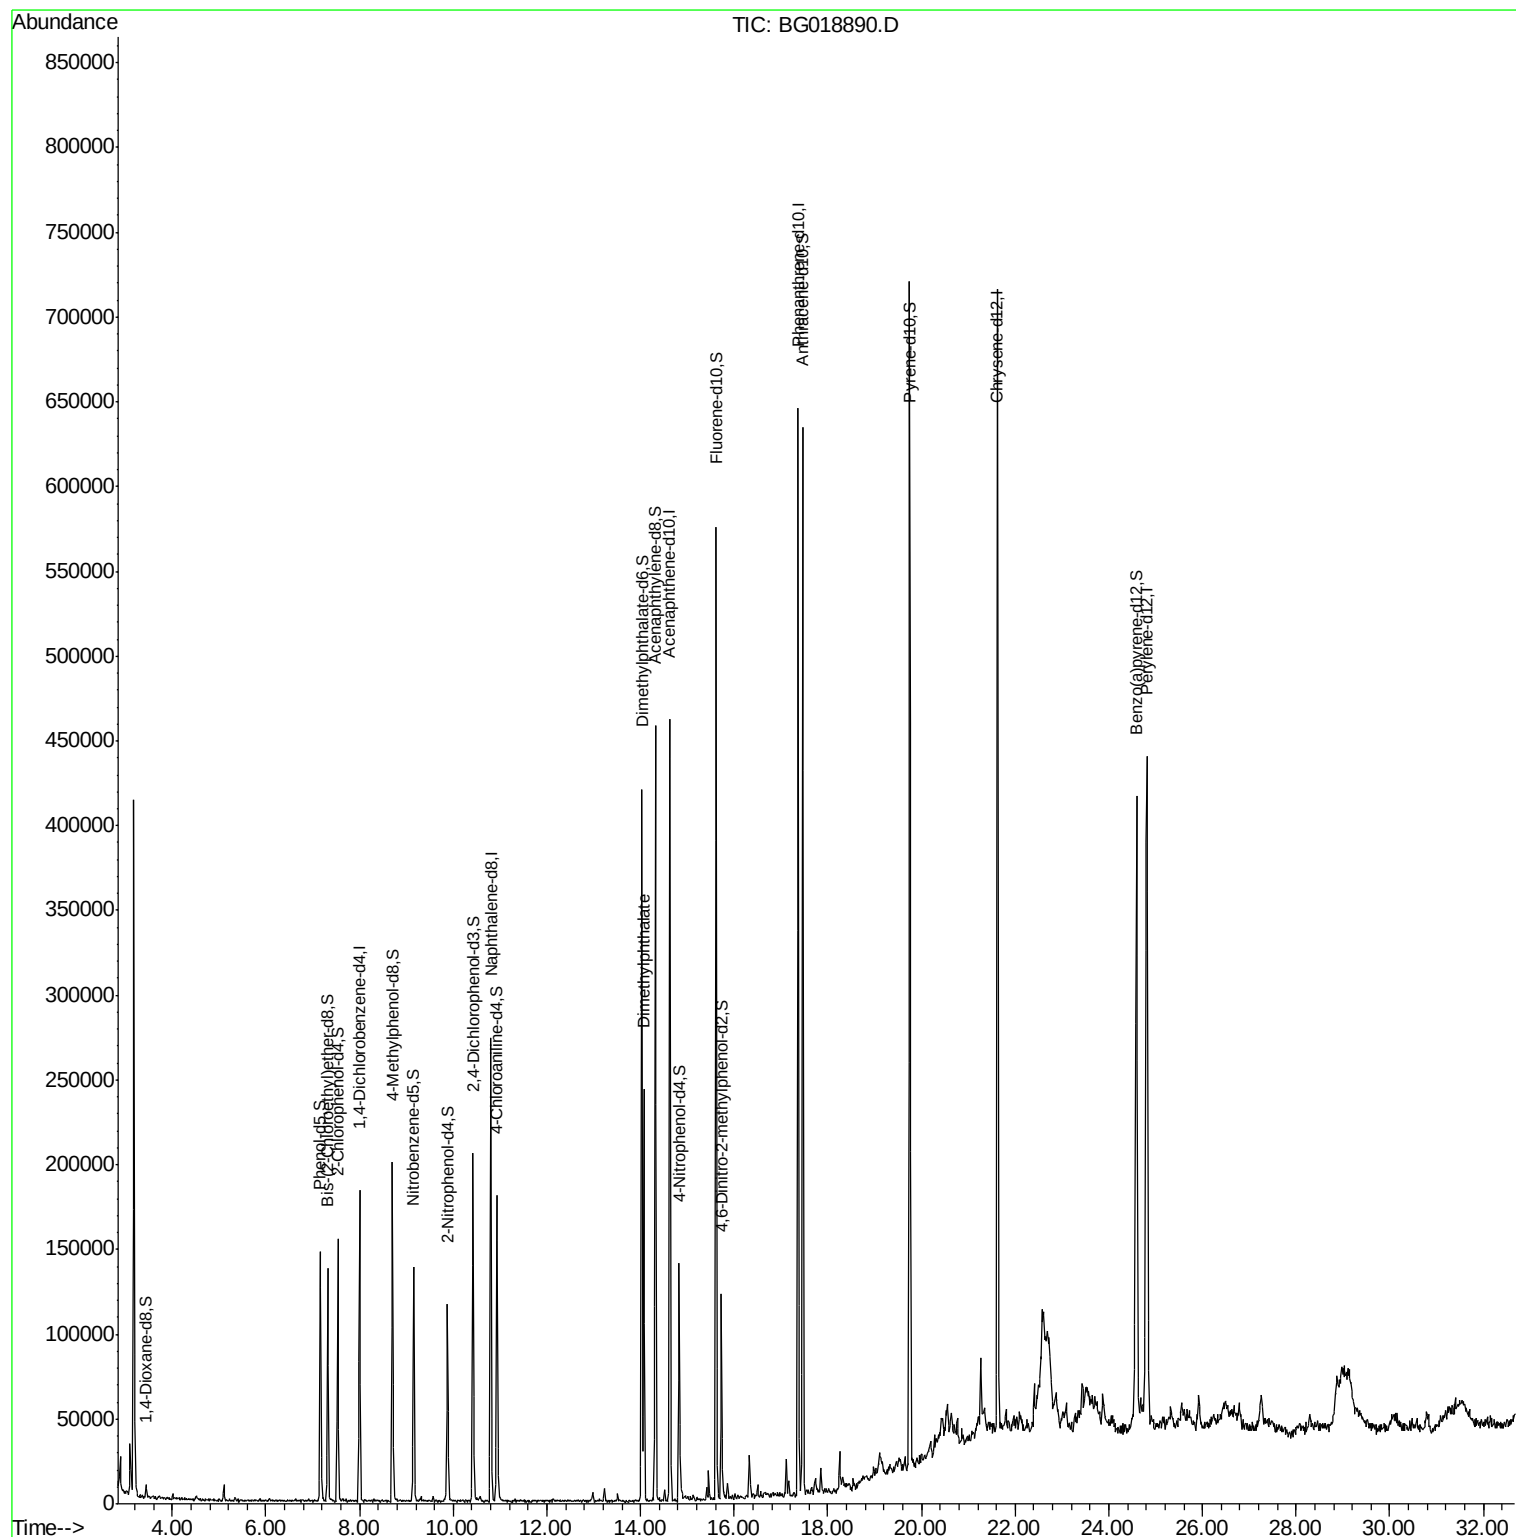

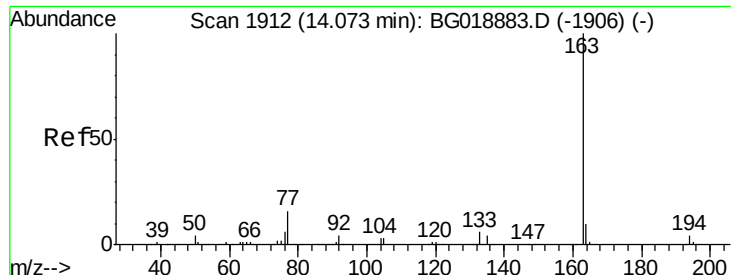

#45

Dimethylphthalate

Concen: 13.68 ng/ul

RT: 14.07 min Scan# 1912

Delta R.T. -0.00 min

Lab File: BG018890.D


Acq: 25 Sep 2015 4:58

Instrument :

BNA_G

ClientSampleId :

E43H8

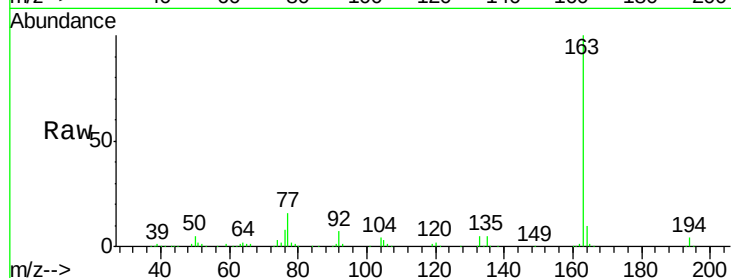


Tgt Ion:163 Resp: 172242

Ion Ratio Lower Upper

163 100

194 3.9 2.9 4.3

164 10.1 7.7 11.5

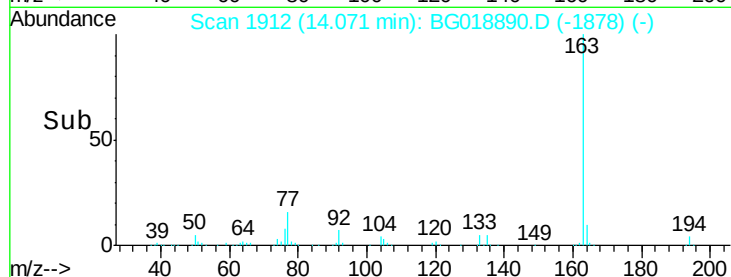

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

