

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG092418\
 Data File : BG036938.D
 Acq On : 25 Sep 2018 4:54
 Operator : JU/SJ
 Sample : J4770-20
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JC-02-092118-J

Quant Time: Sep 25 07:30:49 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 24 10:41:23 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	38949	20.00	ng	0.00
21) Naphthalene-d8	10.85	136	162618	20.00	ng	0.00
38) Acenaphthene-d10	14.67	164	113816	20.00	ng	0.00
63) Phenanthrene-d10	17.41	188	302017	20.00	ng	0.00
75) Chrysene-d12	21.68	240	316928	20.00	ng	-0.01
86) Perylene-d12	24.89	264	305456	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	244873	120.57	ng	0.00
7) Phenol-d6	7.20	99	317890	101.17	ng	-0.01
23) Nitrobenzene-d5	9.20	82	258046	84.98	ng	0.00
41) 2,4,6-Tribromophenol	16.16	330	155320	114.06	ng	-0.01
44) 2-Fluorobiphenyl	13.29	172	607438	79.49	ng	0.00
78) Terphenyl-d14	20.02	244	1138786	94.48	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.20	70	34100	13.045	ng	# 73
50) 2,6-Dinitrotoluene	14.67	165	14285	7.147	ng	# 21
56) 2,4-Dinitrotoluene	14.67	165	14285	5.122	ng	# 20
66) 4-Bromophenyl-phenylether	16.16	248	10590	3.083	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG092418\
Data File : BG036938.D
Acq On : 25 Sep 2018 4:54
Operator : JU/SJ
Sample : J4770-20
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JC-02-092118-J

Quant Time: Sep 25 07:30:49 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 24 10:41:23 2018
Response via : Initial Calibration

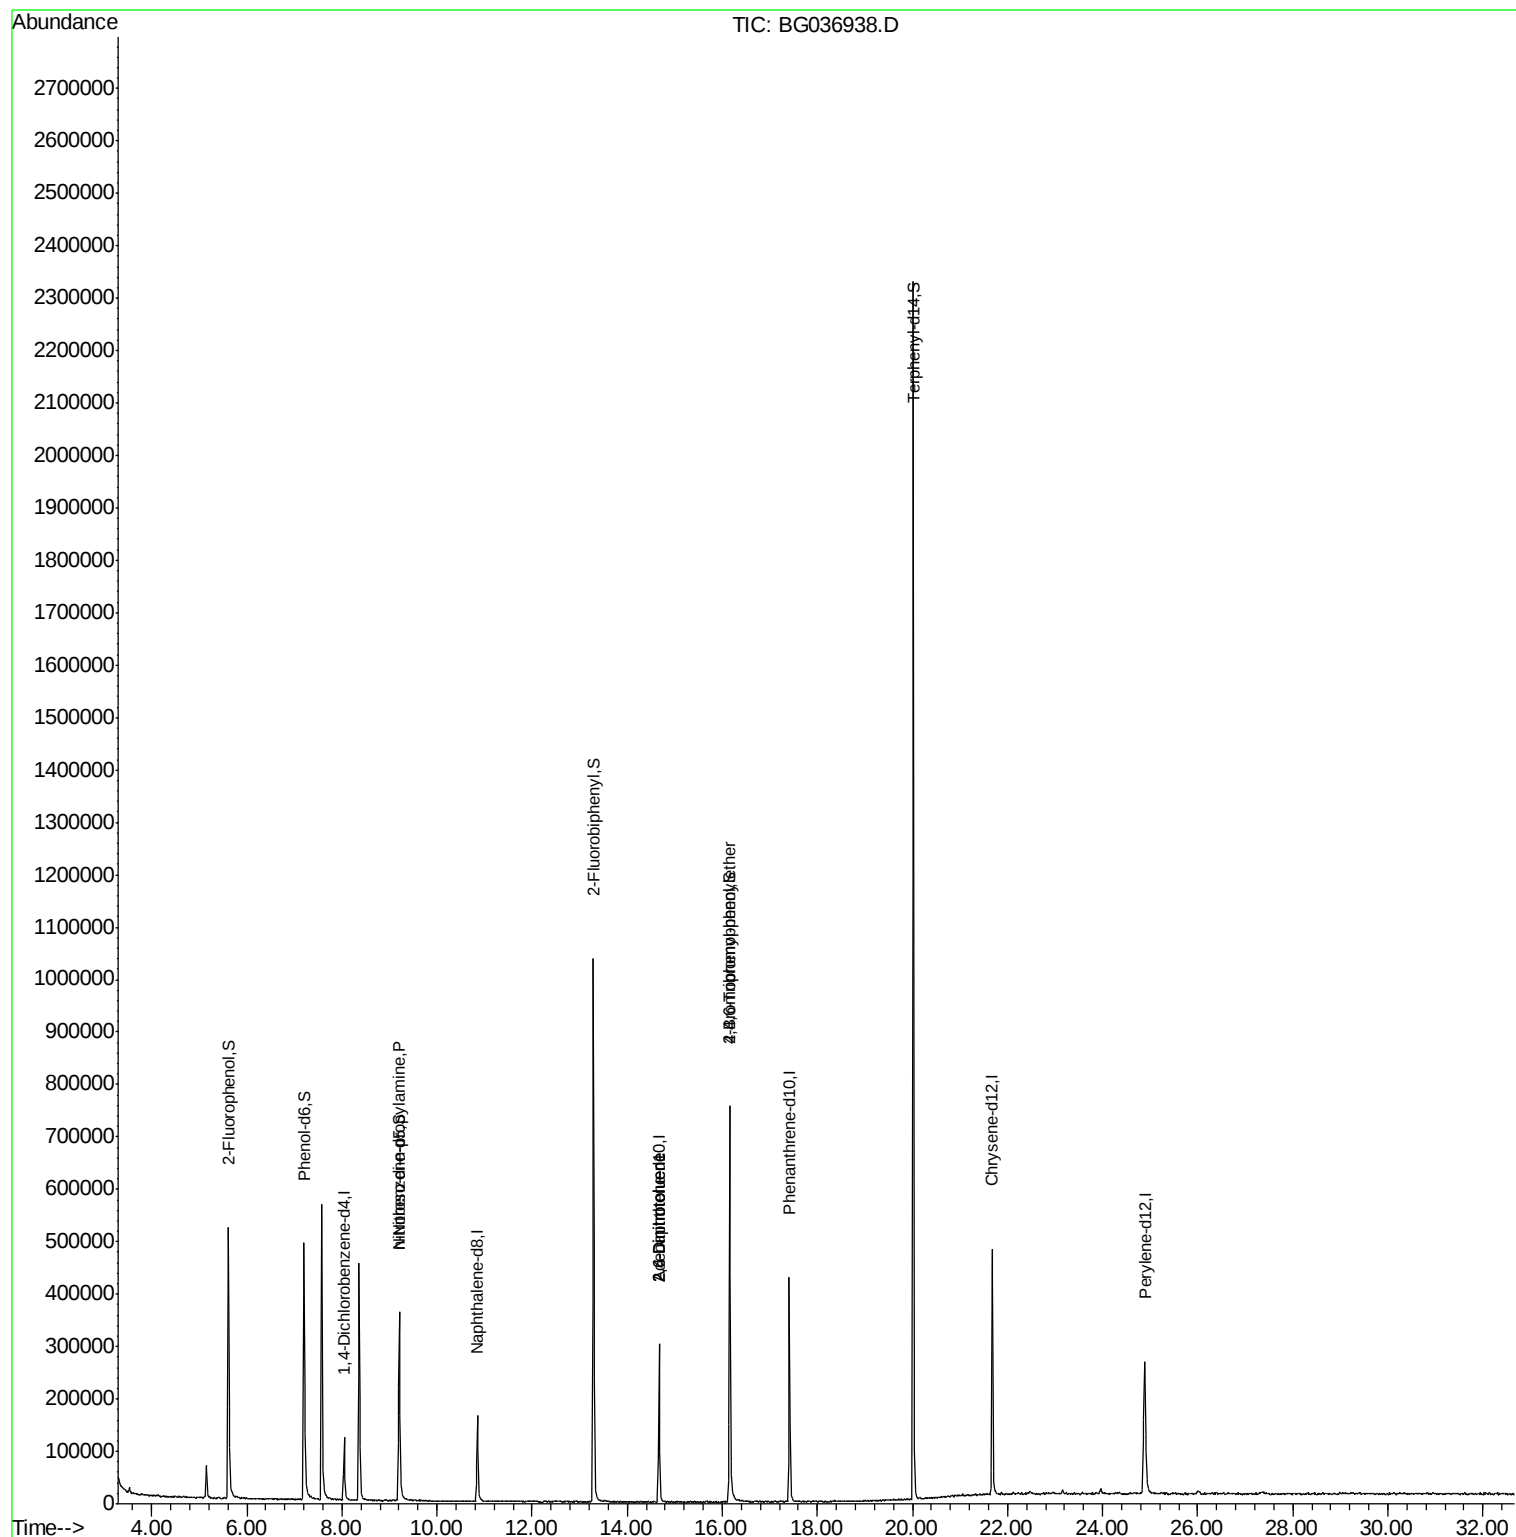

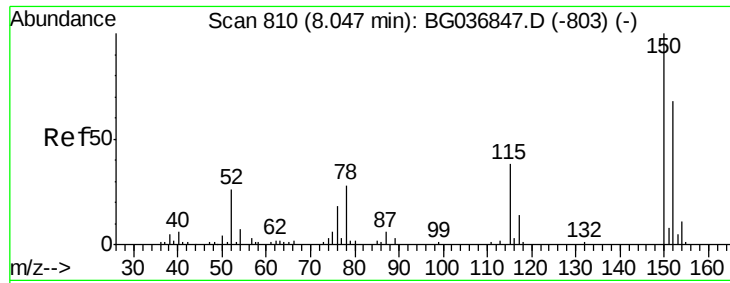


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.05 min Scan# 810
Delta R.T. 0.00 min
Lab File: BG036938.D
Acq: 25 Sep 2018 4:54

Instrument :
BNA_G
ClientSampleId :
JC-02-092118-J

Tgt Ion	Ratio	Lower	Upper
152	100		
150	146.3	119.5	179.3
115	56.8	44.5	66.7



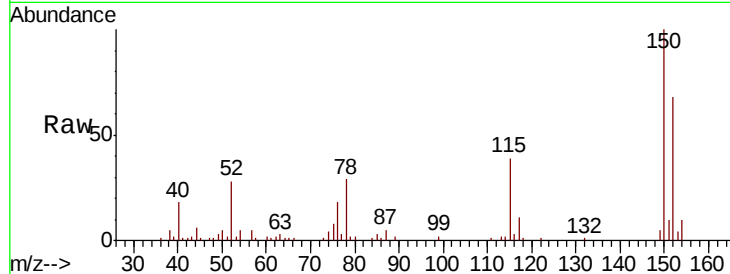


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

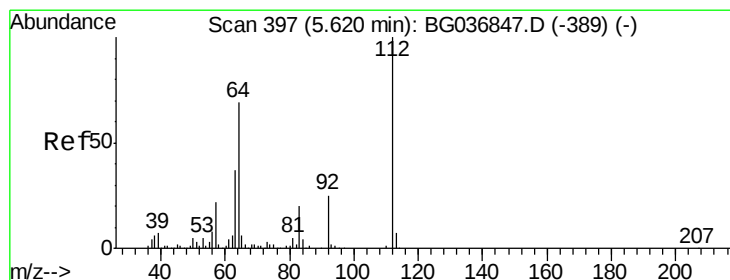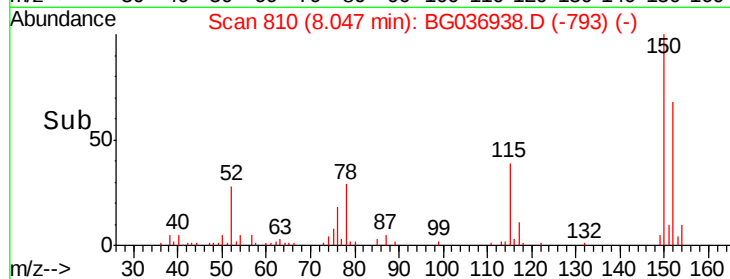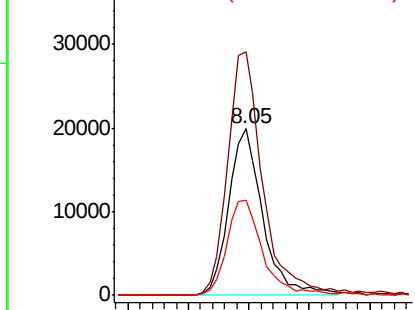

#5

2-Fluorophenol
Concen: 120.571 ng
RT: 5.61 min Scan# 396
Delta R.T. -0.01 min
Lab File: BG036938.D
Acq: 25 Sep 2018 4:54

Tgt Ion	Ratio	Lower	Upper
112	100		
64	71.5	57.2	85.8
63	38.8	30.8	46.2


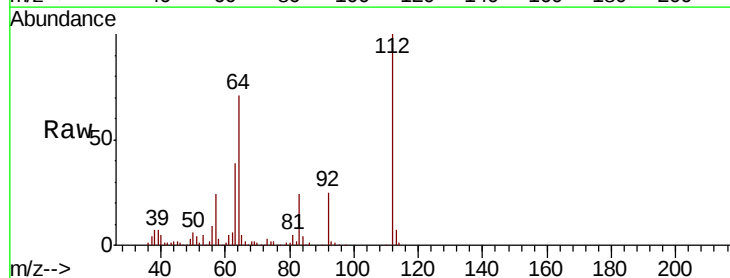





Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG

Ion 63.00 (62.70 to 63.70): BG

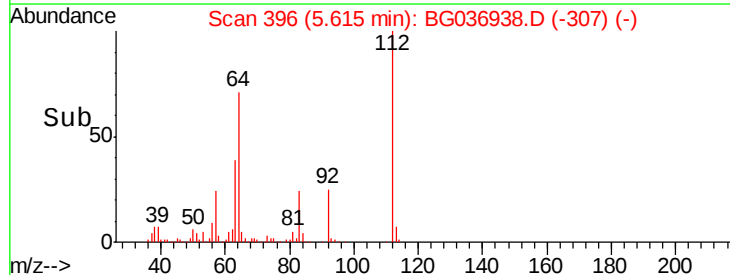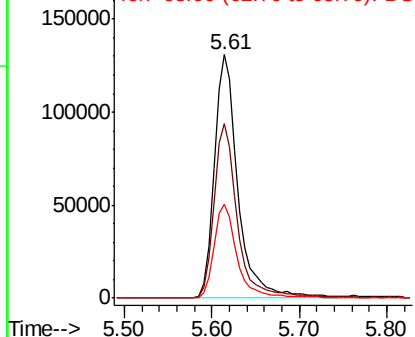

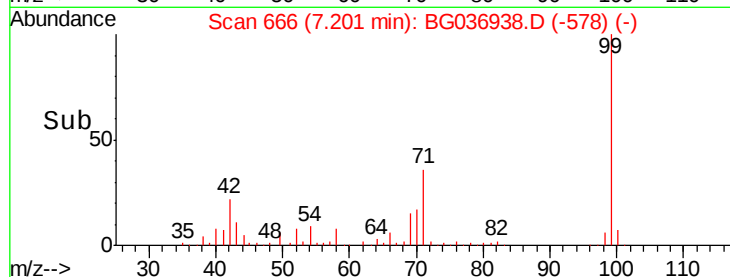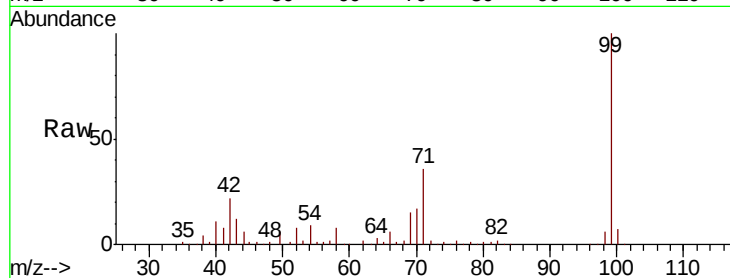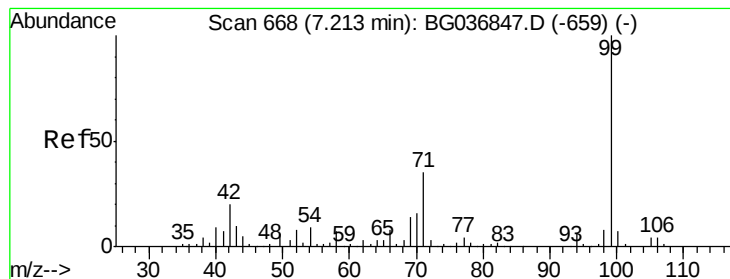

#7

Phenol-d6

Concen: 101.168 ng

RT: 7.20 min Scan# 666

Delta R.T. -0.01 min

Lab File: BG036938.D

Acq: 25 Sep 2018 4:54

Instrument :

BNA_G

ClientSampleId :

JC-02-092118-J





Tgt Ion: 99 Resp: 317890

Ion Ratio Lower Upper

99 100

42 21.9 16.5 24.7

71 36.0 29.4 44.2

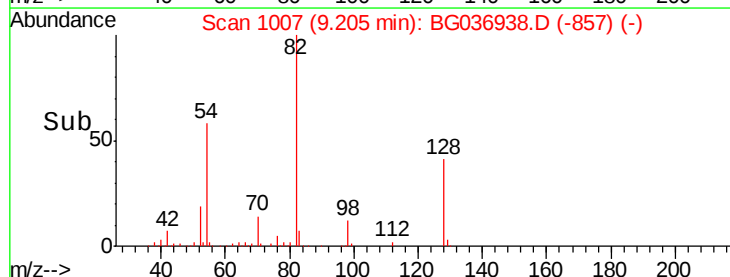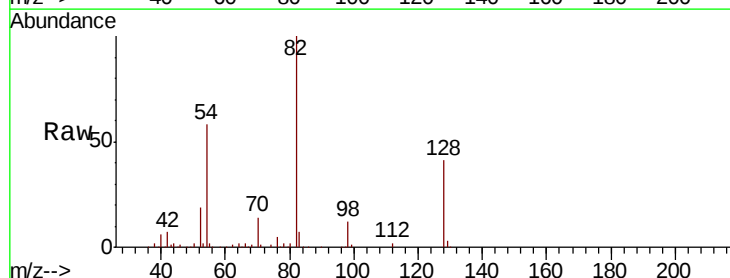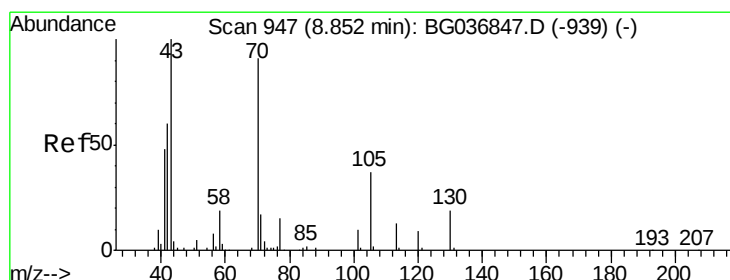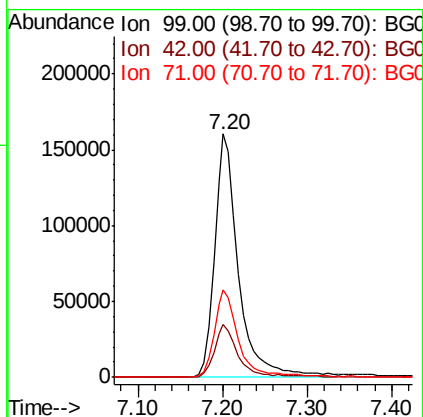

#19

n-Nitroso-di-n-propylamine

Concen: 13.045 ng

RT: 9.20 min Scan# 1007

Delta R.T. 0.35 min

Lab File: BG036938.D

Acq: 25 Sep 2018 4:54

Tgt Ion: 70 Resp: 34100


Ion Ratio Lower Upper

70 100

42 50.8 56.2 84.4#

101 0.0 7.8 11.6#

130 1.8 16.2 24.2#

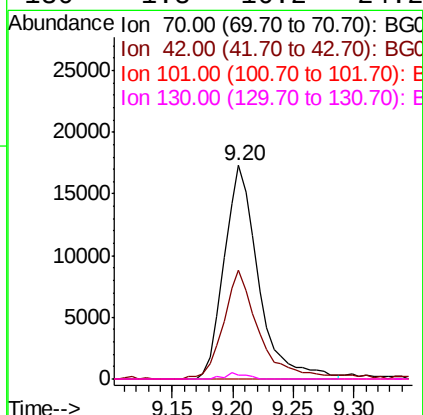







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.85 min Scan# 1287
Delta R.T. -0.01 min
Lab File: BG036938.D
Acq: 25 Sep 2018 4:54

Instrument :
BNA_G
ClientSampleId :
JC-02-092118-J

Tgt Ion:	136	Resp:	162618
Ion	Ratio	Lower	Upper
136	100		
137	9.5	8.8	13.2
54	11.2	9.2	13.8
68	6.2	5.8	8.6

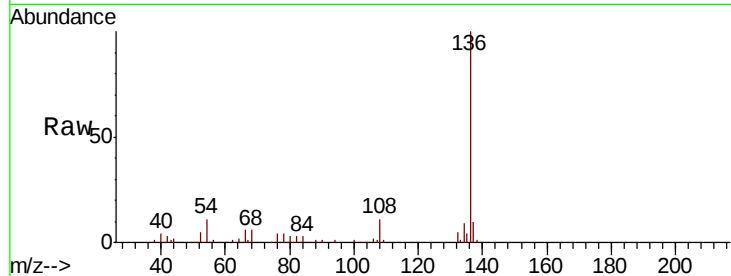


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

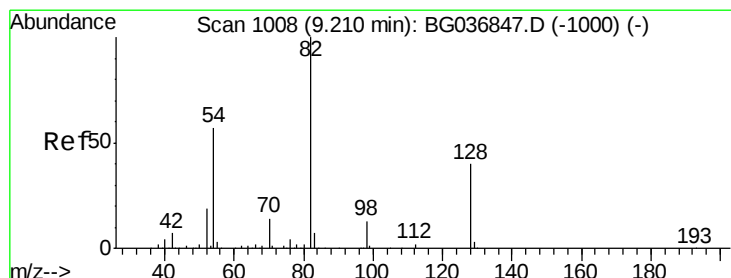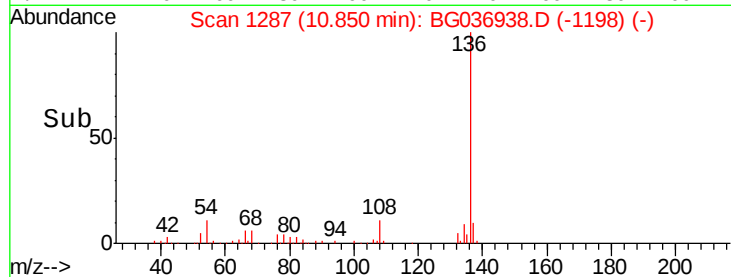
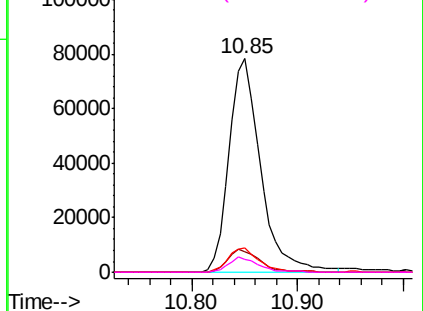



#23
Nitrobenzene-d5
Concen: 84.976 ng
RT: 9.20 min Scan# 1007
Delta R.T. -0.01 min
Lab File: BG036938.D
Acq: 25 Sep 2018 4:54

Tgt Ion:	82	Resp:	258046
Ion	Ratio	Lower	Upper
82	100		
128	41.3	33.3	49.9
54	58.2	45.1	67.7

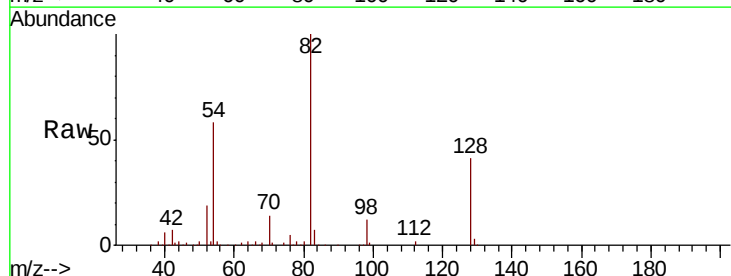

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC

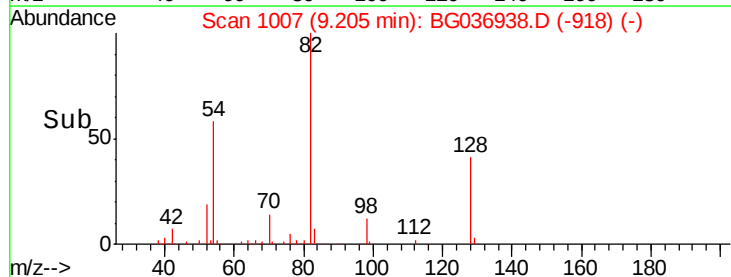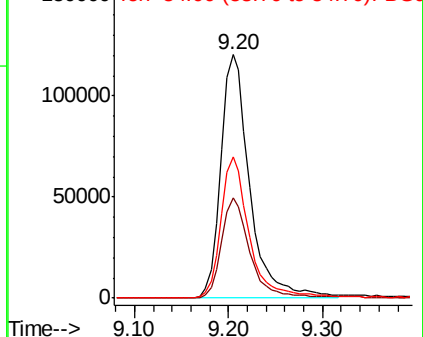

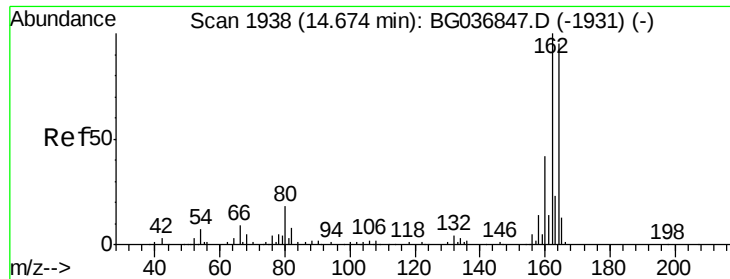

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.67 min Scan# 1937

Delta R.T. -0.01 min

Lab File: BG036938.D

Acq: 25 Sep 2018 4:54

Instrument :

BNA_G

ClientSampleId :

JC-02-092118-J


Tgt Ion:164 Resp: 113816

Ion Ratio Lower Upper

164 100

162 102.4 80.7 121.1




160 44.6 35.3 52.9

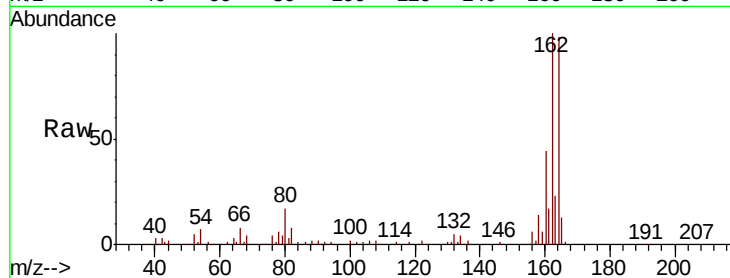

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

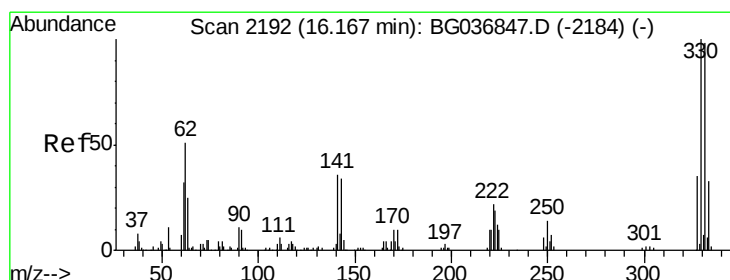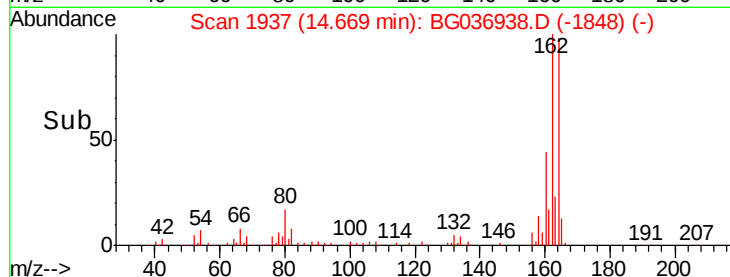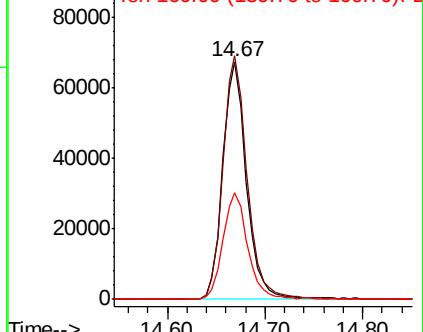

#41

2,4,6-Tribromophenol

Concen: 114.060 ng

RT: 16.16 min Scan# 2190

Delta R.T. -0.01 min

Lab File: BG036938.D

Acq: 25 Sep 2018 4:54


Tgt Ion:330 Resp: 155320

Ion Ratio Lower Upper

330 100

332 97.6 75.4 113.2



141 38.7 30.7 46.1

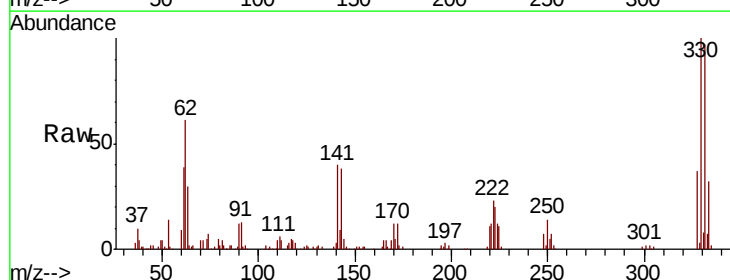


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



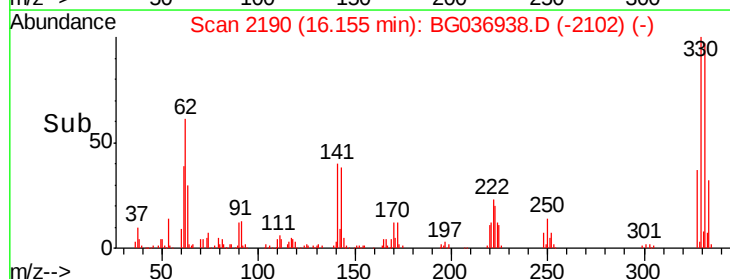
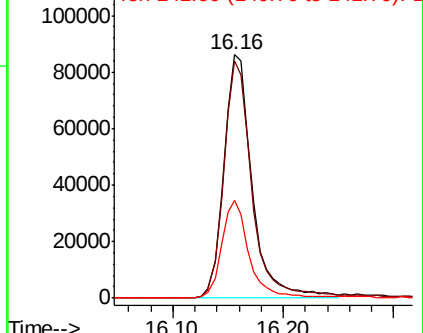


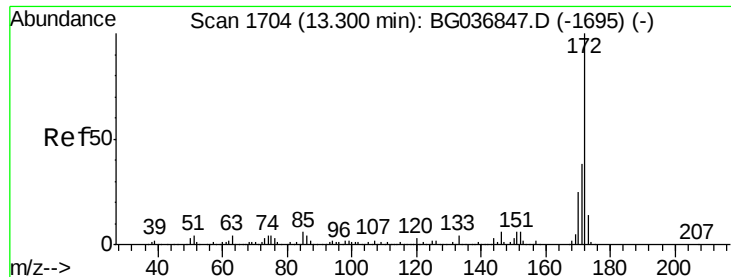

#44
 2-Fluorobiphenyl
 Concen: 79.489 ng
 RT: 13.29 min Scan# 1703
 Delta R.T. -0.01 min
 Lab File: BG036938.D
 Acq: 25 Sep 2018 4:54




Instrument :
 BNA_G
 ClientSampleId :
 JC-02-092118-J


Tgt Ion:172 Resp: 607438
 Ion Ratio Lower Upper
 172 100
 171 37.6 31.3 46.9
 170 24.4 21.0 31.6

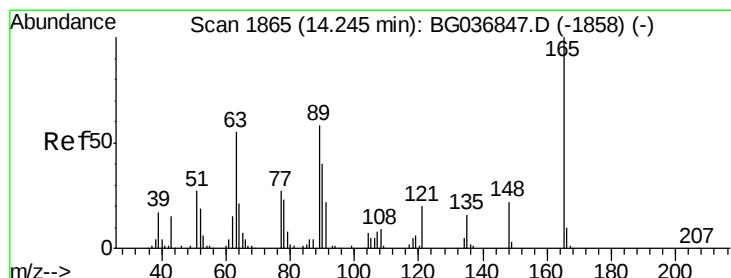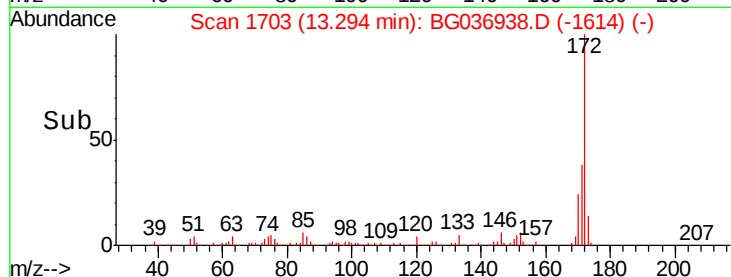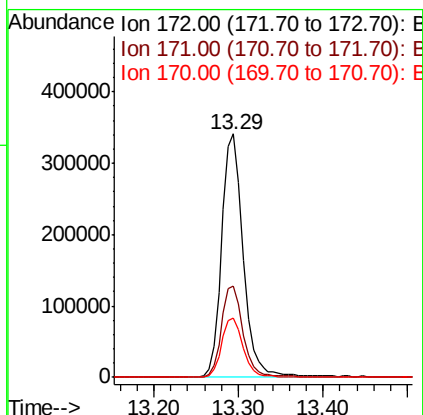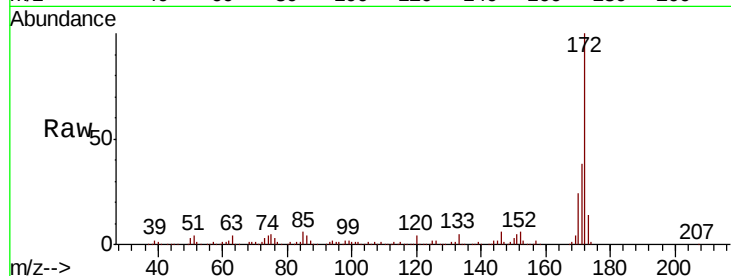

#50
 2,6-Dinitrotoluene
 Concen: 7.147 ng
 RT: 14.67 min Scan# 1937
 Delta R.T. 0.42 min
 Lab File: BG036938.D
 Acq: 25 Sep 2018 4:54

Tgt Ion:165 Resp: 14285
 Ion Ratio Lower Upper
 165 100
 63 0.0 50.1 75.1#
 89 2.1 47.8 71.6#

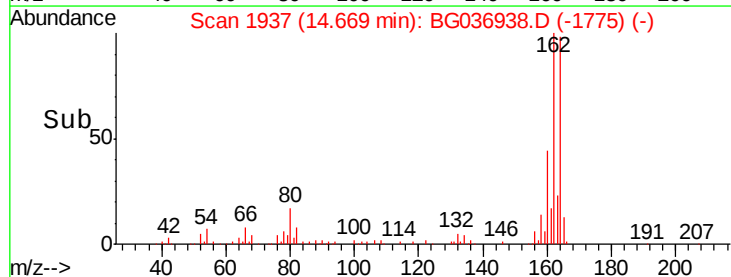
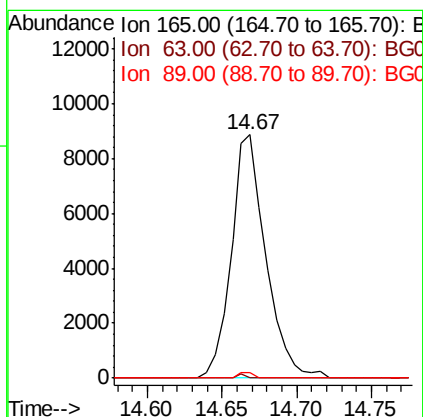
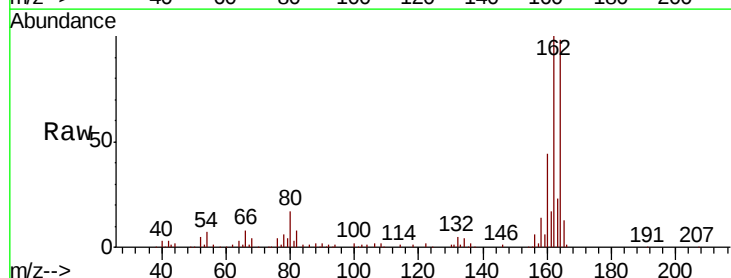


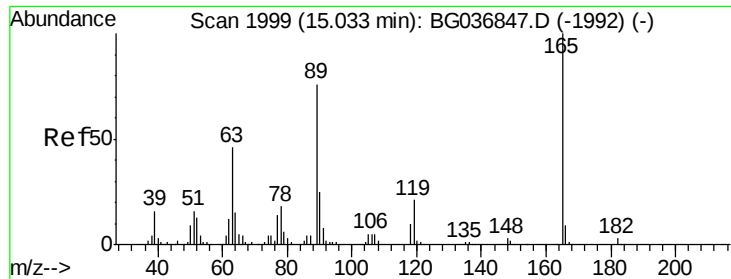

#56
 2,4-Dinitrotoluene
 Concen: 5.122 ng
 RT: 14.67 min Scan# 1937
 Delta R.T. -0.36 min
 Lab File: BG036938.D
 Acq: 25 Sep 2018 4:54




Instrument :
 BNA_G
 ClientSampleId :
 JC-02-092118-J

Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	40.1	60.1#
89	2.1	63.7	95.5#
182	0.0	2.5	3.7#

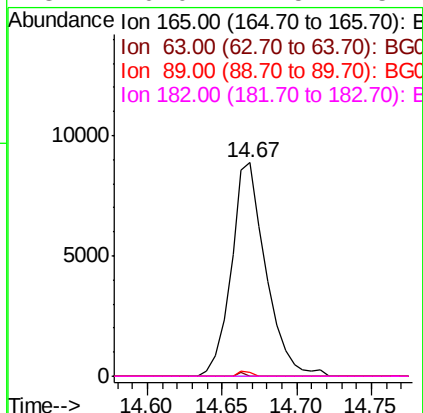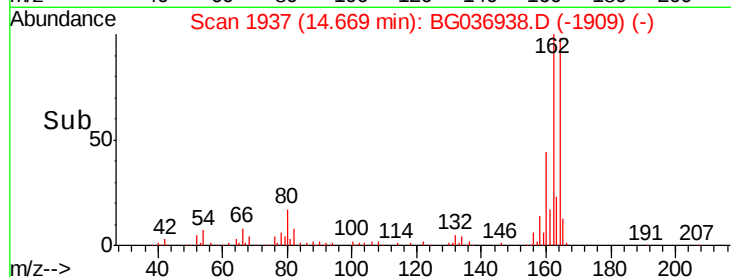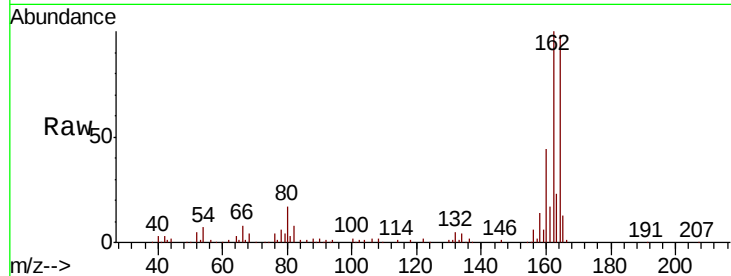

#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.41 min Scan# 2404
 Delta R.T. -0.01 min
 Lab File: BG036938.D
 Acq: 25 Sep 2018 4:54

Tgt Ion	Ratio	Lower	Upper
188	100		
94	7.1	6.7	10.1
80	8.8	8.1	12.1

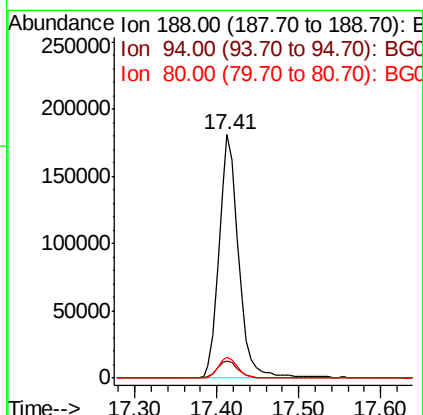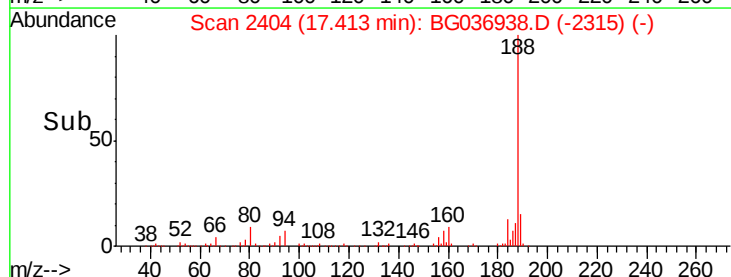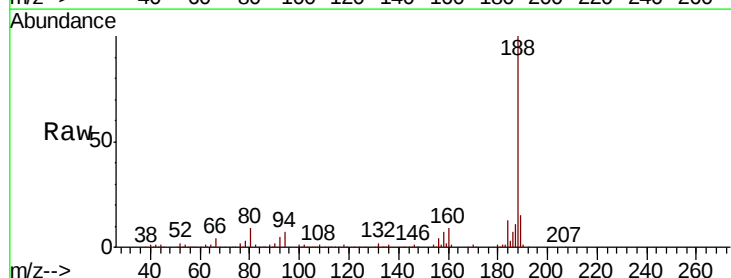






#66
 4-Bromophenyl-phenylether
 Concen: 3.083 ng
 RT: 16.16 min Scan# 2190
 Delta R.T. -0.45 min
 Lab File: BG036938.D
 Acq: 25 Sep 2018 4:54

Instrument :
 BNA_G
 ClientSampleId :
 JC-02-092118-J

Tgt Ion:248 Resp: 10590
 Ion Ratio Lower Upper
 248 100
 250 192.9 78.1 117.1#
 141 548.7 53.7 80.5#

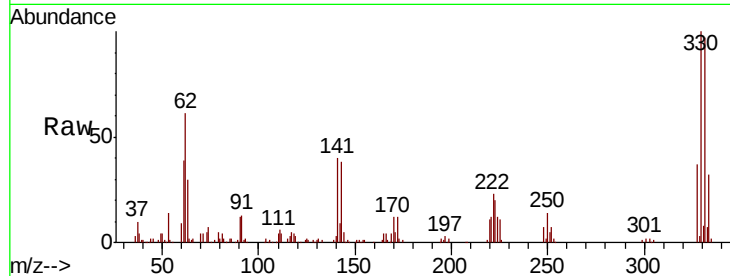


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

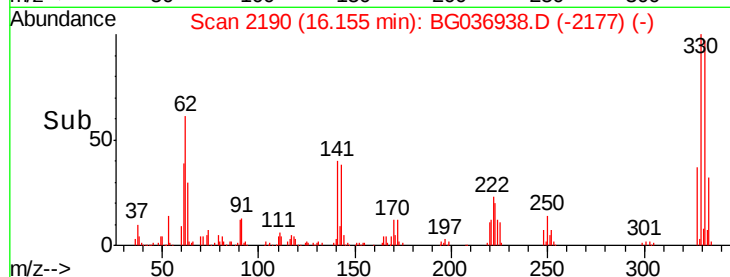
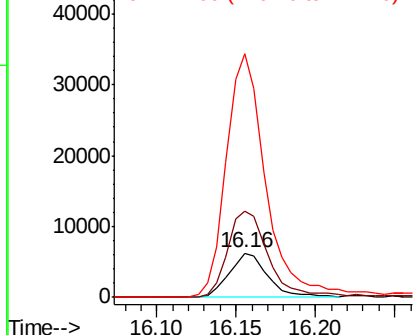



#75
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.68 min Scan# 3130
 Delta R.T. -0.01 min
 Lab File: BG036938.D
 Acq: 25 Sep 2018 4:54

Tgt Ion:240 Resp: 316928
 Ion Ratio Lower Upper
 240 100
 120 8.0 6.9 10.3
 236 26.5 21.2 31.8

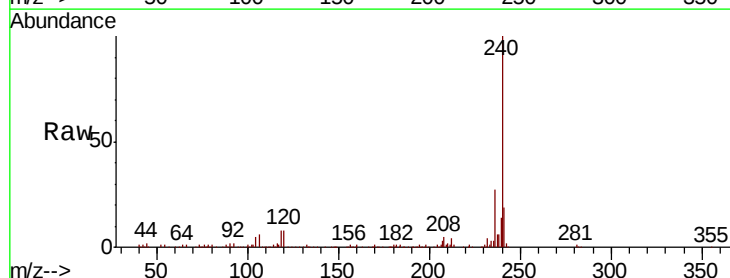

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

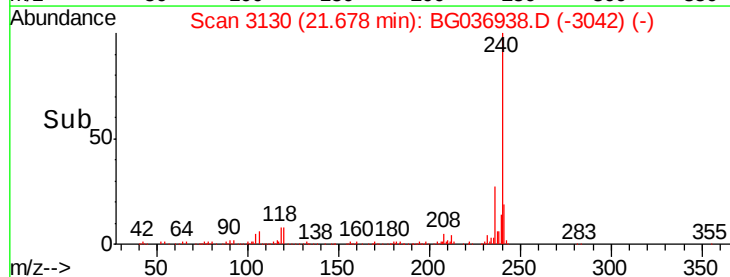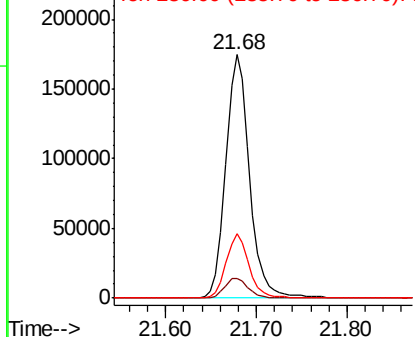

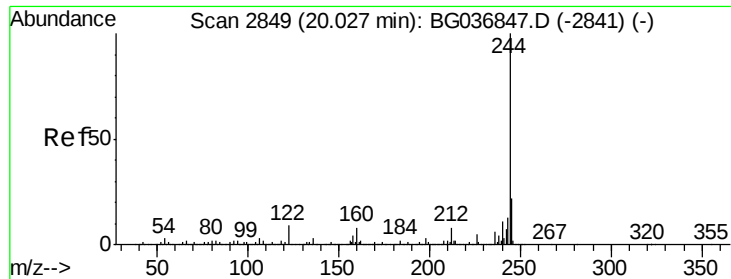

#78

Terphenyl-d14

Concen: 94.483 ng

RT: 20.02 min Scan# 2848

Delta R.T. -0.01 min

Lab File: BG036938.D

Acq: 25 Sep 2018 4:54

Instrument :

BNA_G

ClientSampleId :

JC-02-092118-J


Tgt Ion:244 Resp: 1138786

Ion	Ratio	Lower	Upper
244	100		
212	8.6	7.0	10.6
122	8.6	7.1	10.7

244 100

212 8.6 7.0 10.6

122 8.6 7.1 10.7



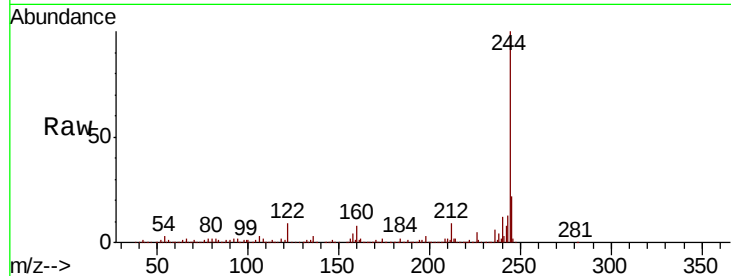


Abundance

Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

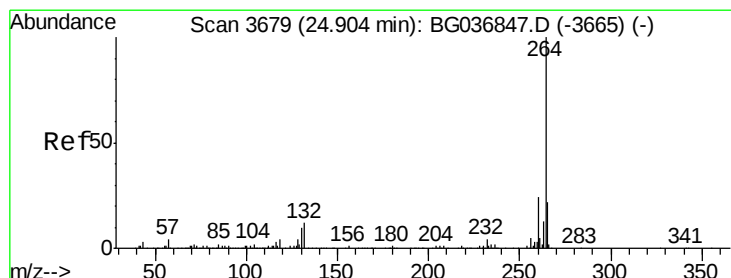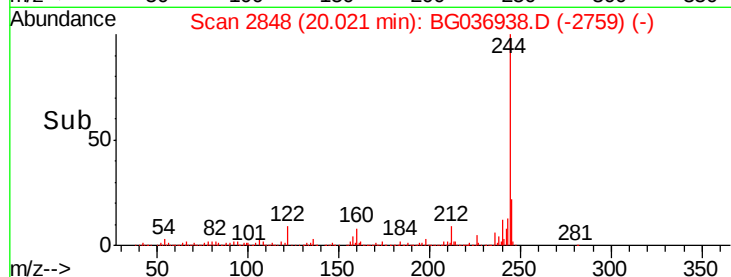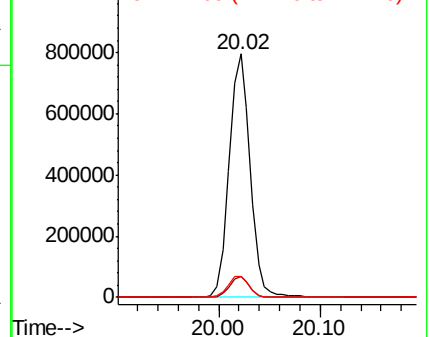

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.89 min Scan# 3676

Delta R.T. -0.02 min

Lab File: BG036938.D

Acq: 25 Sep 2018 4:54


Tgt Ion:264 Resp: 305456

Ion	Ratio	Lower	Upper
264	100		
260	24.2	19.6	29.4
265	22.7	17.4	26.0

264 100

260 24.2 19.6 29.4

265 22.7 17.4 26.0

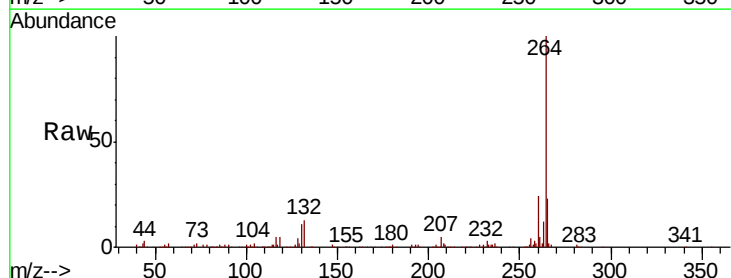

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

