
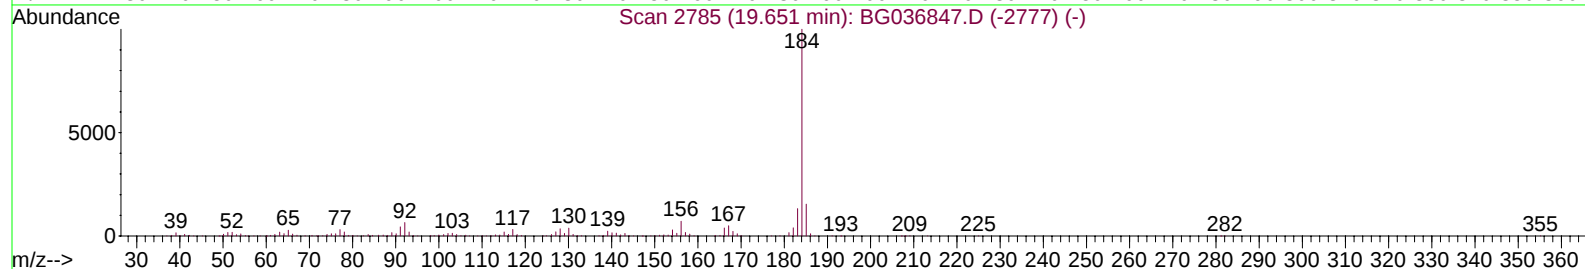
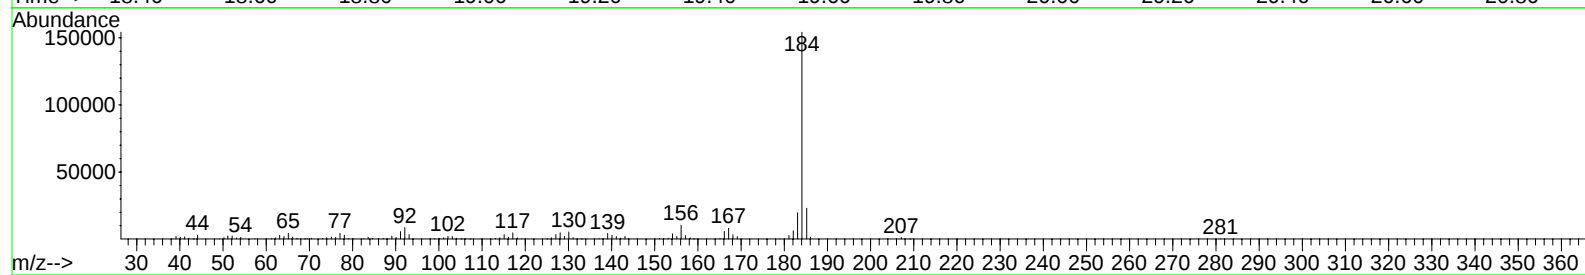


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG092418\
Data File : BG036917.D
Acq On : 24 Sep 2018 14:29
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 24 19:20:15 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 24 10:41:23 2018
Response via : Initial Calibration

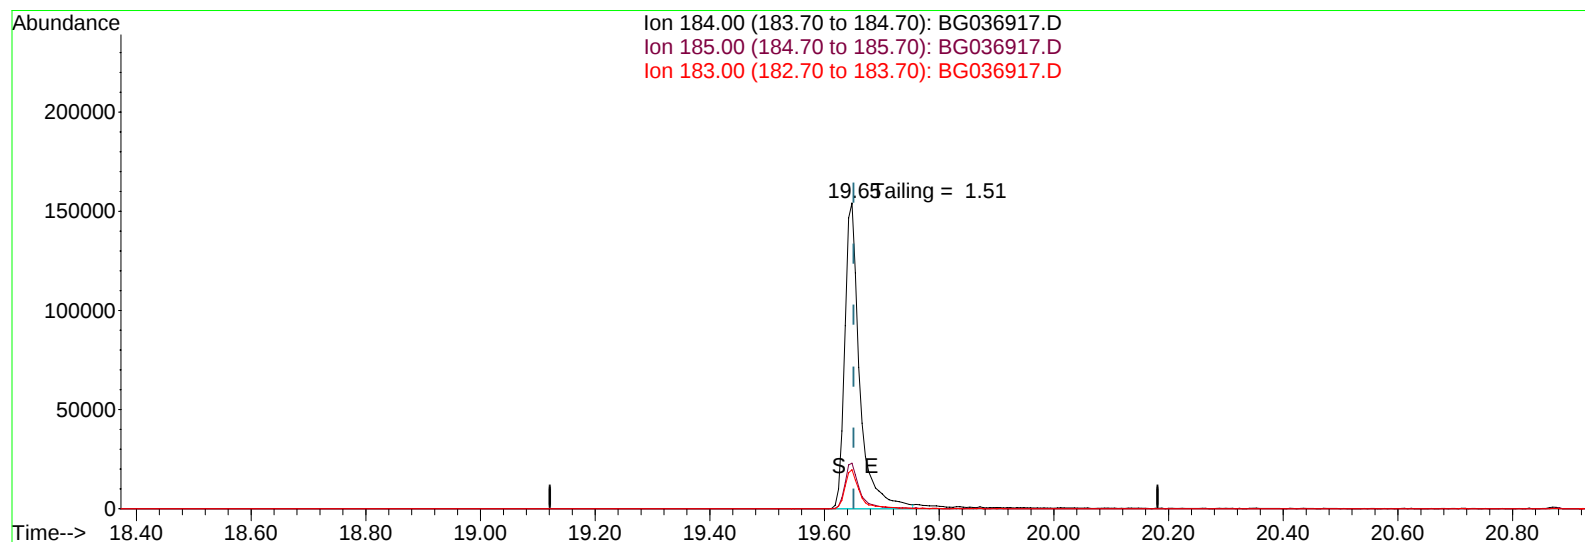

TIC: BG036917.D

(76) Benzidine




19.648min (-0.003) 0.00ng

response 286337

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.92
183.00	13.60	12.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG092418\
Data File : BG036917.D
Acq On : 24 Sep 2018 14:29
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 24 19:20:15 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 24 10:41:23 2018
Response via : Initial Calibration

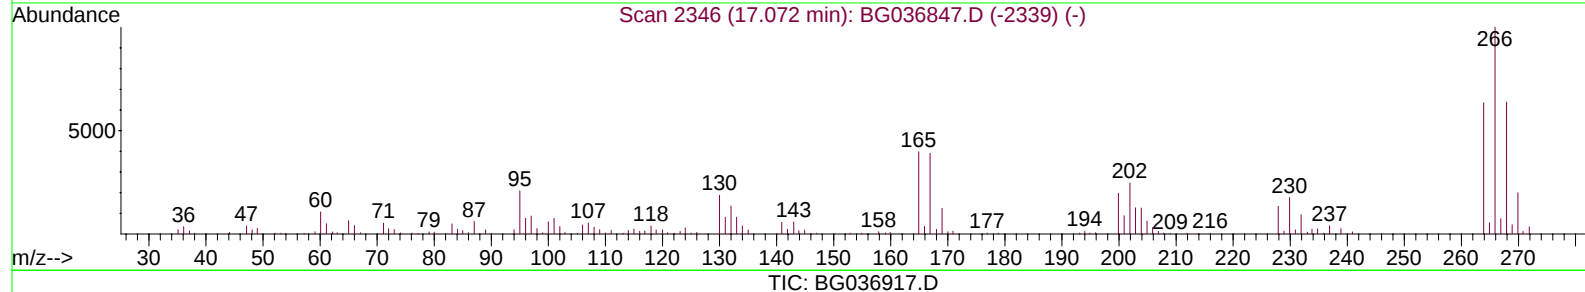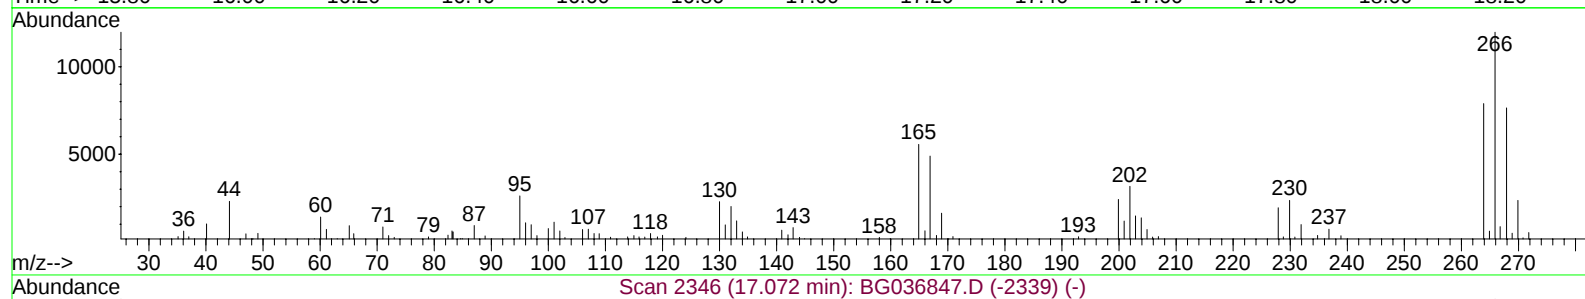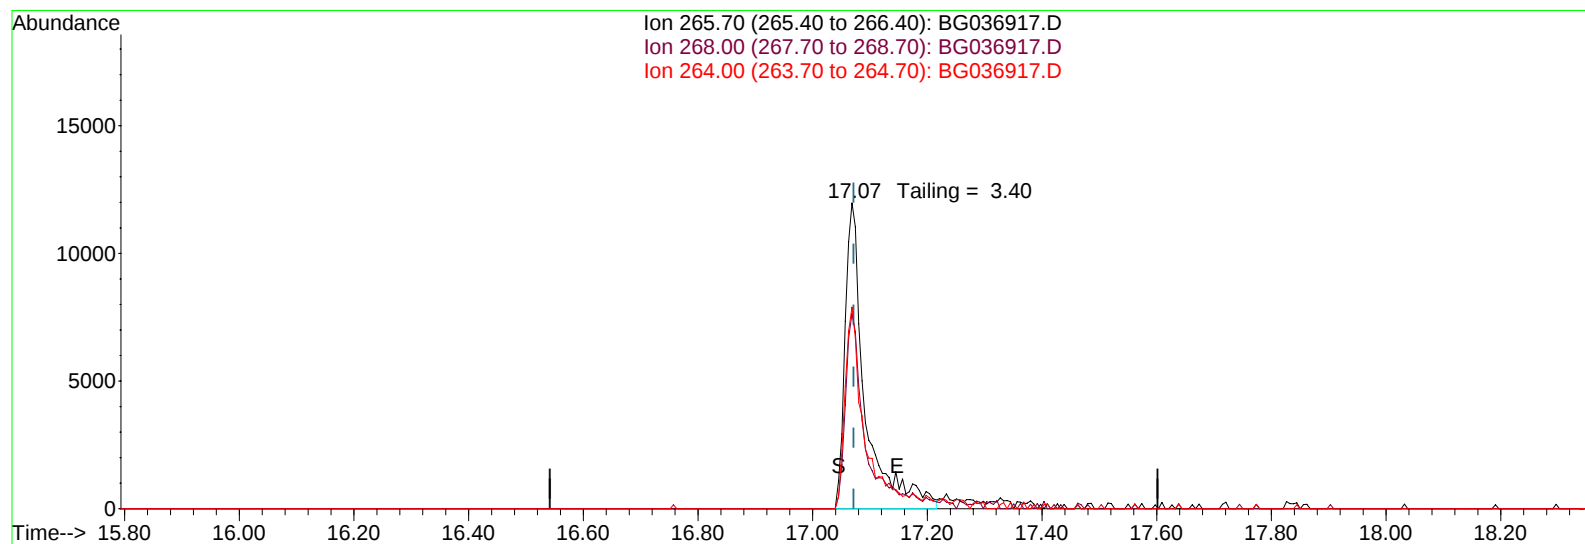

(69) Pentachlorophenol (C)

17.069min (-0.003) 26837.62ng

response 26129

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	63.85
264.00	61.10	65.93
0.00	0.00	0.00