

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG092418\
 Data File : BG036922.D
 Acq On : 24 Sep 2018 17:52
 Operator : JU/SJ
 Sample : J4770-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JC-02-092118-A

Quant Time: Sep 25 07:14:11 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 24 10:41:23 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	39747	20.00	ng	0.00
21) Naphthalene-d8	10.85	136	168385	20.00	ng	0.00
38) Acenaphthene-d10	14.67	164	113578	20.00	ng	0.00
63) Phenanthrene-d10	17.41	188	300438	20.00	ng	0.00
75) Chrysene-d12	21.68	240	318019	20.00	ng	-0.01
86) Perylene-d12	24.88	264	320369	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.62	112	246627	119.00	ng	0.00
7) Phenol-d6	7.20	99	315176	98.29	ng	-0.01
23) Nitrobenzene-d5	9.20	82	262501	83.48	ng	0.00
41) 2,4,6-Tribromophenol	16.16	330	157667	116.03	ng	-0.01
44) 2-Fluorobiphenyl	13.29	172	598834	78.53	ng	0.00
78) Terphenyl-d14	20.02	244	1101451	91.07	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG092418\
Data File : BG036922.D
Acq On : 24 Sep 2018 17:52
Operator : JU/SJ
Sample : J4770-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JC-02-092118-A

Quant Time: Sep 25 07:14:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 24 10:41:23 2018
Response via : Initial Calibration

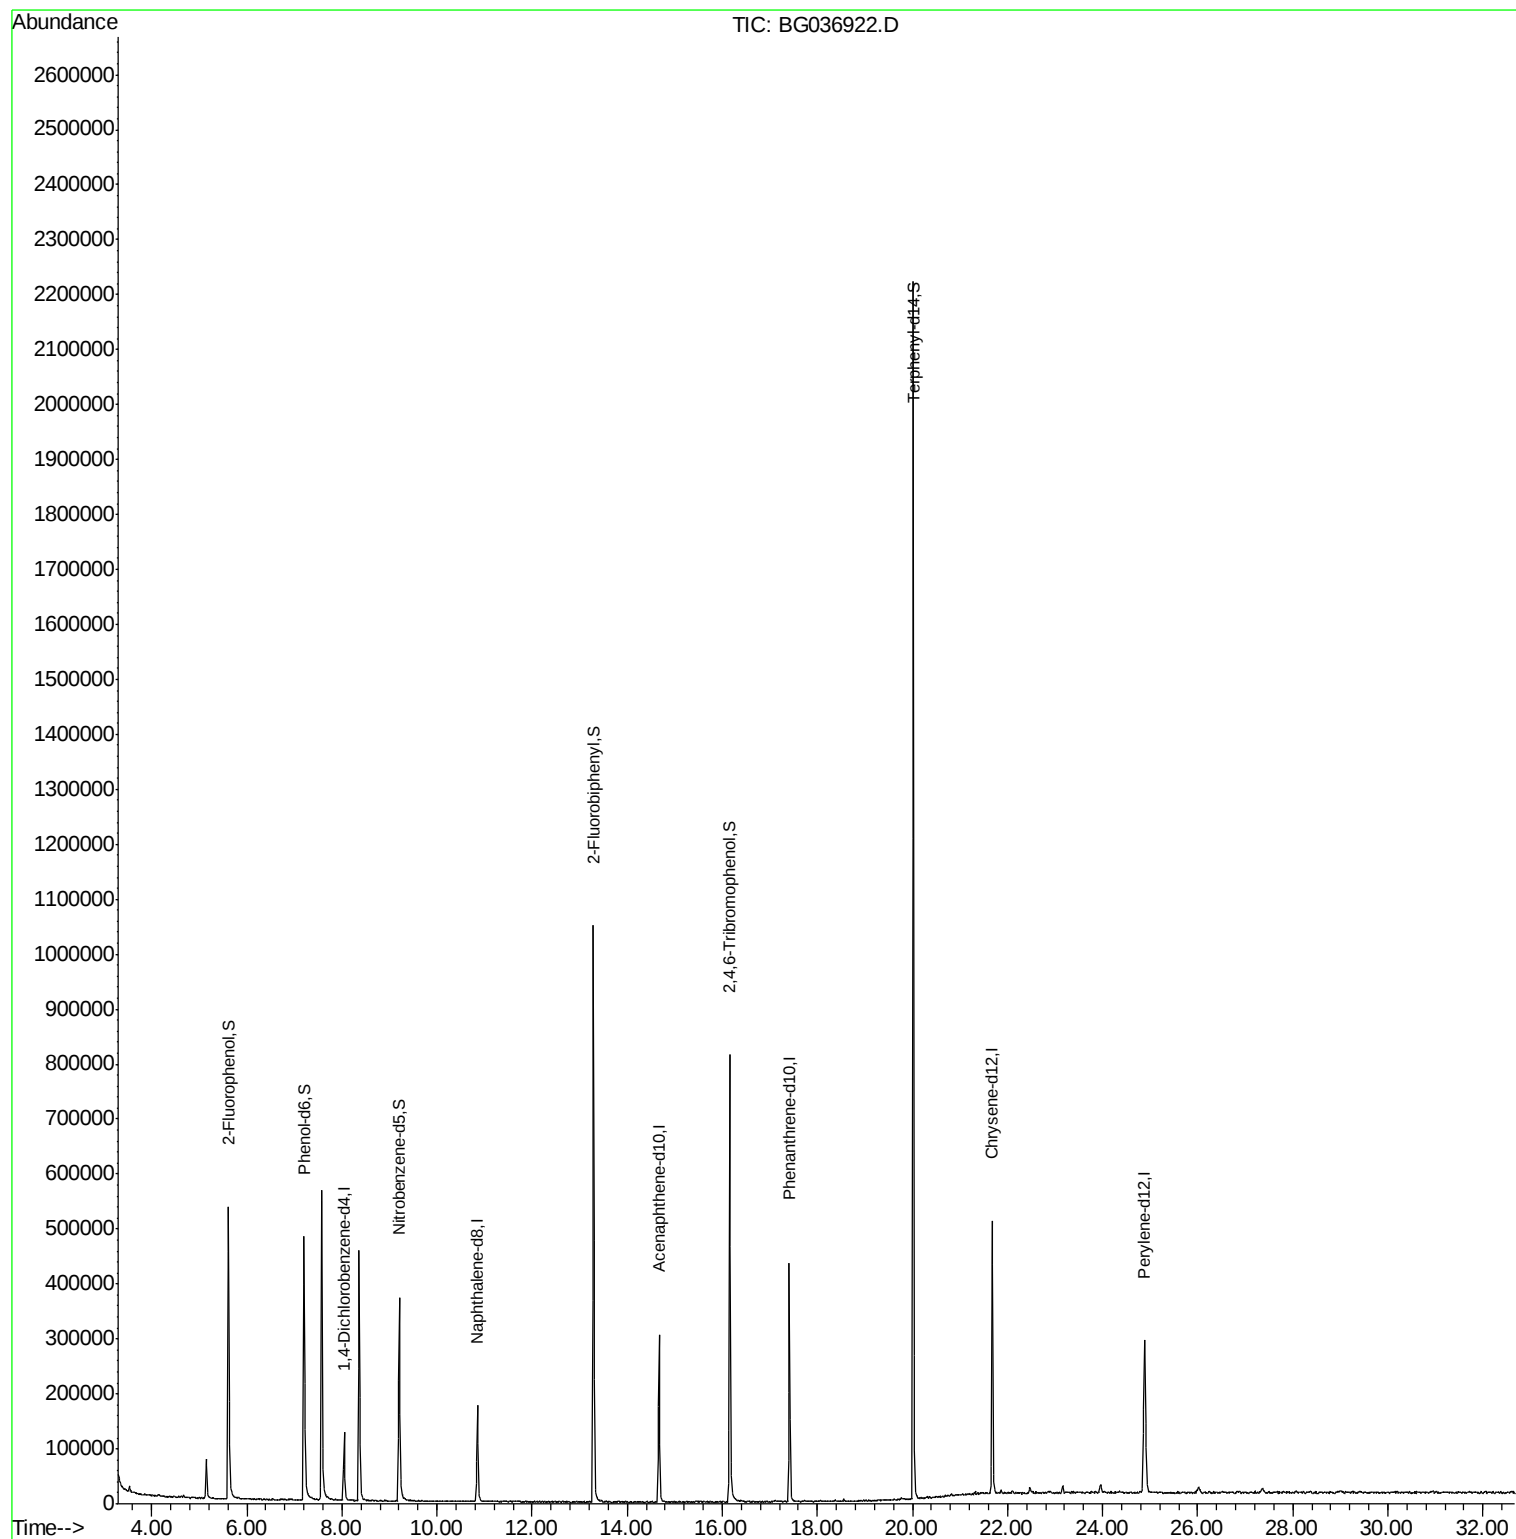

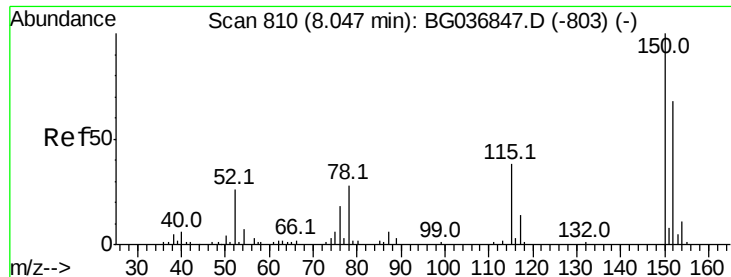


#1

1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.04 min Scan# 809
 Delta R.T. -0.01 min
 Lab File: BG036922.D
 Acq: 24 Sep 2018 17:52

Instrument :
 BNA_G
 ClientSampleId :
 JC-02-092118-A

Tot Ion	Ratio	Lower	Upper
152	100		
150	151.0	119.5	179.3
115	60.5	44.5	66.7



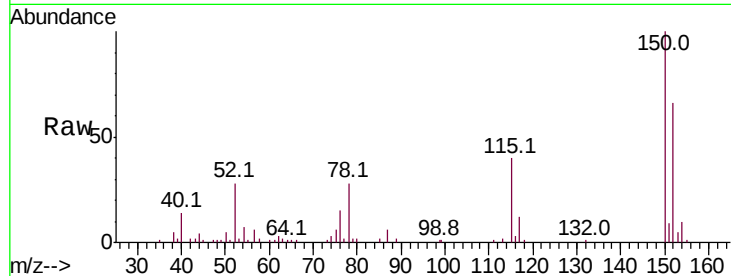


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

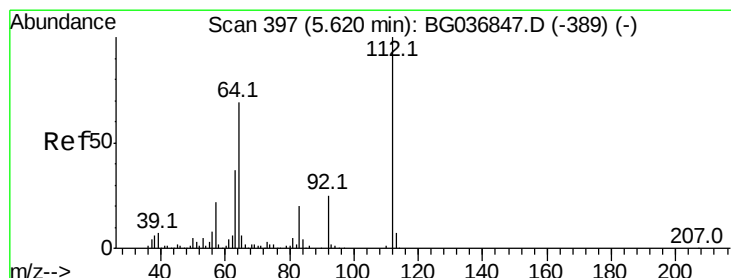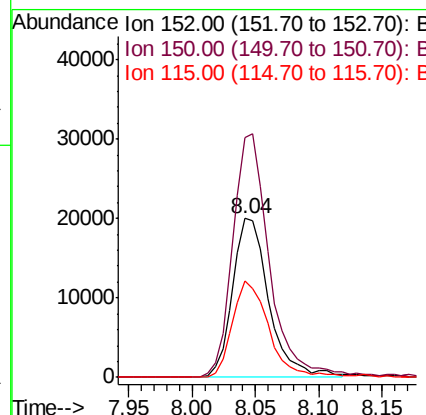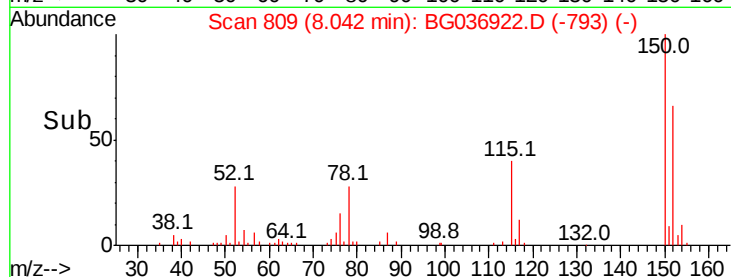

#5

2-Fluorophenol
 Concen: 118.997 ng
 RT: 5.62 min Scan# 396
 Delta R.T. -0.01 min
 Lab File: BG036922.D
 Acq: 24 Sep 2018 17:52

Tgt Ion	Ratio	Lower	Upper
112	100		
64	69.8	57.2	85.8
63	37.4	30.8	46.2


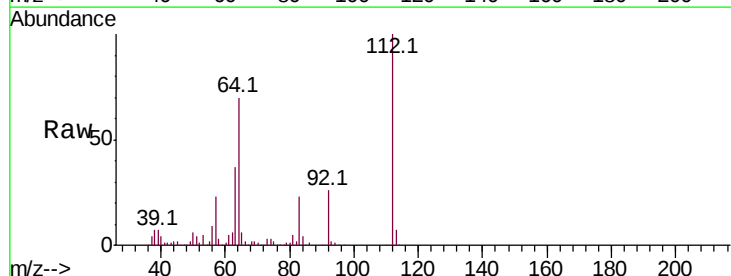



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG

Ion 63.00 (62.70 to 63.70): BG

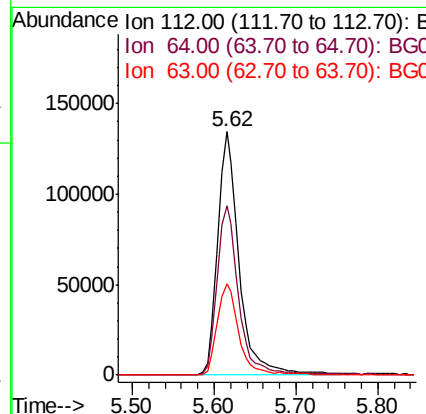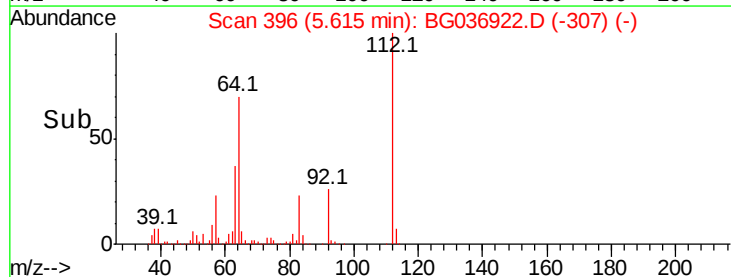

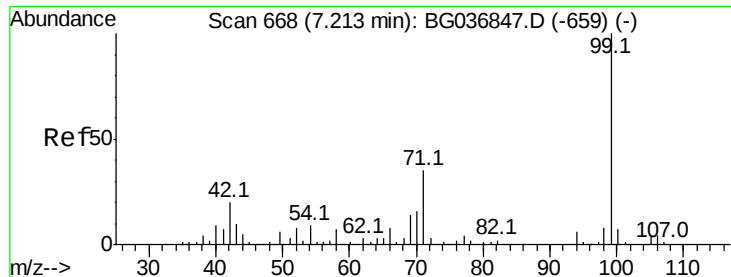

#7

Phenol-d6

Concen: 98.290 ng

RT: 7.20 min Scan# 666

Delta R.T. -0.01 min

Lab File: BG036922.D

Acq: 24 Sep 2018 17:52

Instrument :

BNA_G

ClientSampleId :

JC-02-092118-A





Tot Ion: 99 Resp: 315176

Ion Ratio Lower Upper

99 100

42 22.6 16.5 24.7

71 36.8 29.4 44.2

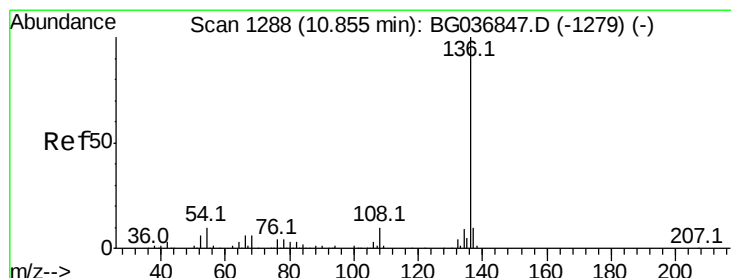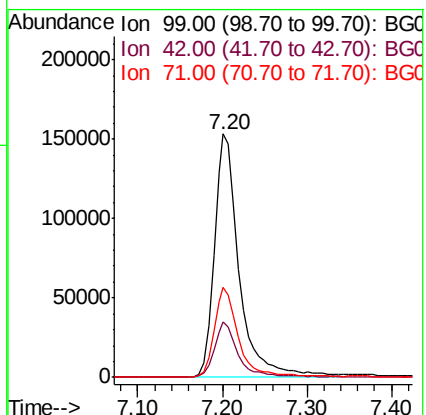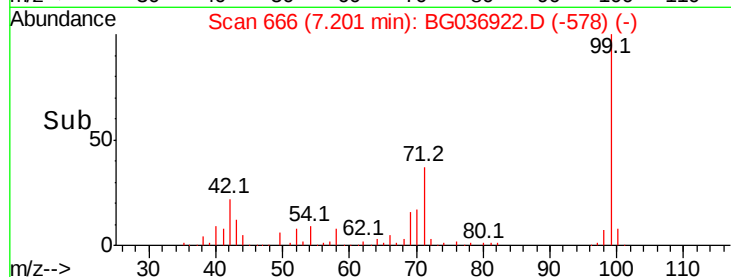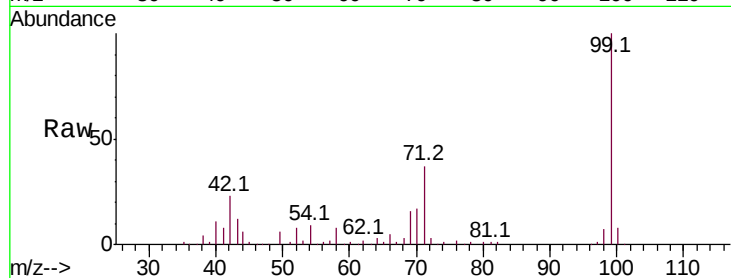

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.85 min Scan# 1287

Delta R.T. -0.01 min

Lab File: BG036922.D

Acq: 24 Sep 2018 17:52

Tgt Ion: 136 Resp: 168385




Ion Ratio Lower Upper


136 100

137 11.9 8.8 13.2

54 11.4 9.2 13.8

68 7.4 5.8 8.6


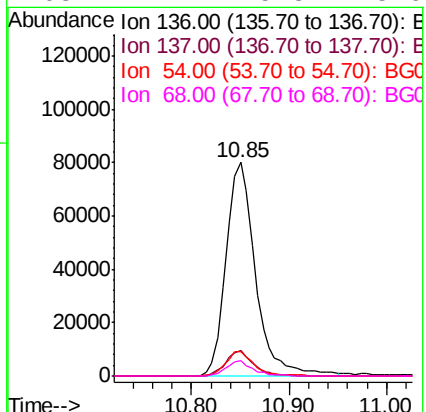
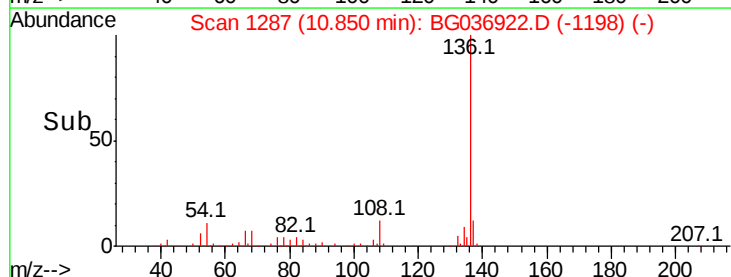
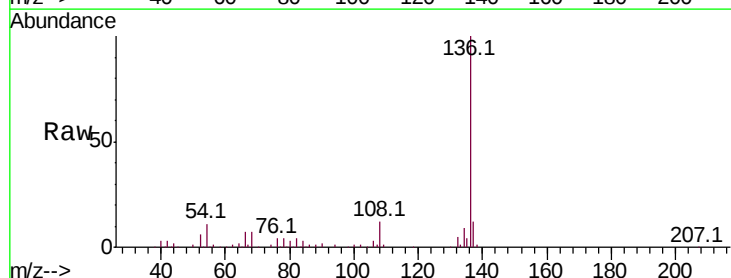


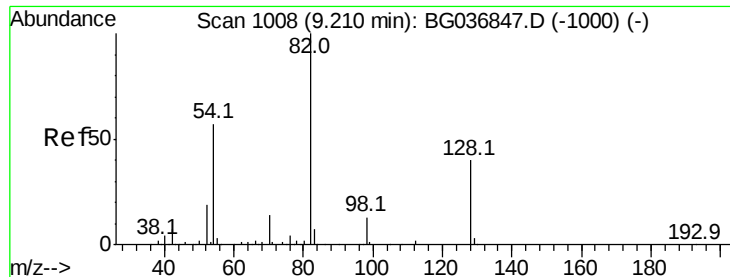

#23
 Nitrobenzene-d5
 Concen: 83.482 ng
 RT: 9.20 min Scan# 1007
 Delta R.T. -0.01 min
 Lab File: BG036922.D
 Acq: 24 Sep 2018 17:52




Instrument :
 BNA_G
 ClientSampleId :
 JC-02-092118-A


Tot Ion: 82 Resp: 262501
 Ion Ratio Lower Upper
 82 100
 128 40.1 33.3 49.9
 54 55.6 45.1 67.7

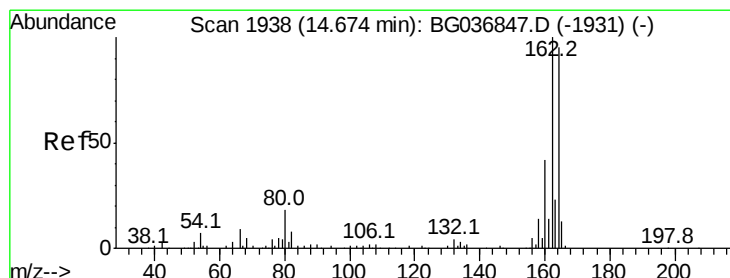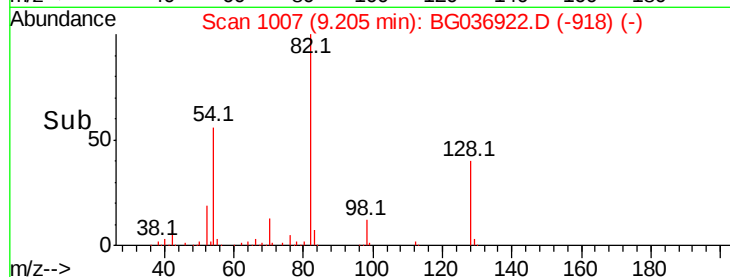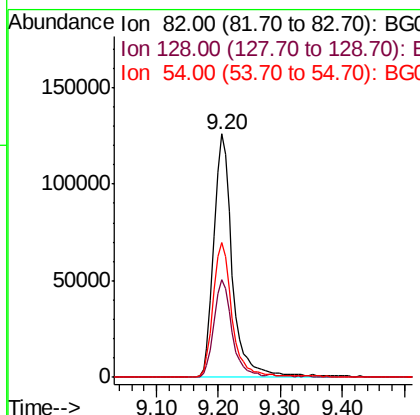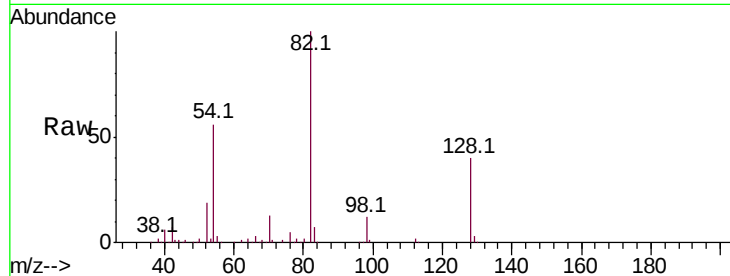

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.67 min Scan# 1937
 Delta R.T. -0.01 min
 Lab File: BG036922.D
 Acq: 24 Sep 2018 17:52

Tgt Ion: 164 Resp: 113578
 Ion Ratio Lower Upper
 164 100
 162 100.3 80.7 121.1
 160 44.9 35.3 52.9

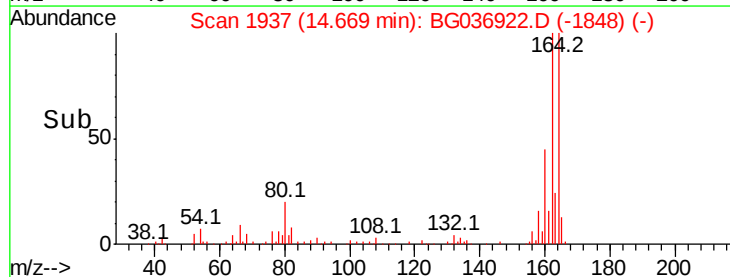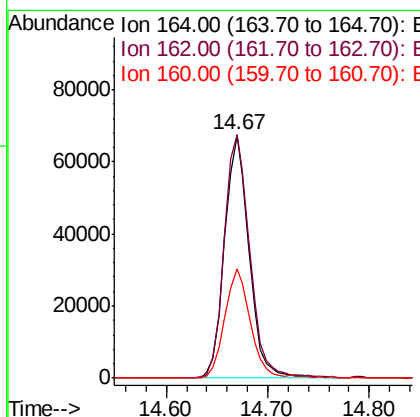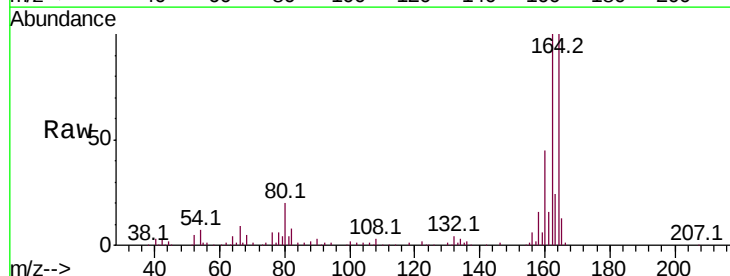


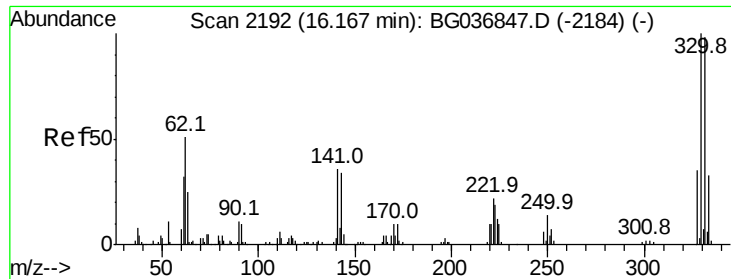

#41
 2,4,6-Tribromophenol
 Concen: 116.026 ng
 RT: 16.16 min Scan# 2190
 Delta R.T. -0.01 min
 Lab File: BG036922.D
 Acq: 24 Sep 2018 17:52

Instrument :
 BNA_G
 ClientSampleId :
 JC-02-092118-A

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.7	75.4	113.2
141	38.8	30.7	46.1



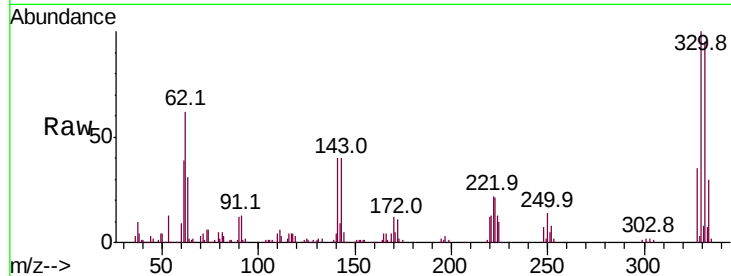


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

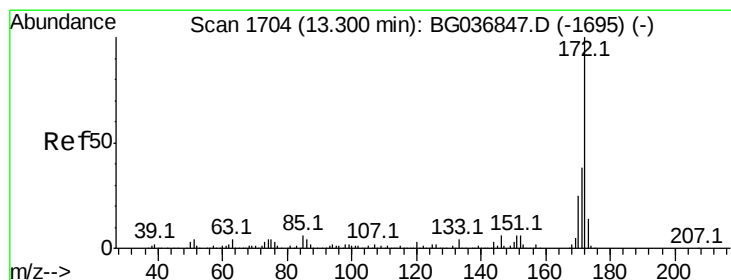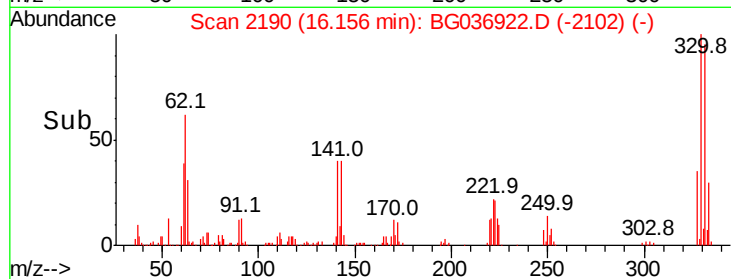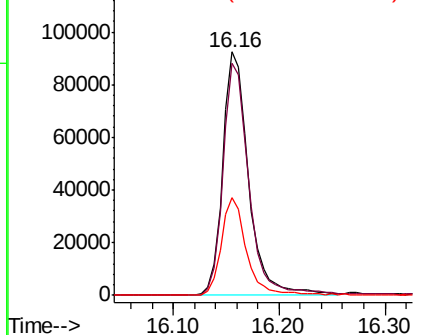

#44
 2-Fluorobiphenyl
 Concen: 78.527 ng
 RT: 13.29 min Scan# 1703
 Delta R.T. -0.01 min
 Lab File: BG036922.D
 Acq: 24 Sep 2018 17:52

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.3	31.3	46.9
170	24.3	21.0	31.6


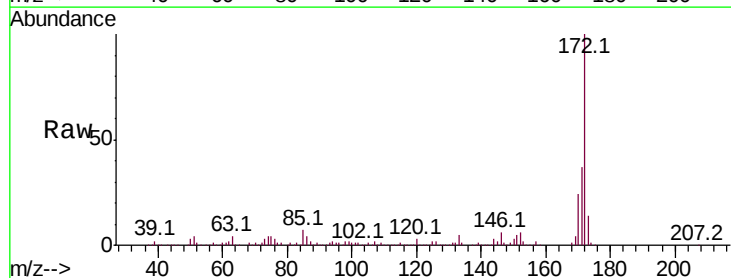



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E



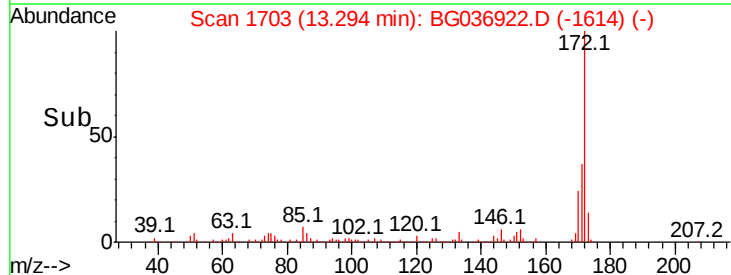
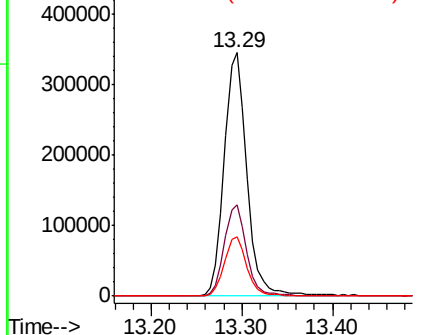


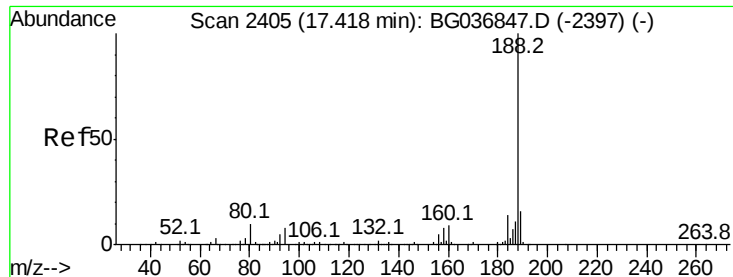

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.41 min Scan# 2404
Delta R.T. -0.01 min
Lab File: BG036922.D
Acq: 24 Sep 2018 17:52




Instrument :
BNA_G
ClientSampleId :
JC-02-092118-A


Tot Ion:188 Resp: 300438
Ion Ratio Lower Upper
188 100
94 7.9 6.7 10.1
80 9.6 8.1 12.1

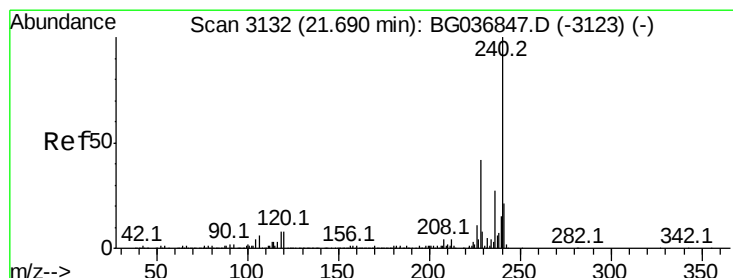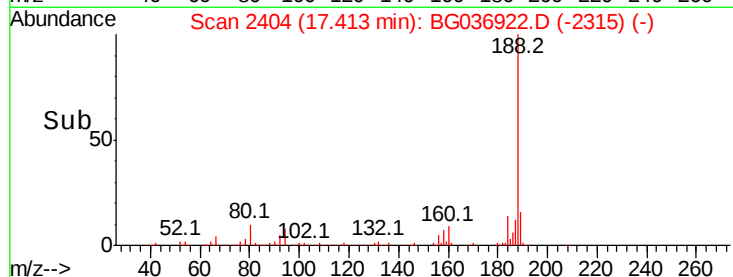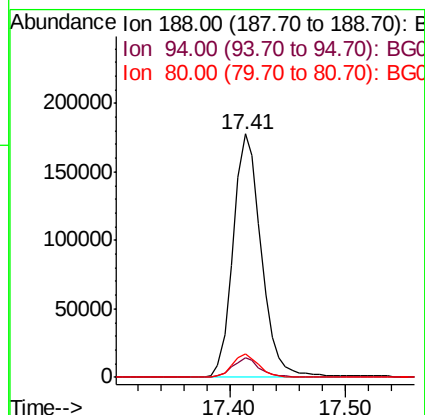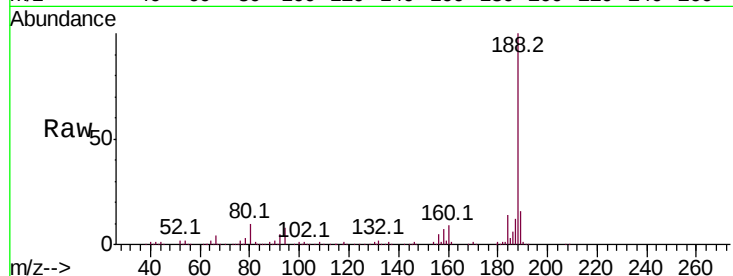

#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.68 min Scan# 3130
Delta R.T. -0.01 min
Lab File: BG036922.D
Acq: 24 Sep 2018 17:52

Tgt Ion:240 Resp: 318019
Ion Ratio Lower Upper
240 100
120 8.2 6.9 10.3
236 27.3 21.2 31.8

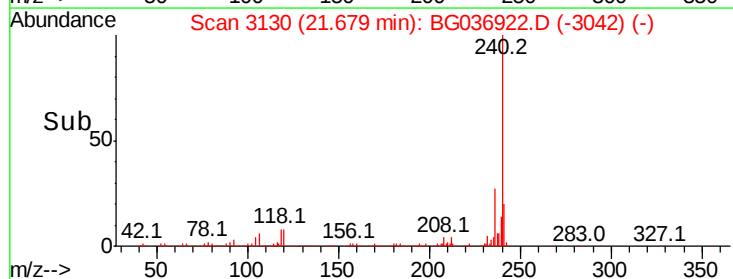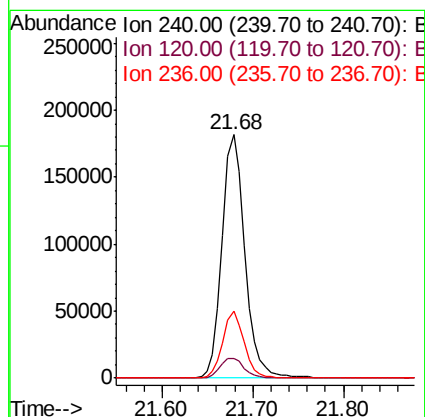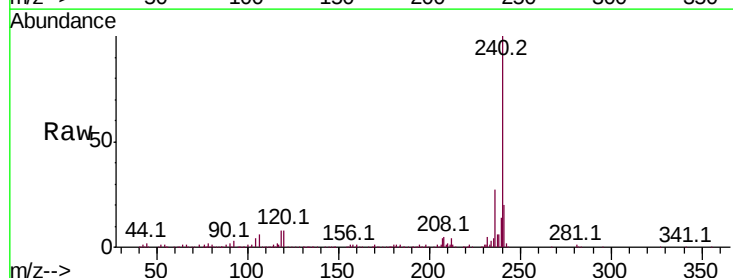

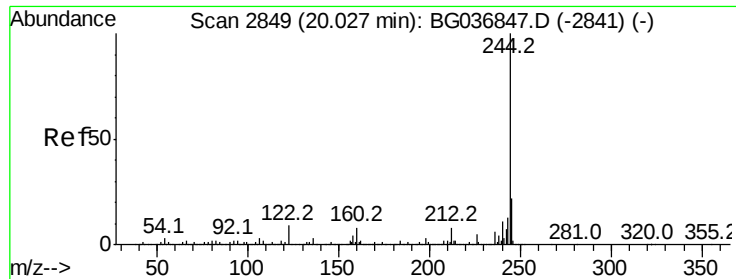

#78

Terphenyl-d14

Concen: 91.072 ng

RT: 20.02 min Scan# 2848

Delta R.T. -0.01 min

Lab File: BG036922.D

Acq: 24 Sep 2018 17:52

Instrument :

BNA_G

ClientSampleId :

JC-02-092118-A


Tot Ion:244 Resp: 1101451

Ion Ratio Lower Upper

244 100

212 8.7 7.0 10.6




122 9.1 7.1 10.7

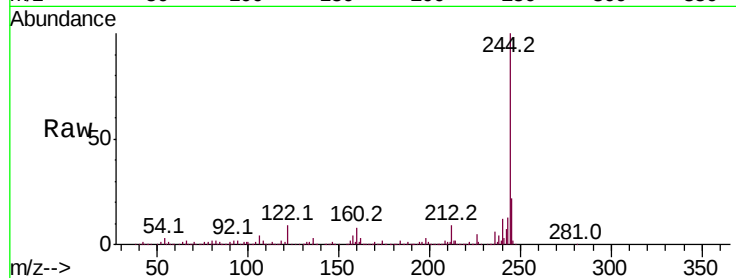

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

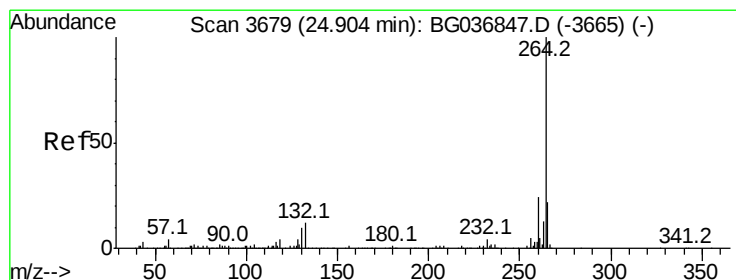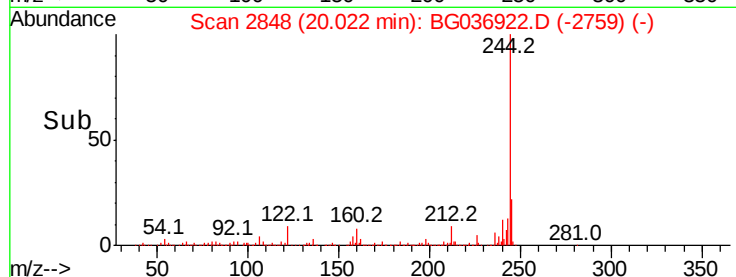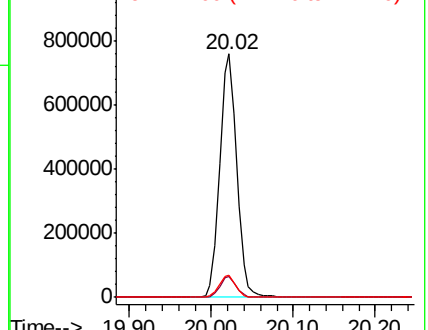

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.88 min Scan# 3675

Delta R.T. -0.02 min

Lab File: BG036922.D

Acq: 24 Sep 2018 17:52


Tgt Ion:264 Resp: 320369

Ion Ratio Lower Upper

264 100

260 23.7 19.6 29.4

265 20.7 17.4 26.0

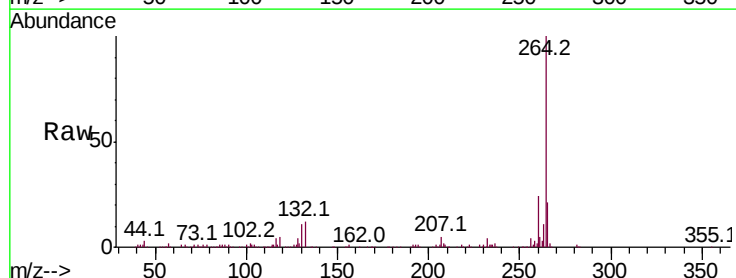

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

