

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG092418\
 Data File : BG036929.D
 Acq On : 24 Sep 2018 22:24
 Operator : JU/SJ
 Sample : J4770-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JC-02-092118-F

Quant Time: Sep 25 07:22:01 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 24 10:41:23 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	36234	20.00	ng	0.00
21) Naphthalene-d8	10.85	136	154350	20.00	ng	0.00
38) Acenaphthene-d10	14.67	164	103300	20.00	ng	0.00
63) Phenanthrene-d10	17.41	188	276912	20.00	ng	0.00
75) Chrysene-d12	21.68	240	296028	20.00	ng	-0.01
86) Perylene-d12	24.88	264	285456	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	238866	126.43	ng	0.00
7) Phenol-d6	7.20	99	298061	101.96	ng	-0.01
23) Nitrobenzene-d5	9.20	82	247003	85.70	ng	0.00
41) 2,4,6-Tribromophenol	16.15	330	147223	119.12	ng	-0.01
44) 2-Fluorobiphenyl	13.29	172	572684	82.57	ng	0.00
78) Terphenyl-d14	20.02	244	1073071	95.32	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG092418\
Data File : BG036929.D
Acq On : 24 Sep 2018 22:24
Operator : JU/SJ
Sample : J4770-12
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JC-02-092118-F

Quant Time: Sep 25 07:22:01 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 24 10:41:23 2018
Response via : Initial Calibration

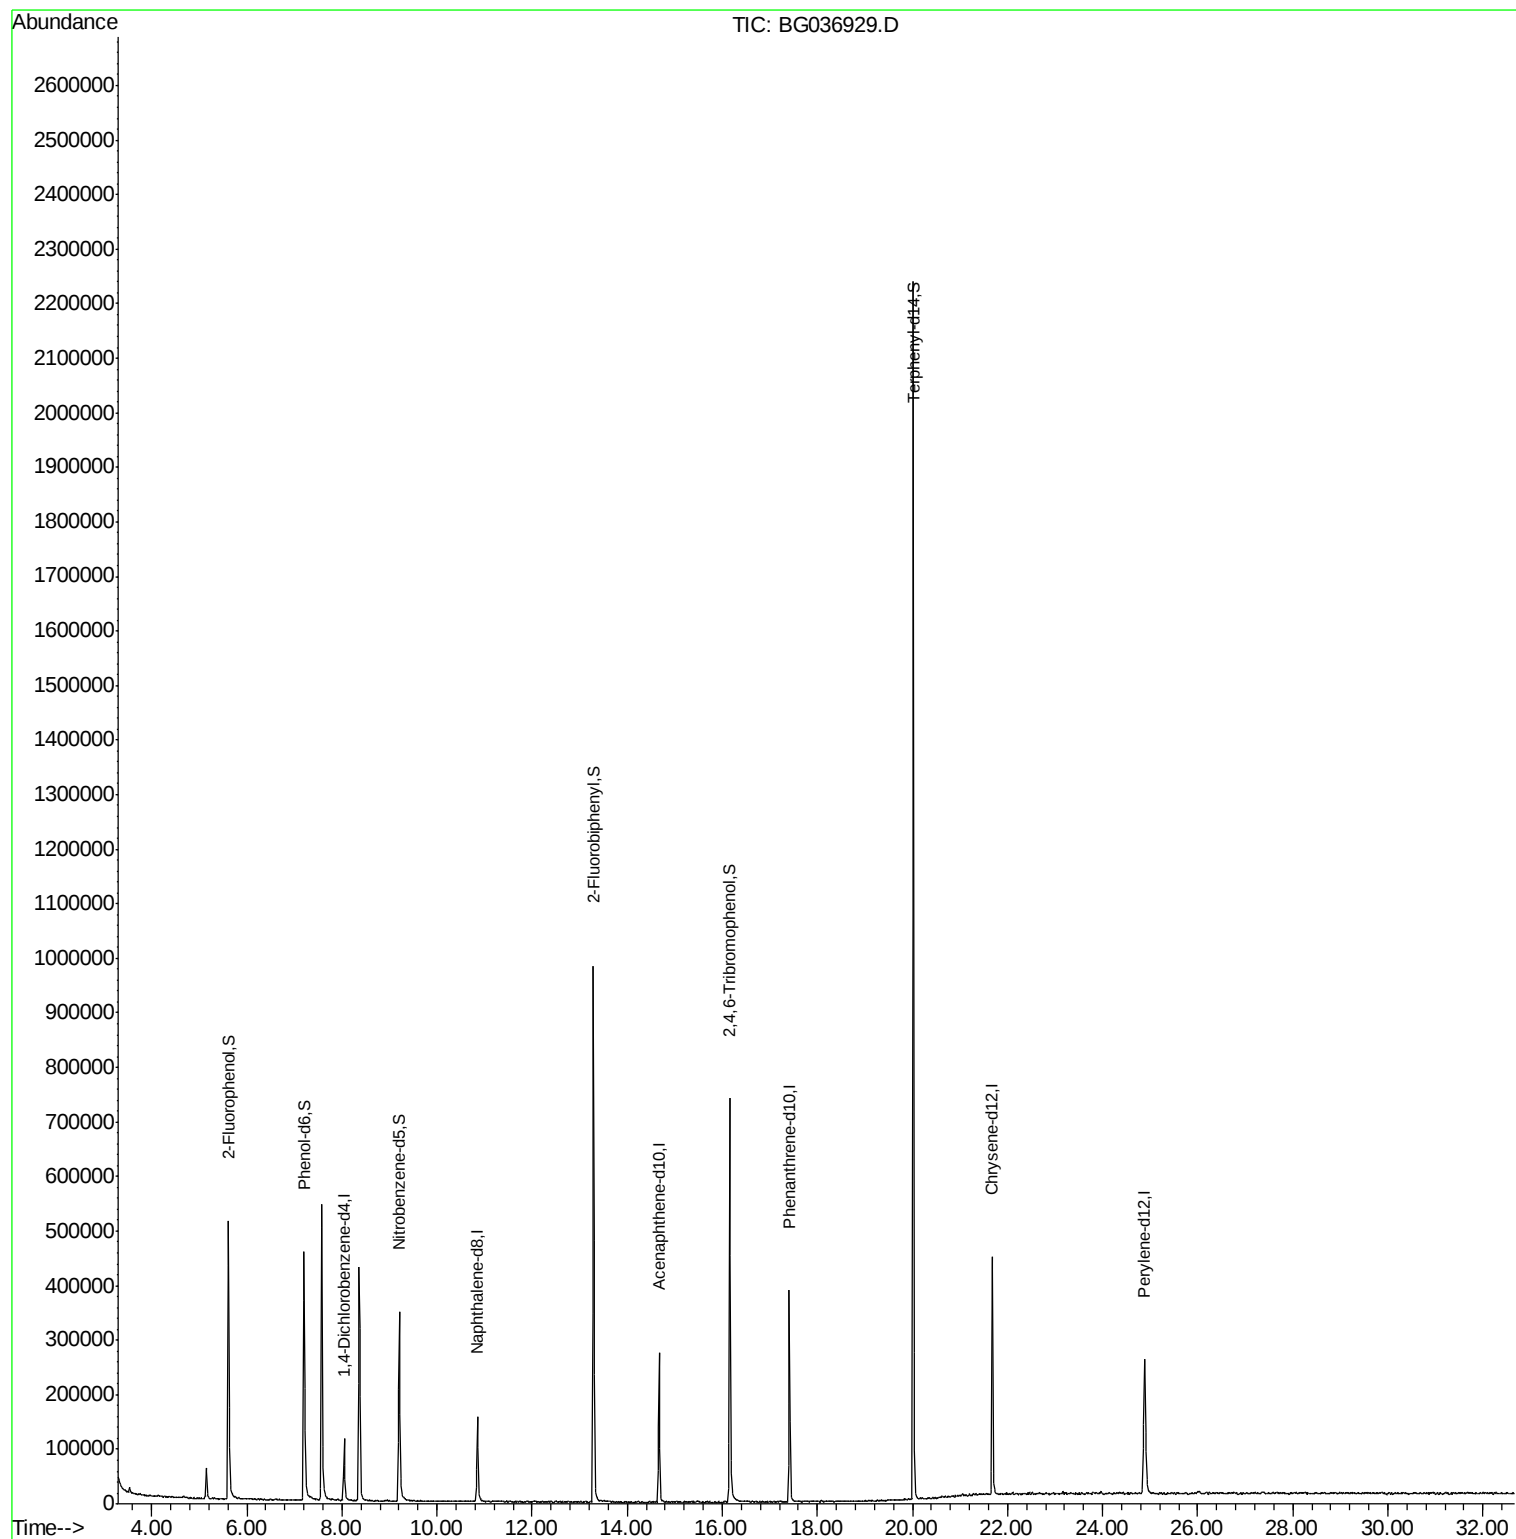

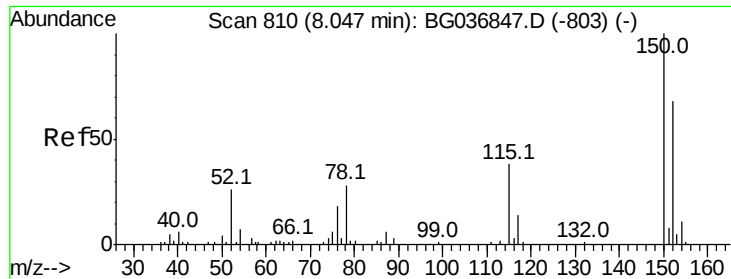


#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.05 min Scan# 810
 Delta R.T. -0.00 min
 Lab File: BG036929.D
 Acq: 24 Sep 2018 22:24

Instrument :
 BNA_G
 ClientSampleId :
 JC-02-092118-F

Tot Ion	Ratio	Lower	Upper
152	100		
150	141.7	119.5	179.3
115	60.9	44.5	66.7

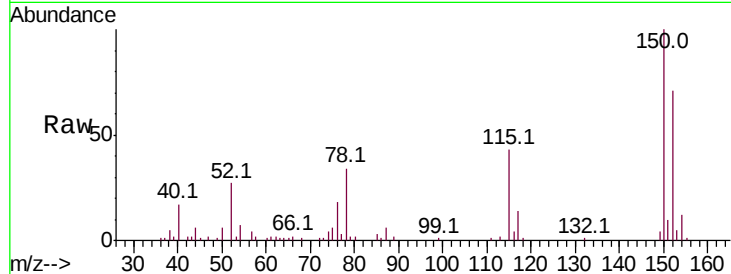


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

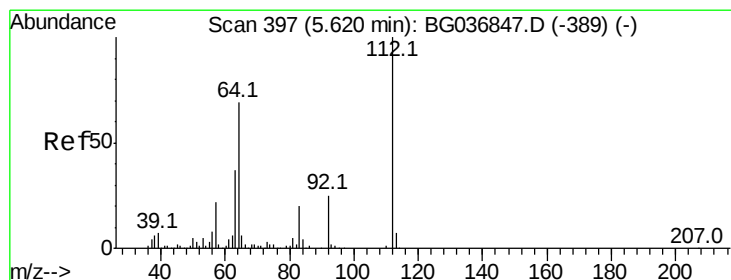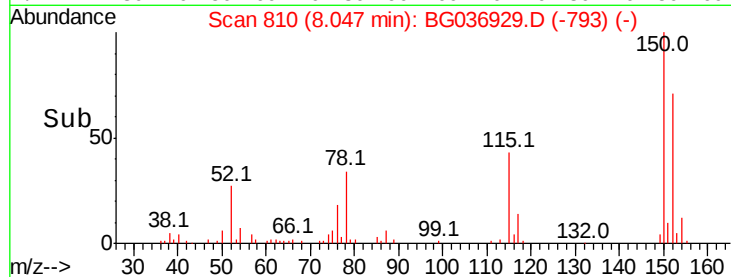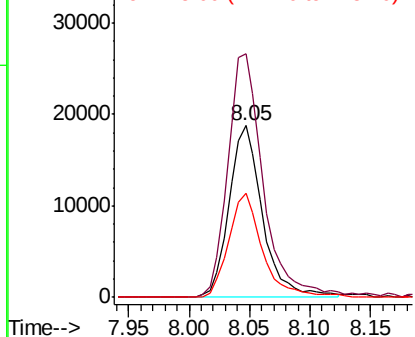



#5

2-Fluorophenol
 Concen: 126.426 ng
 RT: 5.61 min Scan# 396
 Delta R.T. -0.01 min
 Lab File: BG036929.D
 Acq: 24 Sep 2018 22:24

Tgt Ion	Ratio	Lower	Upper
112	100		
64	71.4	57.2	85.8
63	38.5	30.8	46.2

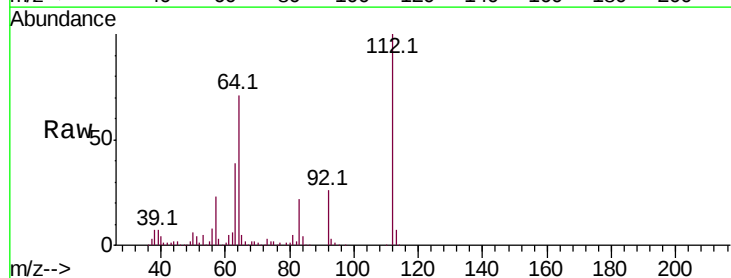

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BG
 Ion 63.00 (62.70 to 63.70): BG

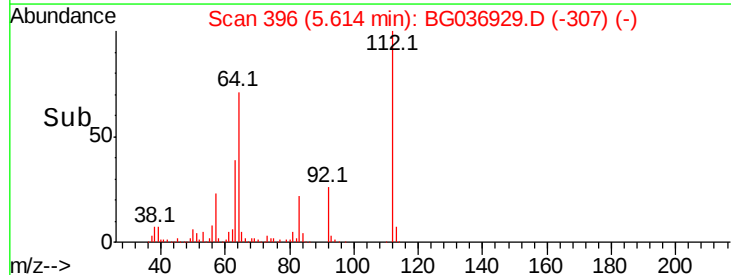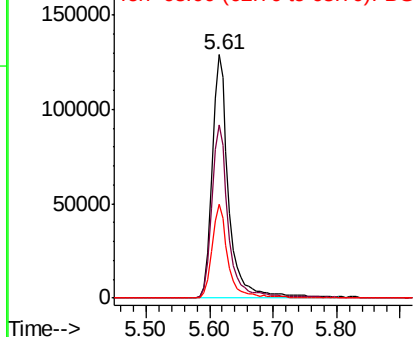



#7

Phenol-d6

Concen: 101.965 ng

RT: 7.20 min Scan# 666

Delta R.T. -0.01 min

Lab File: BG036929.D

Acq: 24 Sep 2018 22:24

Instrument :

BNA_G

ClientSampleId :

JC-02-092118-F


Tot Ion: 99 Resp: 298061

Ion Ratio Lower Upper



99 100

42 22.3 16.5 24.7

71 37.3 29.4 44.2

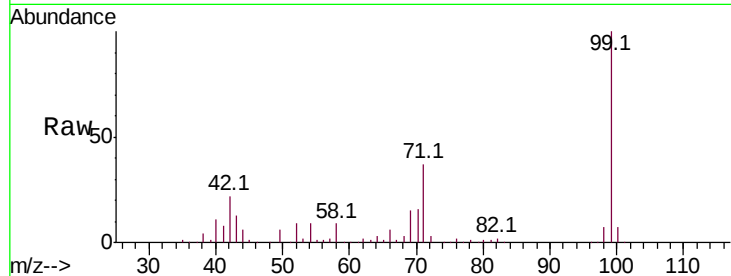

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

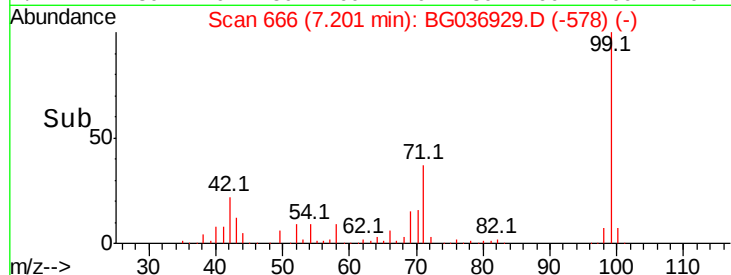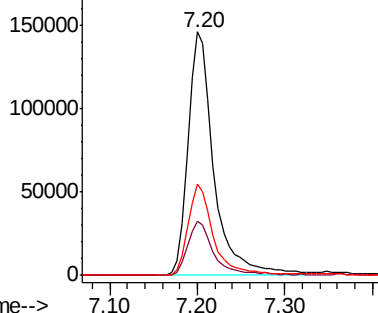

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.85 min Scan# 1287

Delta R.T. -0.01 min

Lab File: BG036929.D

Acq: 24 Sep 2018 22:24

Tgt Ion: 136 Resp: 154350


Ion Ratio Lower Upper

136 100



137 11.2 8.8 13.2


54 11.7 9.2 13.8

68 6.4 5.8 8.6

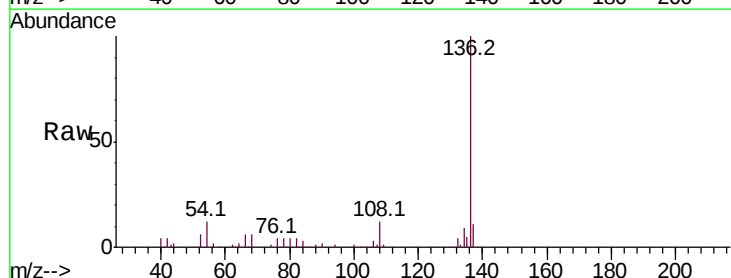

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



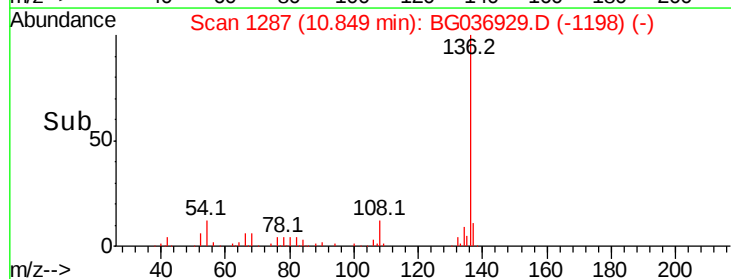
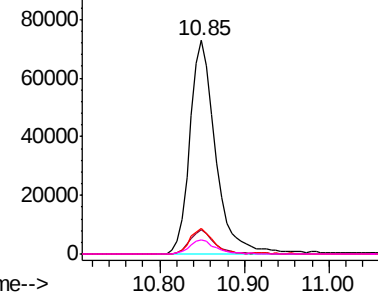


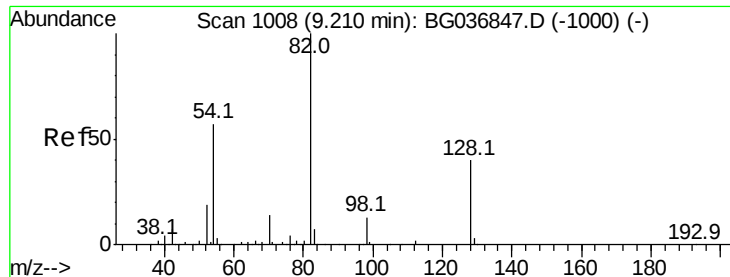

#23
Nitrobenzene-d5
Concen: 85.697 ng
RT: 9.20 min Scan# 1007
Delta R.T. -0.01 min
Lab File: BG036929.D
Acq: 24 Sep 2018 22:24




Instrument :
BNA_G
ClientSampleId :
JC-02-092118-F


Tot Ion	82	Resp	247003
Ion Ratio	Lower	Upper	
82	100		
128	38.8	33.3	49.9
54	56.2	45.1	67.7

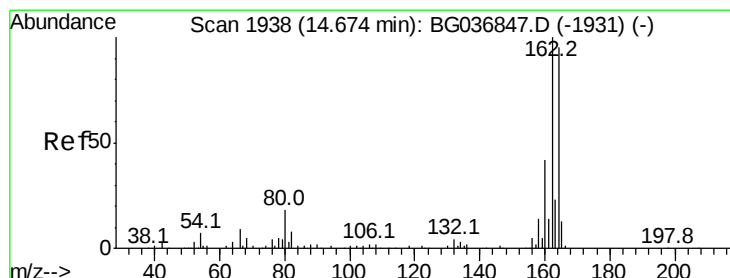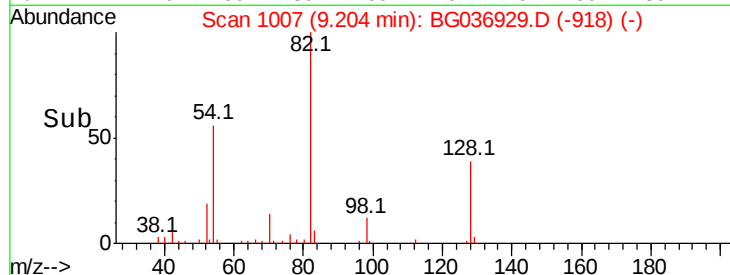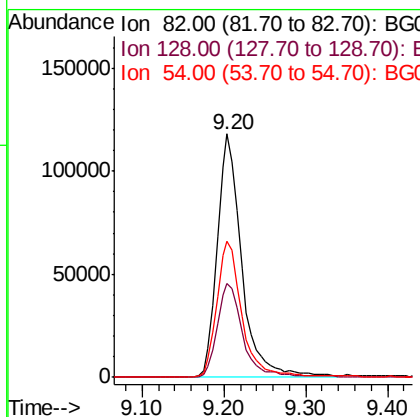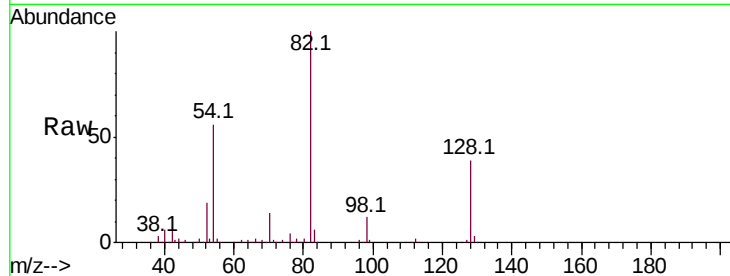

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.67 min Scan# 1937
Delta R.T. -0.01 min
Lab File: BG036929.D
Acq: 24 Sep 2018 22:24

Tgt Ion	164	Resp	103300
Ion Ratio	Lower	Upper	
164	100		
162	102.5	80.7	121.1
160	45.1	35.3	52.9

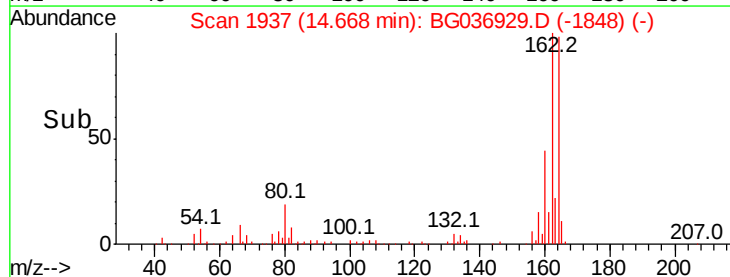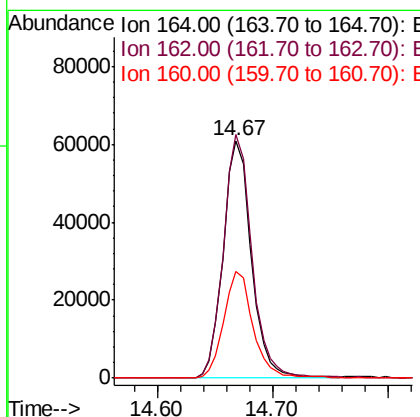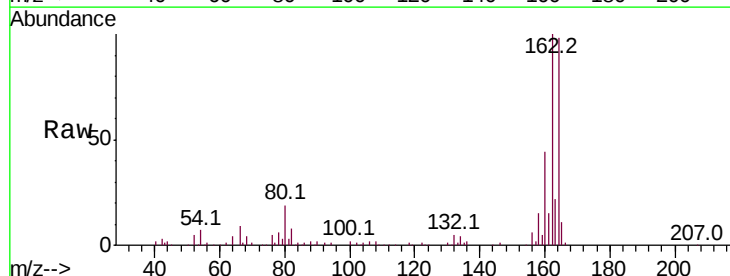


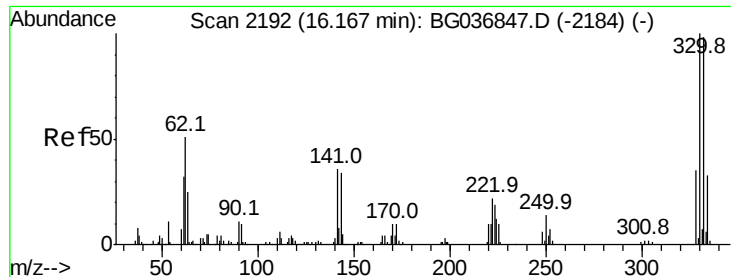



#41
 2,4,6-Tribromophenol
 Concen: 119.120 ng
 RT: 16.15 min Scan# 2190
 Delta R.T. -0.01 min
 Lab File: BG036929.D
 Acq: 24 Sep 2018 22:24

Instrument :
 BNA_G
 ClientSampleId :
 JC-02-092118-F

Tot Ion	Ratio	Lower	Upper
330	100		
332	94.3	75.4	113.2
141	38.9	30.7	46.1

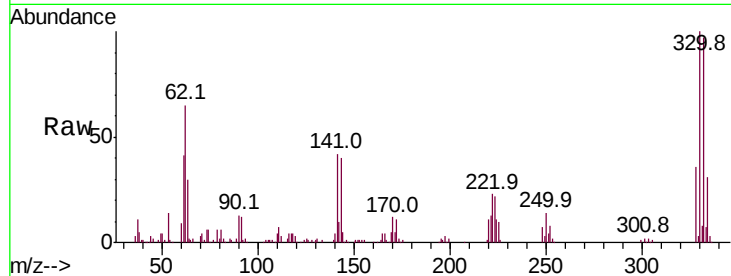


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

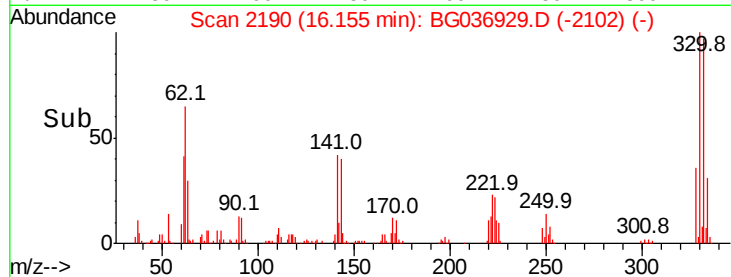
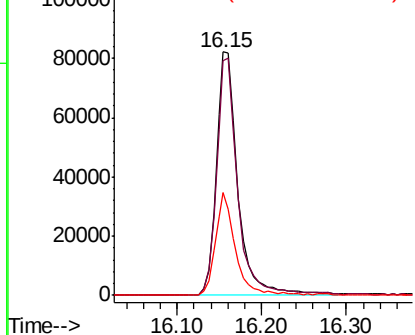



#44
 2-Fluorobiphenyl
 Concen: 82.570 ng
 RT: 13.29 min Scan# 1703
 Delta R.T. -0.01 min
 Lab File: BG036929.D
 Acq: 24 Sep 2018 22:24

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.6	31.3	46.9
170	25.0	21.0	31.6

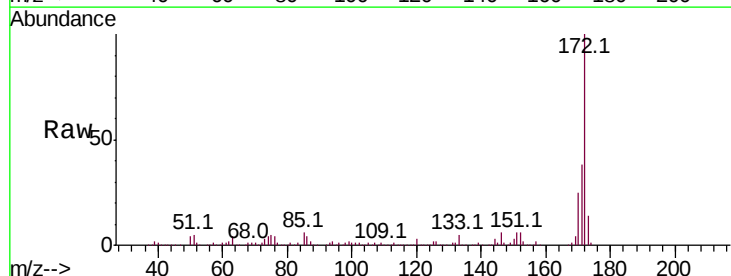

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



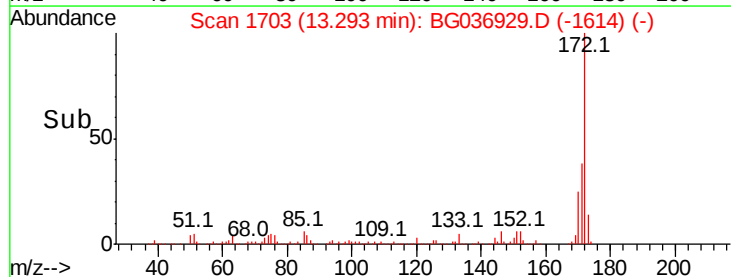
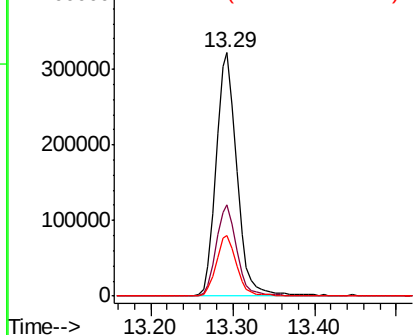


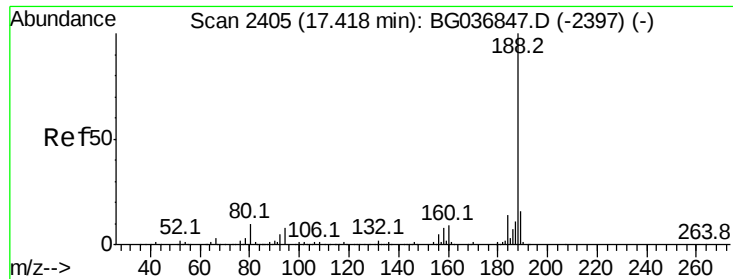

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.41 min Scan# 2404
Delta R.T. -0.01 min
Lab File: BG036929.D
Acq: 24 Sep 2018 22:24




Instrument :
BNA_G
ClientSampleId :
JC-02-092118-F

Tot Ion:188 Resp: 276912
Ion Ratio Lower Upper
188 100
94 7.6 6.7 10.1
80 9.0 8.1 12.1

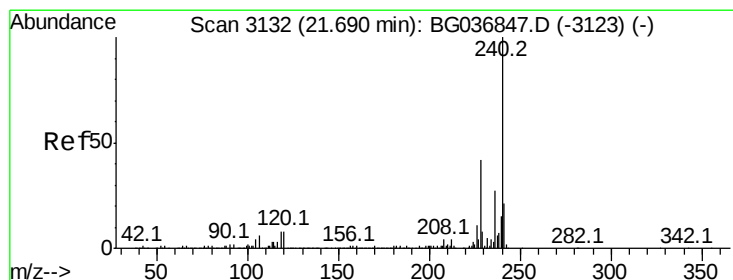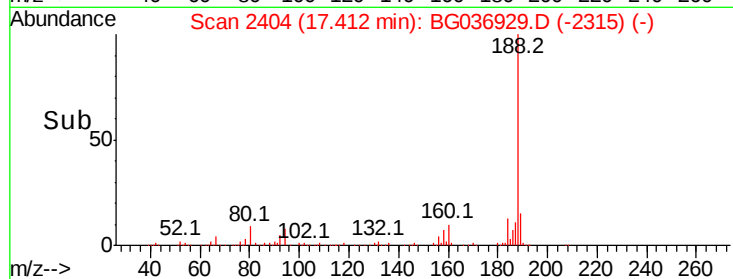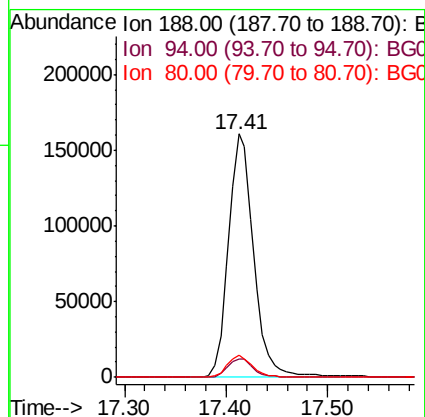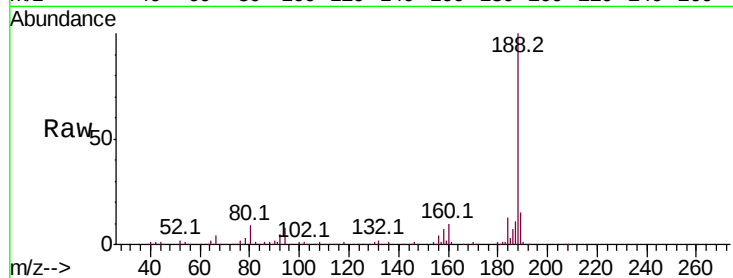

#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.68 min Scan# 3130
Delta R.T. -0.01 min
Lab File: BG036929.D
Acq: 24 Sep 2018 22:24

Tgt Ion:240 Resp: 296028
Ion Ratio Lower Upper
240 100
120 7.9 6.9 10.3
236 26.6 21.2 31.8


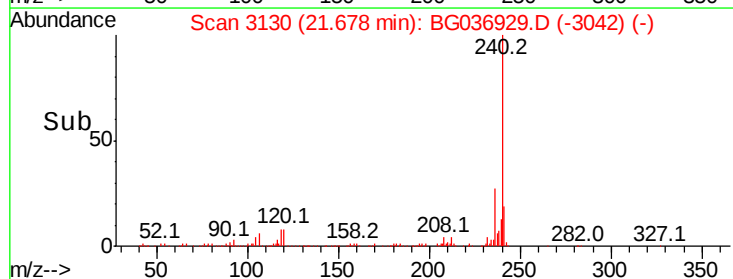
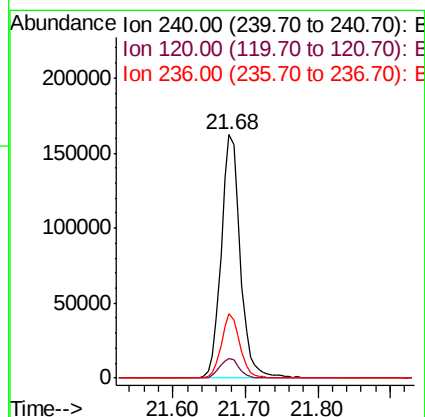
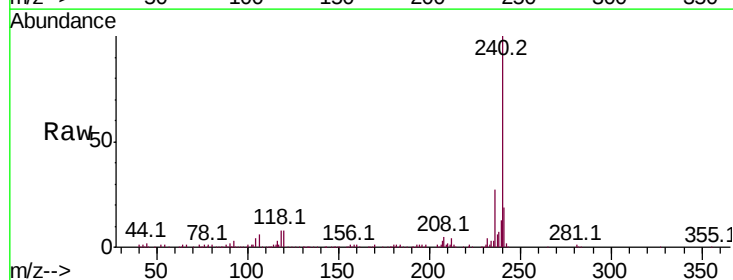




#78
 Terphenyl-d14
 Concen: 95.316 ng
 RT: 20.02 min Scan# 2848
 Delta R.T. -0.01 min
 Lab File: BG036929.D
 Acq: 24 Sep 2018 22:24

Instrument :
 BNA_G
 ClientSampleId :
 JC-02-092118-F

Tot Ion:244 Resp: 1073071
 Ion Ratio Lower Upper
 244 100
 212 8.4 7.0 10.6
 122 8.9 7.1 10.7

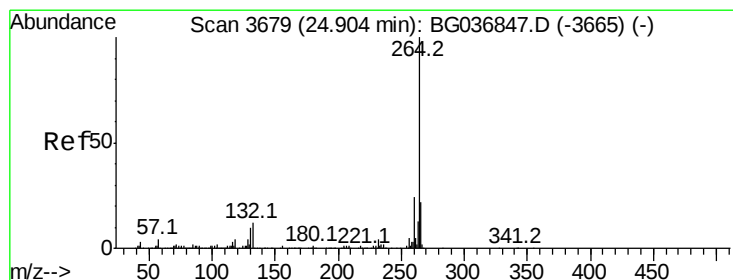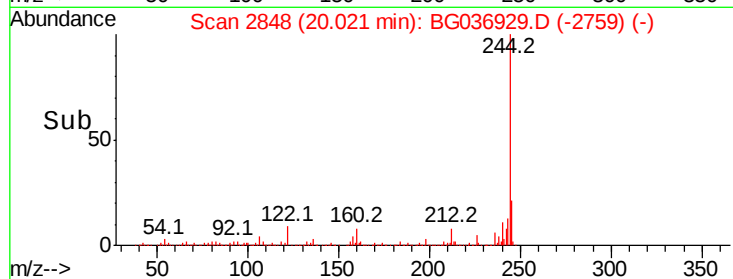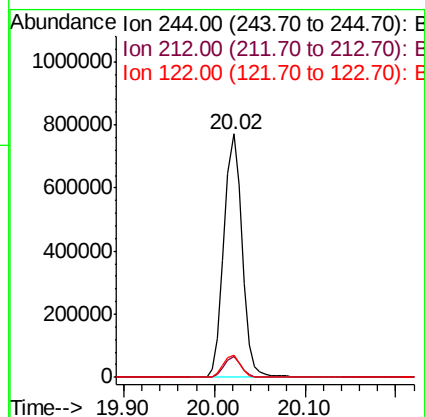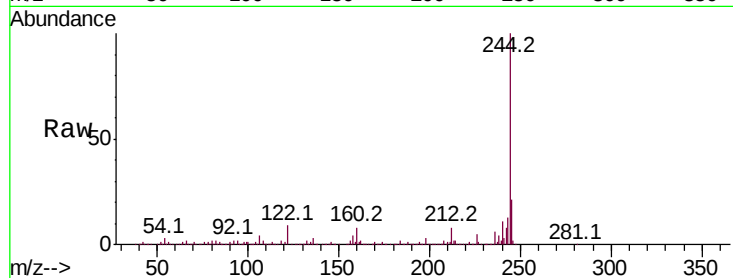

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.88 min Scan# 3675
 Delta R.T. -0.02 min
 Lab File: BG036929.D
 Acq: 24 Sep 2018 22:24

Tgt Ion:264 Resp: 285456
 Ion Ratio Lower Upper
 264 100
 260 21.7 19.6 29.4
 265 21.6 17.4 26.0

