

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG092515\
 Data File : BG018899.D
 Acq On : 26 Sep 2015 4:24
 Operator : UM/NP
 Sample : PB85776BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK76

Quant Time: Sep 26 06:48:16 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG091015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 26 04:18:39 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.99	152	45555	20.00	ng/ul	0.00
18) Naphthalene-d8	10.79	136	185816	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.61	164	123367	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.35	188	349713	20.00	ng/ul	0.00
78) Chrysene-d12	21.60	240	417490	20.00	ng/ul	0.00
86) Perylene-d12	24.78	264	420112	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.43	96	4738	5.00	ng/uL	0.00
5) Phenol-d5	7.15	99	95909	25.64	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.32	67	58981	27.21	ng/ul	0.00
9) 2-Chlorophenol-d4	7.52	132	81041	28.60	ng/ul	0.00
13) 4-Methylphenol-d8	8.69	113	80554	26.54	ng/ul	0.00
19) Nitrobenzene-d5	9.15	128	41325	29.35	ng/ul	0.00
22) 2-Nitrophenol-d4	9.87	143	48494	34.26	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.41	165	81623	27.38	ng/ul	0.00
29) 4-Chloroaniline-d4	10.92	131	125575	36.21	ng/ul	0.00
44) Dimethylphthalate-d6	14.01	166	342164	34.46	ng/ul	0.00
47) Acenaphthylene-d8	14.31	160	350261	29.77	ng/ul	0.00
52) 4-Nitrophenol-d4	14.81	143	54633	28.67	ng/ul	0.00
58) Fluorene-d10	15.60	176	271045	31.22	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.72	200	15494	9.36	ng/ul	0.00
71) Anthracene-d10	17.45	188	483163	31.38	ng/ul	0.00
79) Pyrene-d10	19.74	212	609831	31.75	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.56	264	654521	32.01	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
46) 2,6-Dinitrotoluene	14.02	165	2056	1.06	ng/ul#	37


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG092515\
Data File : BG018899.D
Acq On : 26 Sep 2015 4:24
Operator : UM/NP
Sample : PB85776BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK76

Quant Time: Sep 26 06:48:16 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG091015.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 26 04:18:39 2015
Response via : Initial Calibration

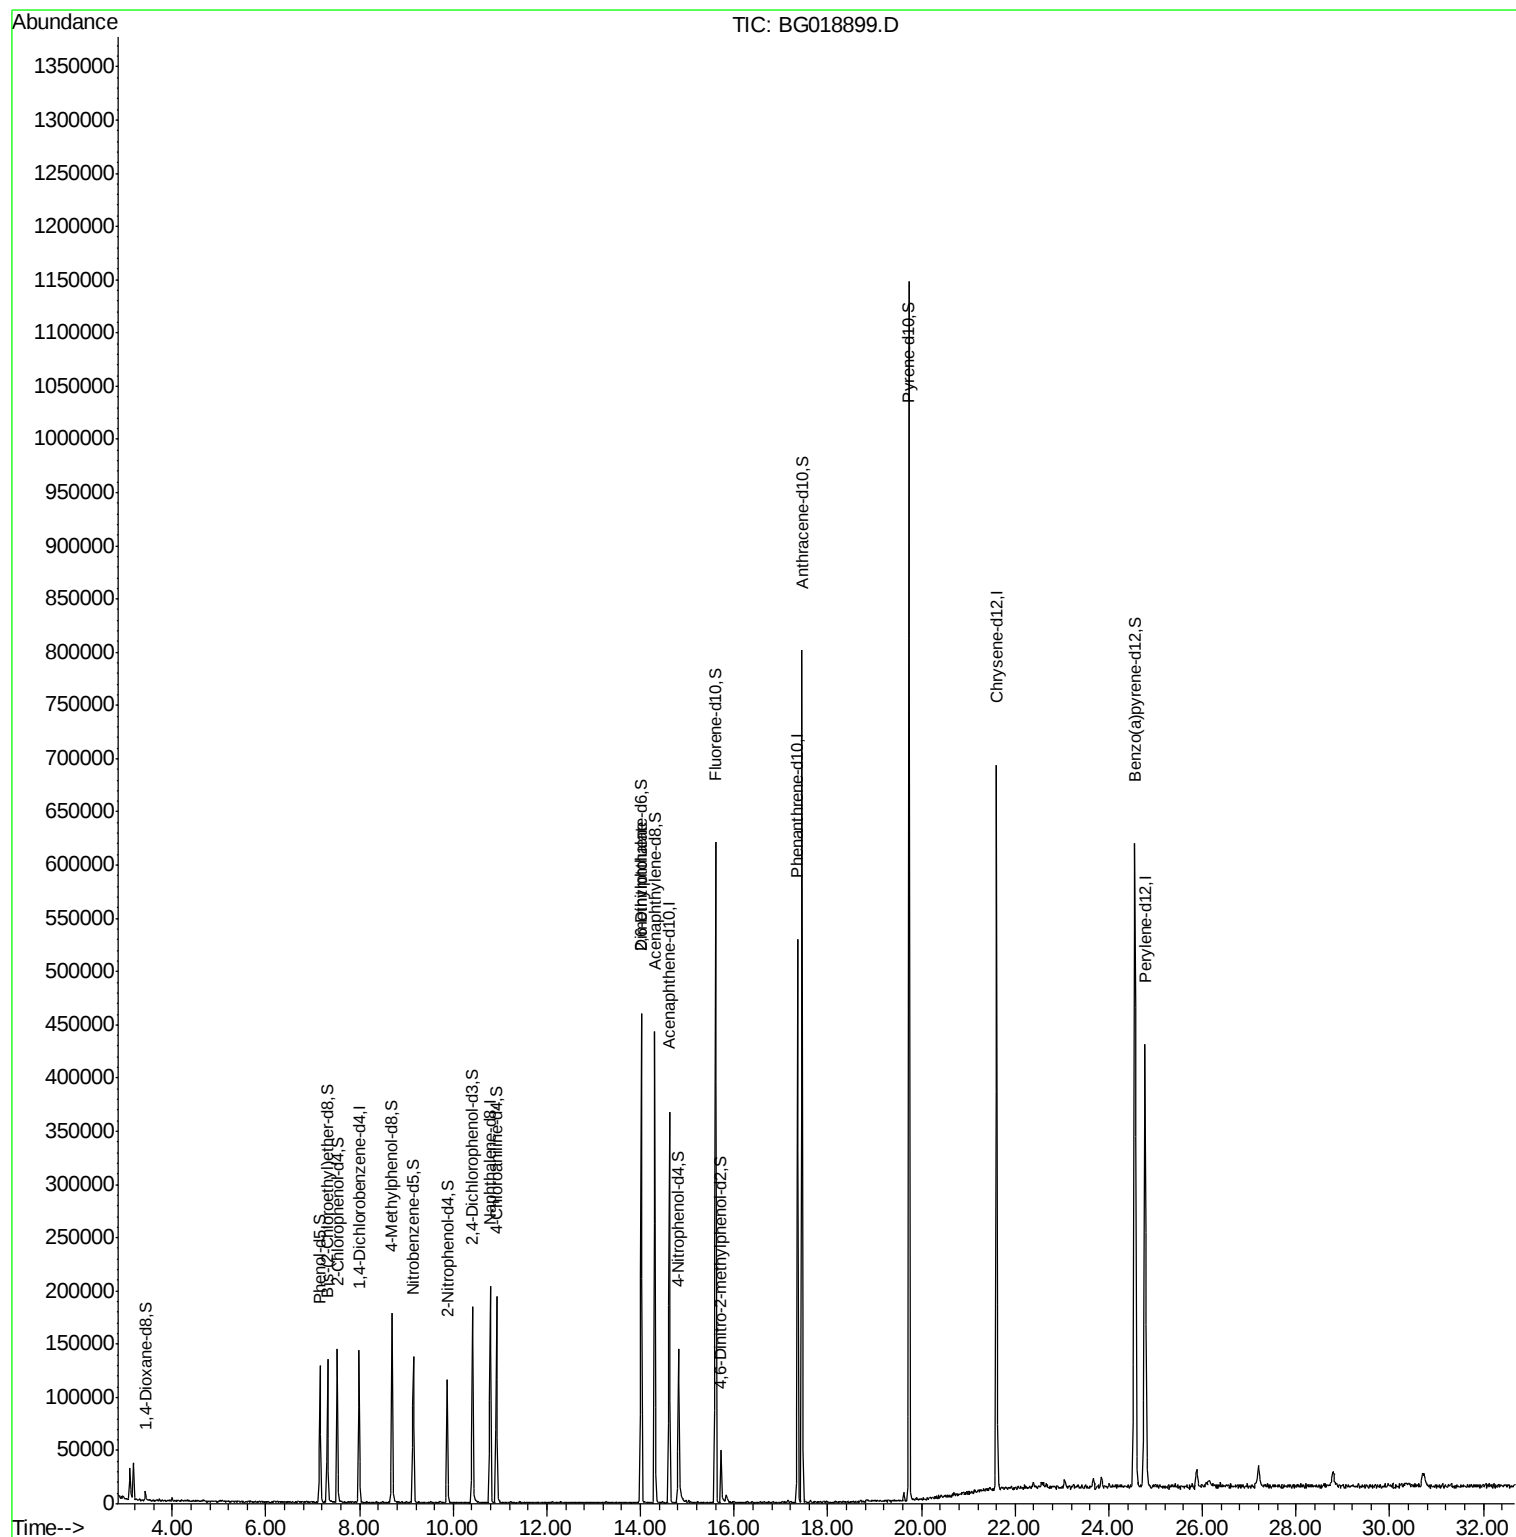

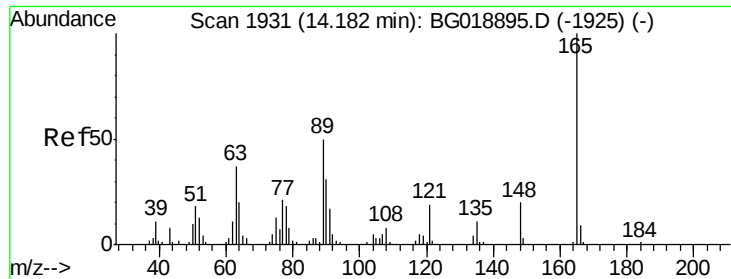

#46
 2,6-Dinitrotoluene
 Concen: 1.06 ng/ul
 RT: 14.02 min Scan# 1903
 Delta R.T. -0.16 min
 Lab File: BG018899.D
 Acq: 26 Sep 2015 4:24

Instrument :
 BNA_G
 ClientSampleId :
 SBLK76

Tgt Ion	Ratio	Lower	Upper
165	100		
89	0.0	50.2	75.2#
121	16.2	19.4	29.2#

