

Data Path : Z:\HPCHEM1\BNA G\DATA\BG092515\
 Data File : BG018916.D
 Acq On : 26 Sep 2015 17:10
 Operator : UM/NP
 Sample : G3800-13
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C03H2

Quant Time: Sep 28 00:54:05 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG091015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 28 00:51:47 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.99	152	48062	20.00	ng/ul	0.00
18) Naphthalene-d8	10.79	136	205990	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.61	164	139416	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.36	188	377835	20.00	ng/ul	0.00
78) Chrysene-d12	21.61	240	436167	20.00	ng/ul	0.00
86) Perylene-d12	24.78	264	444750	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.43	96	1429	1.43	ng/uL	0.00
5) Phenol-d5	7.16	99	30702	7.78	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.32	67	71327	31.19	ng/ul	0.00
9) 2-Chlorophenol-d4	7.53	132	84725	28.34	ng/ul	0.00
13) 4-Methylphenol-d8	8.70	113	58186	18.17	ng/ul	0.00
19) Nitrobenzene-d5	9.15	128	51757	33.16	ng/ul	0.00
22) 2-Nitrophenol-d4	9.87	143	58384	37.20	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.41	165	108228	32.75	ng/ul	0.00
29) 4-Chloroaniline-d4	10.92	131	115647	30.08	ng/ul	0.00
44) Dimethylphthalate-d6	14.01	166	379971	33.87	ng/ul	0.00
47) Acenaphthylene-d8	14.31	160	349245	26.27	ng/ul	0.00
52) 4-Nitrophenol-d4	14.82	143	15489	7.19	ng/ul	0.00
58) Fluorene-d10	15.61	176	224905	22.92	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.72	200	46757	26.14	ng/ul	0.00
71) Anthracene-d10	17.45	188	199611	12.00	ng/ul	0.00
79) Pyrene-d10	19.74	212	379585	18.92	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.56	264	359131	16.59	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	14.06	163	27119	2.49 ng/ul#	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG092515\
Data File : BG018916.D
Acq On : 26 Sep 2015 17:10
Operator : UM/NP
Sample : G3800-13
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C03H2

Quant Time: Sep 28 00:54:05 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG091015.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 28 00:51:47 2015
Response via : Initial Calibration

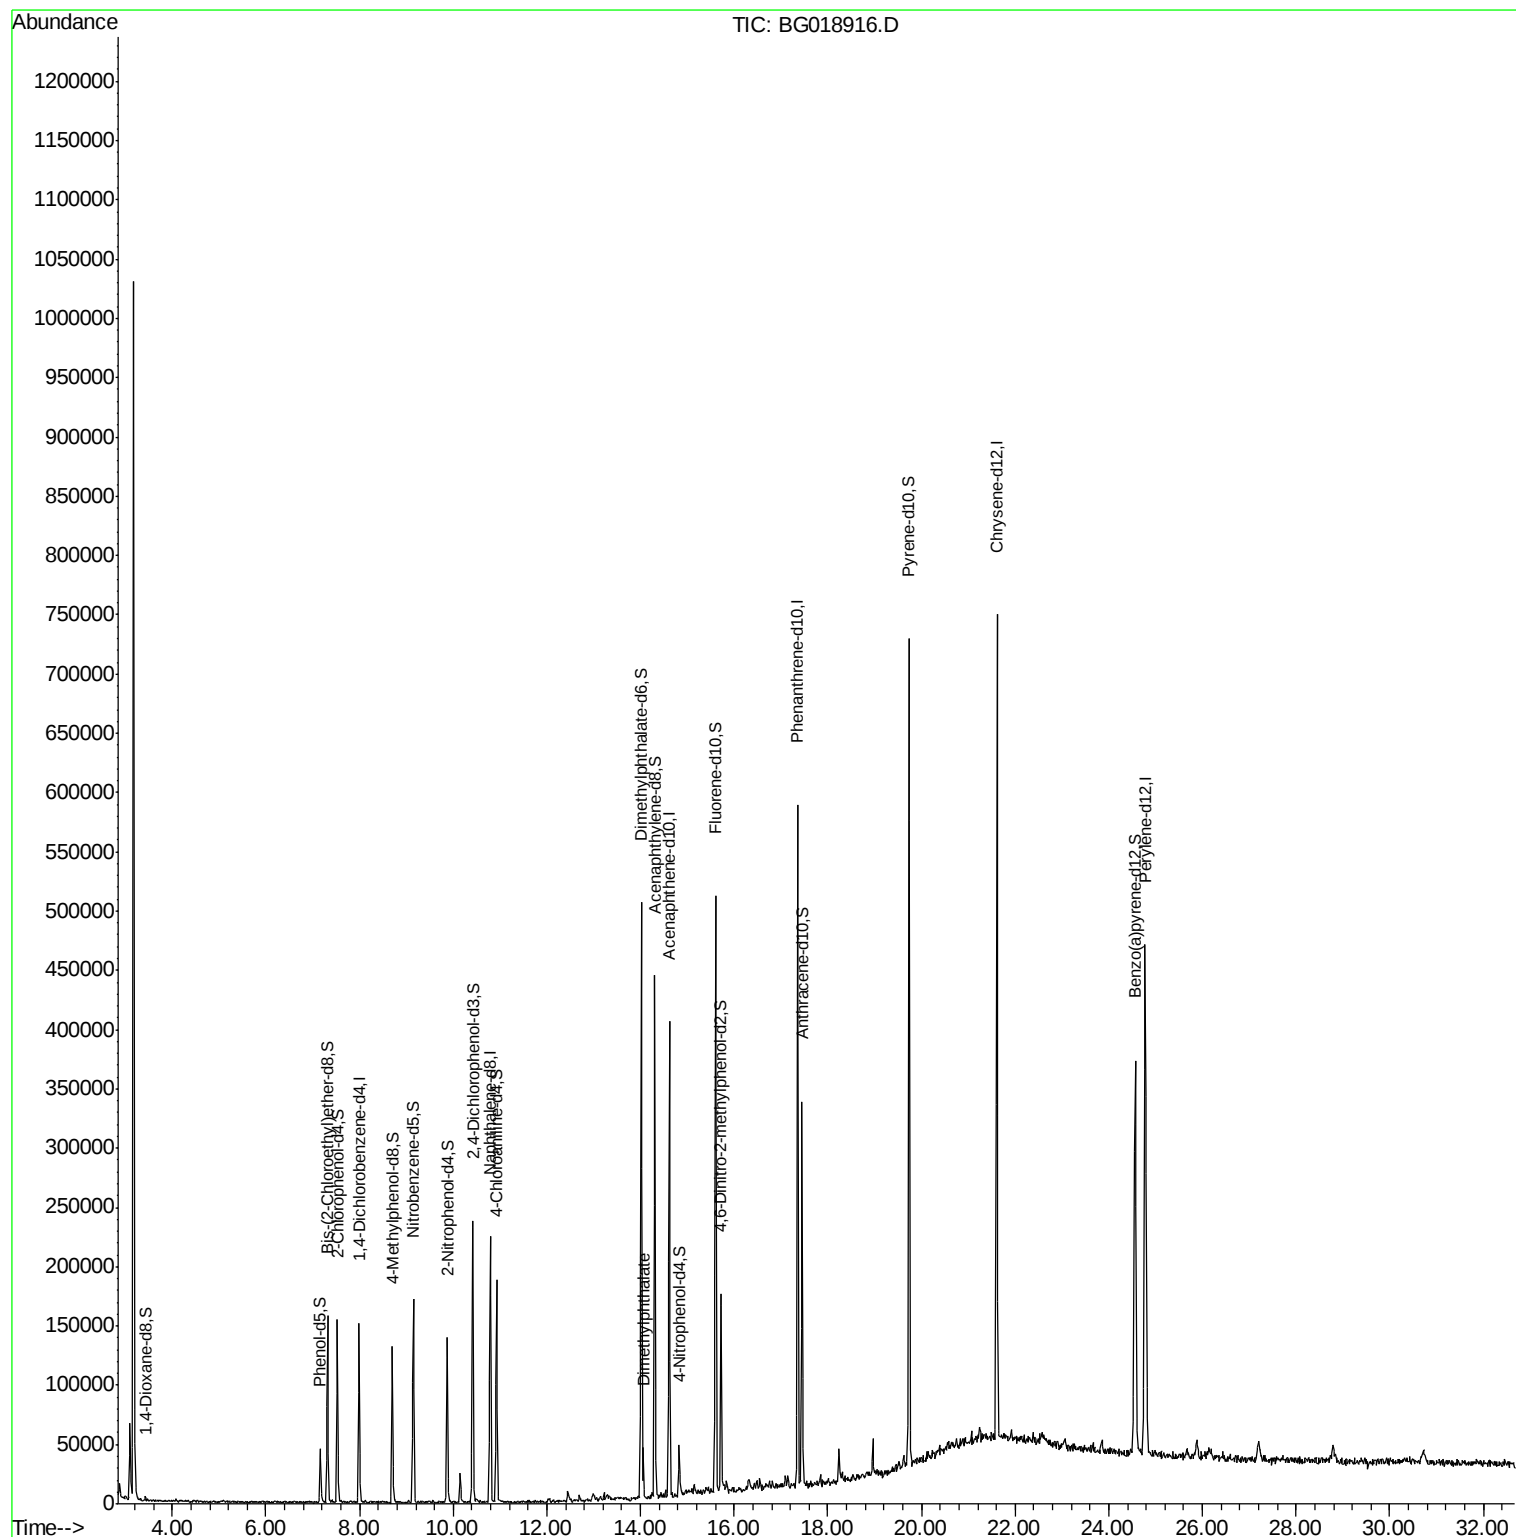

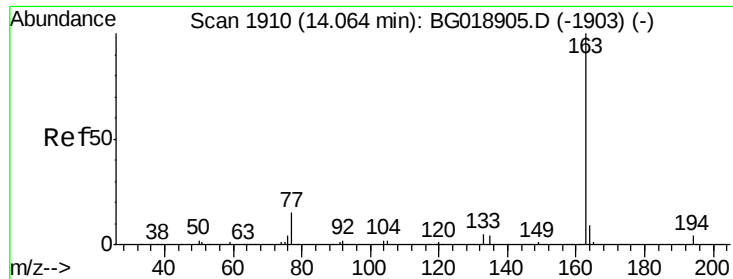

#45

Dimethylphthalate

Concen: 2.49 ng/ul

RT: 14.06 min Scan# 1910

Delta R.T. -0.00 min

Lab File: BG018916.D

Acq: 26 Sep 2015 17:10

Instrument :

BNA_G

ClientSampleId :

C03H2


Tot Ion:163 Resp: 27119

Ion Ratio Lower Upper

163 100

194 5.1 2.9 4.3#

164 12.1 7.7 11.5#

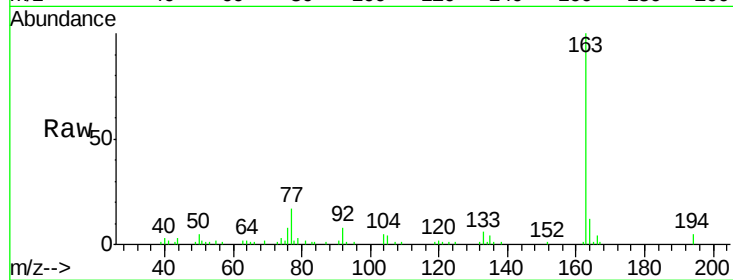

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

